




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012128.D
 Acq On : 14 Oct 2022 09:32
 Operator : CG/JU
 Sample : PB148234BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK234

Manual IntegrationsAPPROVED

Quant Time: Oct 14 23:01:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/15/2022
 Supervised By :mohammad ahmed 10/16/2022

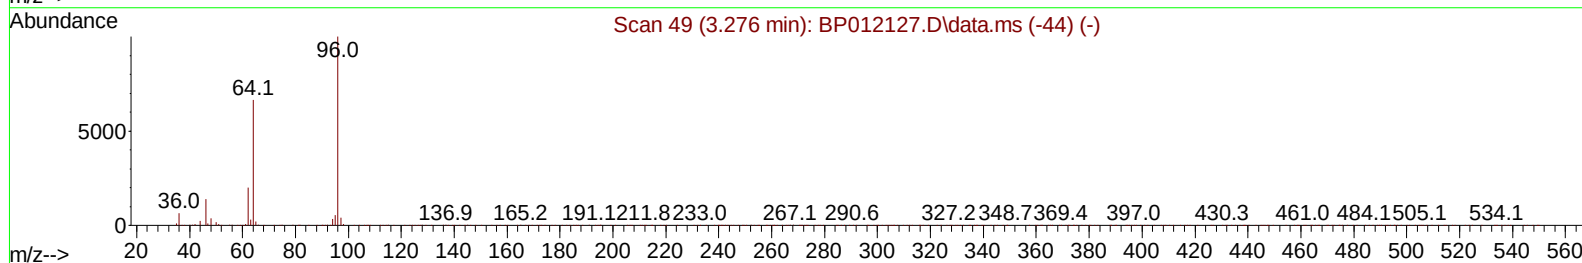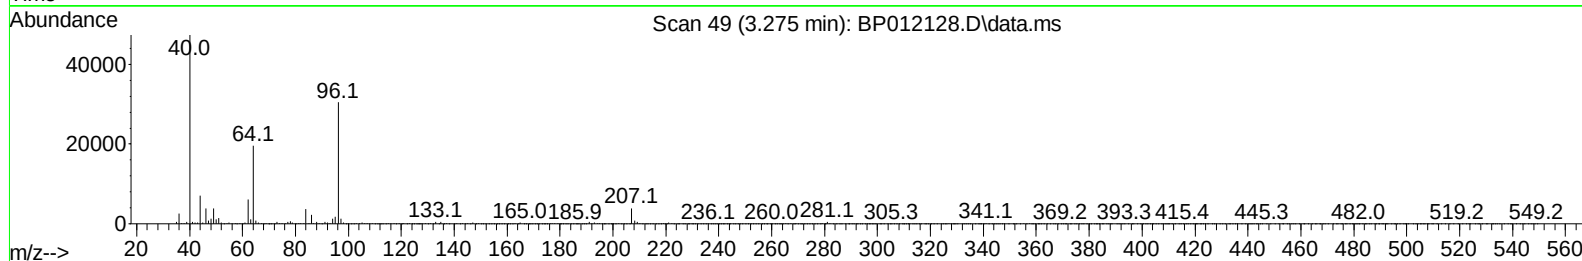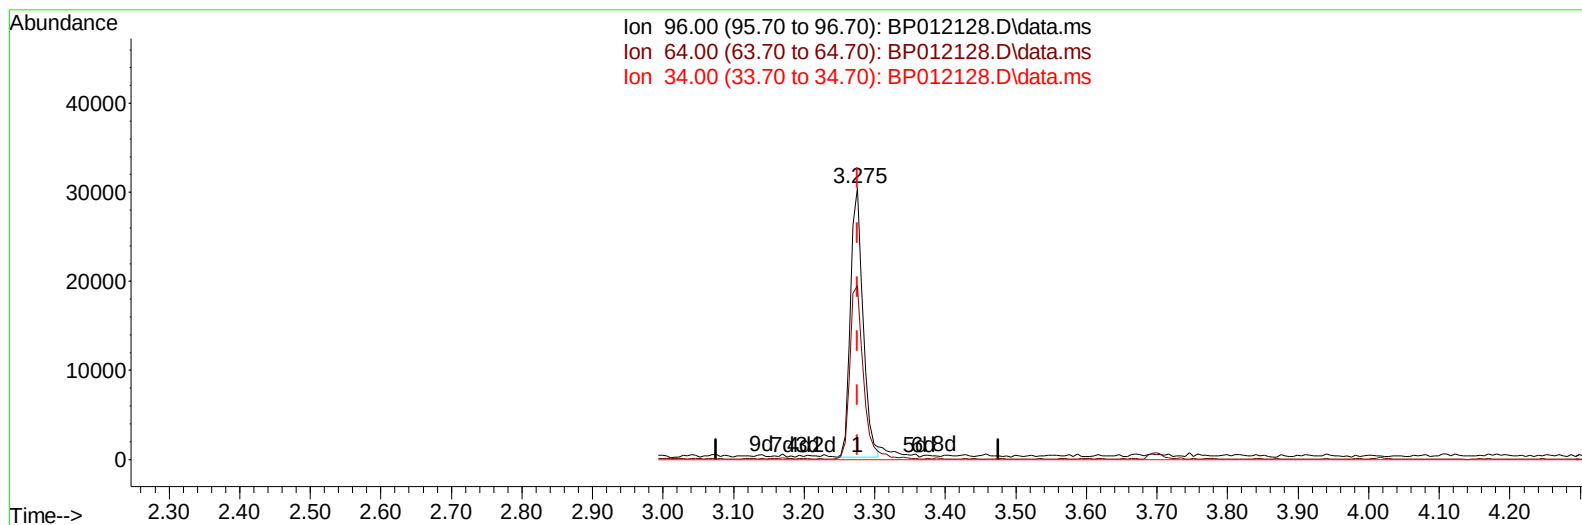

TIC: BP012128.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.275min (-0.000) 4.73 ng/uL

response 37619

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	64.01
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012128.D
 Acq On : 14 Oct 2022 09:32
 Operator : CG/JU
 Sample : PB148234BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK234

Manual IntegrationsAPPROVED

Quant Time: Oct 14 23:01:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/15/2022
 Supervised By :mohammad ahmed 10/16/2022

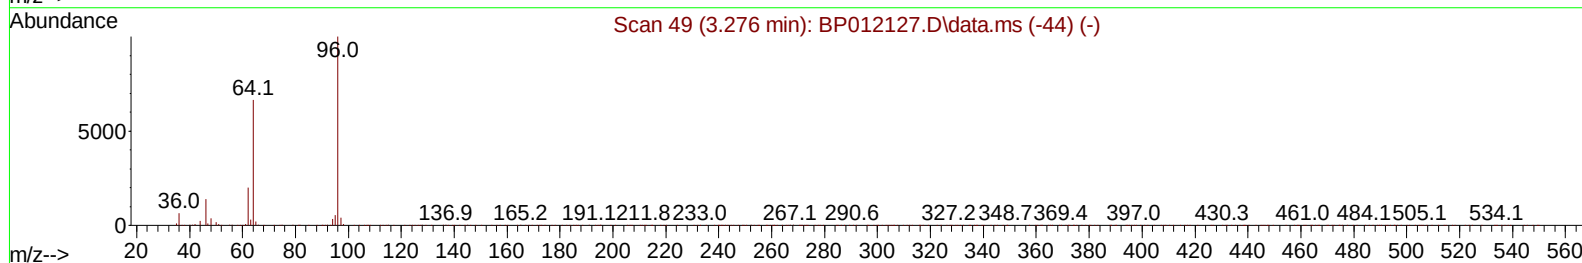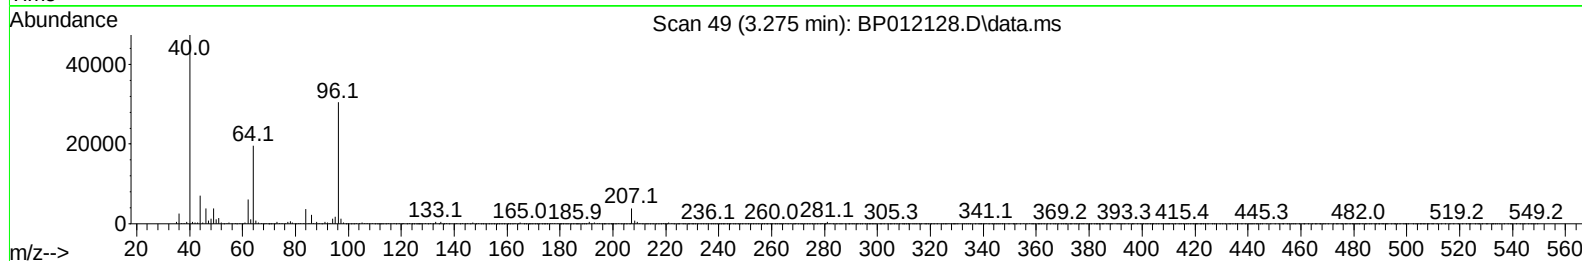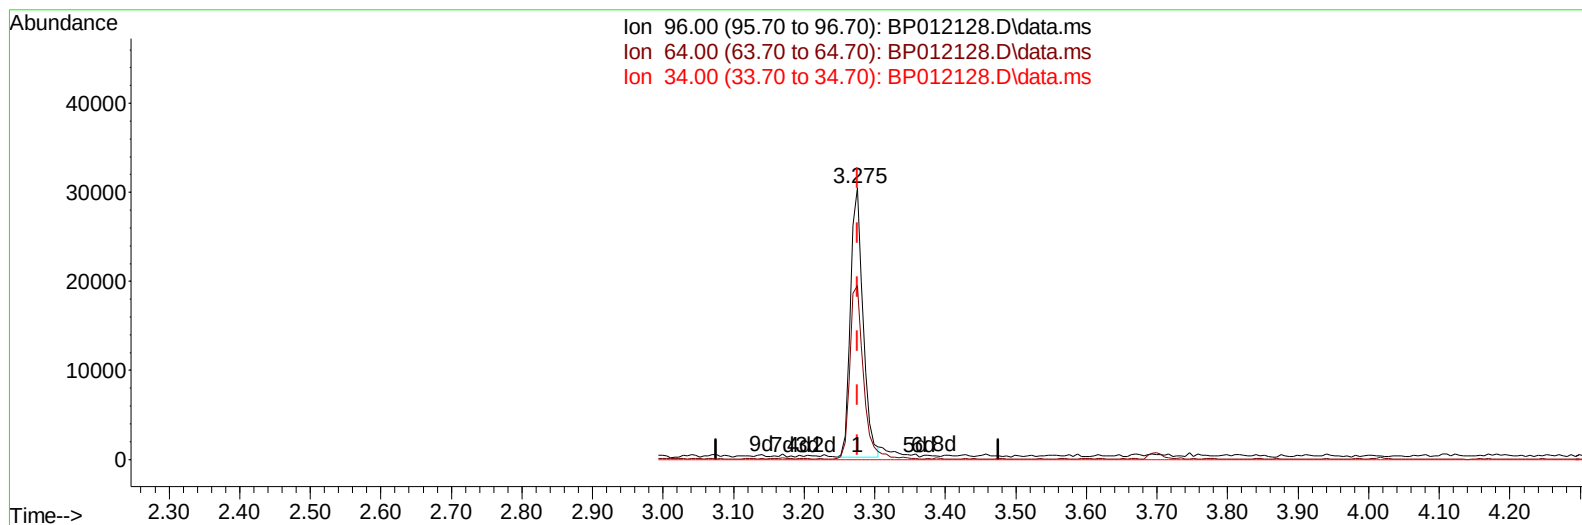

TIC: BP012128.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.275min (-0.000) 4.73 ng/uL

response 37619

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	64.01
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012128.D
Acq On : 14 Oct 2022 09:32
Operator : CG/JU
Sample : PB148234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/15/2022
Supervised By :mohammad ahmed 10/16/2022

Quant Time: Oct 14 23:01:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

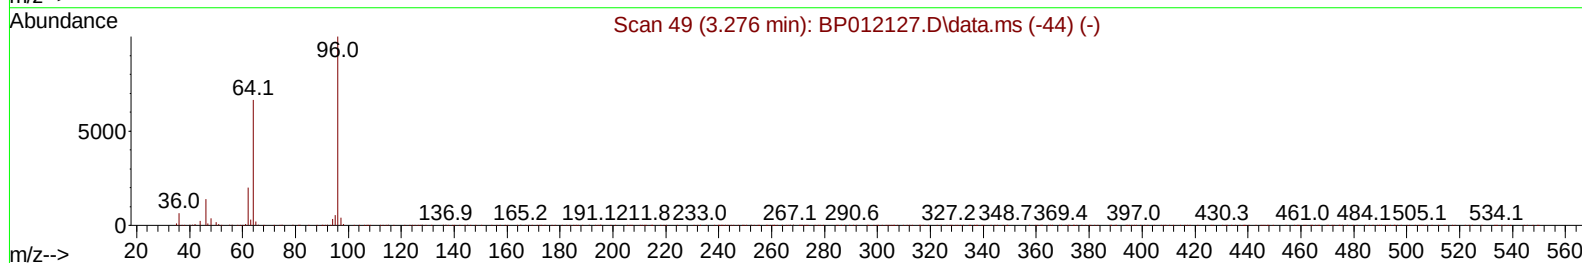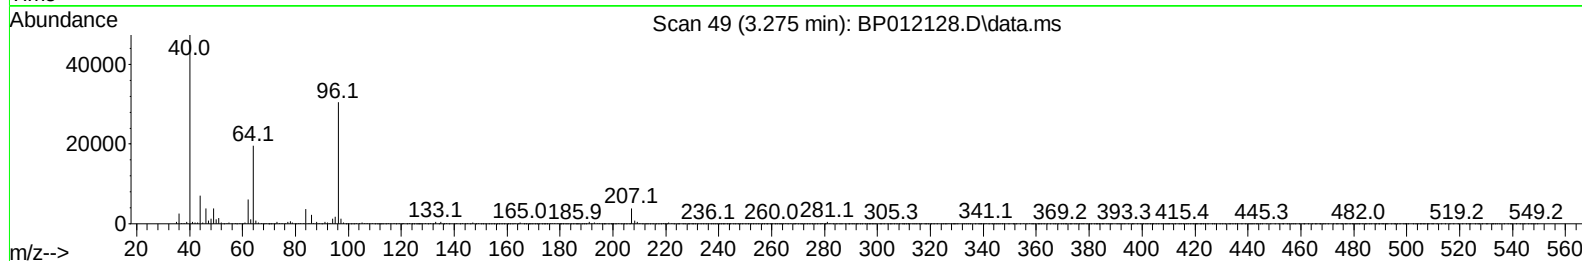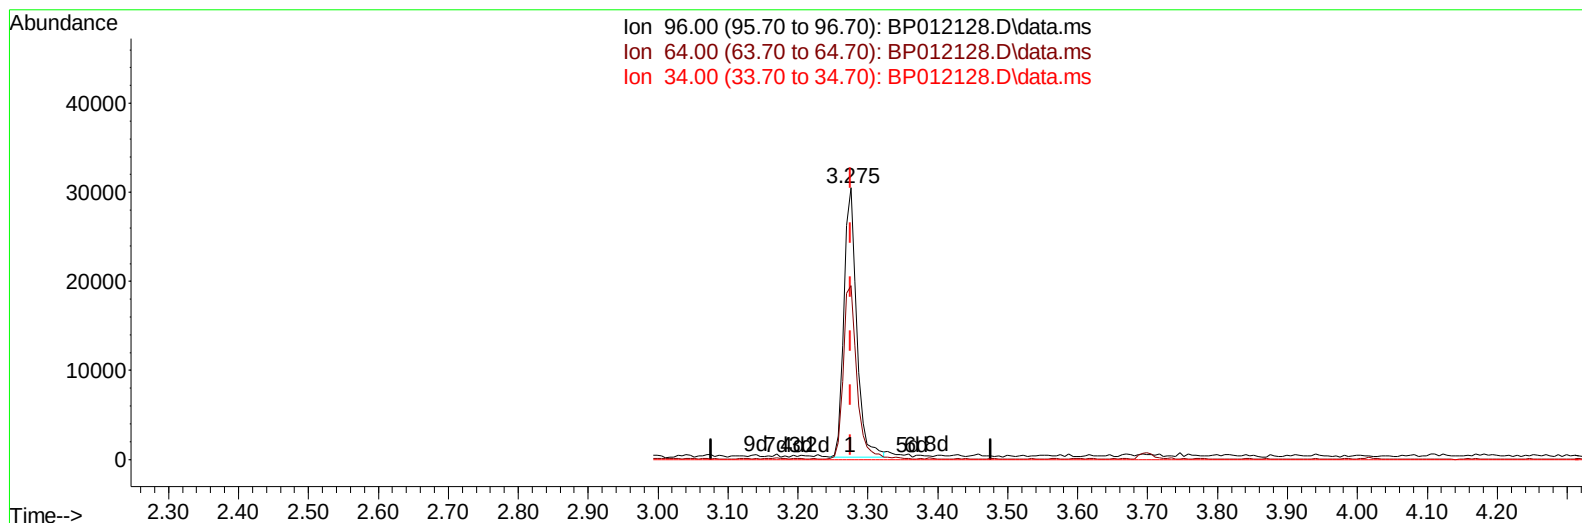

TIC: BP012128.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.275min (-0.000) 4.84 ng/uL m

response 38499

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	64.01
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012128.D
 Acq On : 14 Oct 2022 09:32
 Operator : CG/JU
 Sample : PB148234BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK234

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/15/2022
 Supervised By :mohammad ahmed 10/16/2022

Quant Time: Oct 14 23:01:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	313649	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	1336854	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	725044	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.257	188	1294635	20.000	ng/ul	0.00
79) Chrysene-d12	21.345	240	1287912	20.000	ng/ul	0.00
88) Perylene-d12	23.763	264	1372919	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	38499m	4.839	ng/uL	0.00
4) Pyridine-d5	3.693	84	508148	24.019	ng/ul	0.00
7) Phenol-d5	7.016	99	674458	26.737	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	392003	27.378	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	557551	27.845	ng/ul	0.00
15) 4-Methylphenol-d8	8.557	113	519529	26.814	ng/ul	0.00
21) Nitrobenzene-d5	9.016	128	272224	28.833	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	280927	29.344	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	472171	25.449	ng/ul	0.00
31) 4-Chloroaniline-d4	10.799	131	736050	26.920	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	1214670	26.453	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	1531280	26.968	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	162270	18.001	ng/ul	0.00
60) Fluorene-d10	15.492	176	1088973	26.212	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	112904	16.516	ng/ul	0.00
73) Anthracene-d10	17.357	188	1520036	27.038	ng/ul	0.00
81) Pyrene-d10	19.592	212	1708907	25.900	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.610	264	1843533	27.622	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012128.D
Acq On : 14 Oct 2022 09:32
Operator : CG/JU
Sample : PB148234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/15/2022
Supervised By :mohammad ahmed 10/16/2022

Quant Time: Oct 14 23:01:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

