




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012150.D
 Acq On : 14 Oct 2022 22:44
 Operator : CG/JU
 Sample : N4984-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGNC4

Manual IntegrationsAPPROVED

Quant Time: Oct 15 02:14:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/15/2022
 Supervised By :mohammad ahmed 10/16/2022

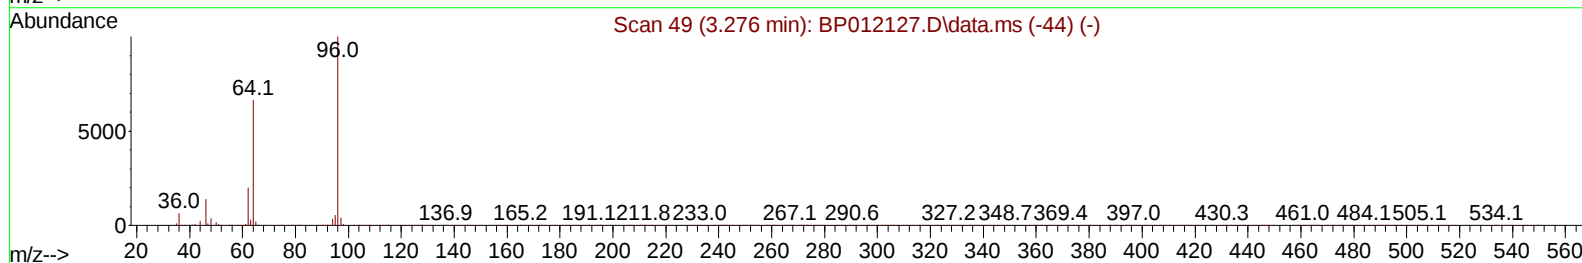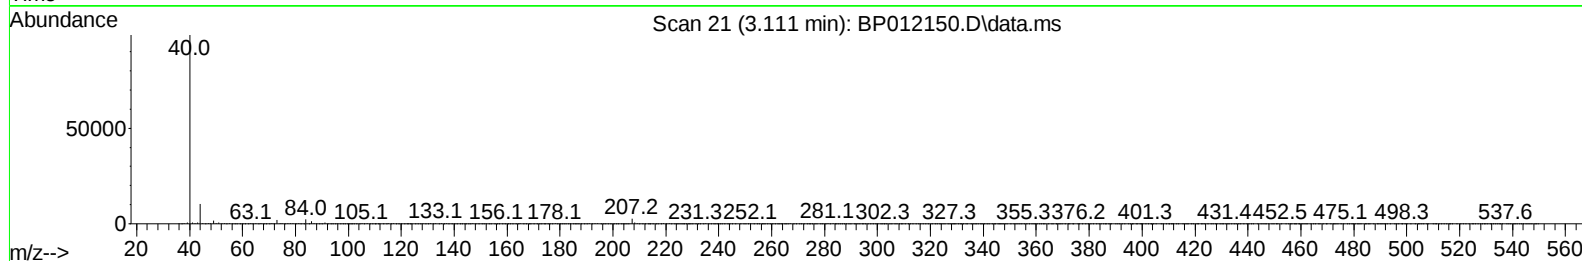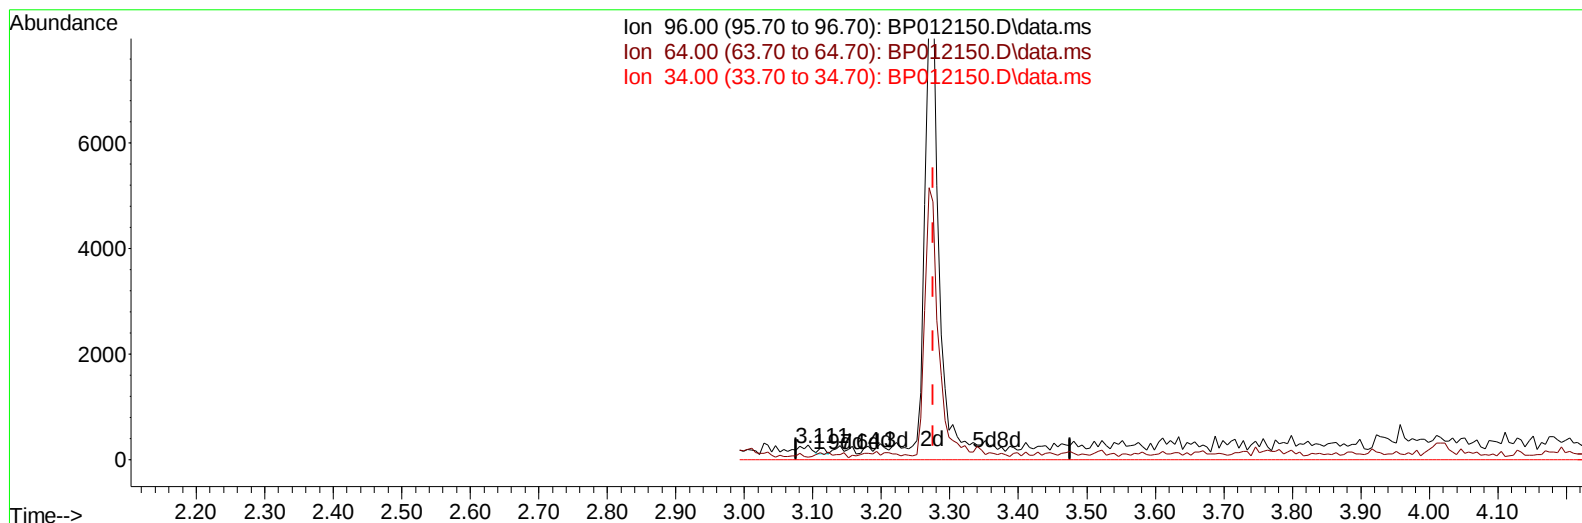

TIC: BP012150.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.111min (-0.165) 0.01 ng/uL

response 76

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	58.06
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012150.D
 Acq On : 14 Oct 2022 22:44
 Operator : CG/JU
 Sample : N4984-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGNC4

Manual IntegrationsAPPROVED

Quant Time: Oct 15 02:14:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/15/2022
 Supervised By :mohammad ahmed 10/16/2022

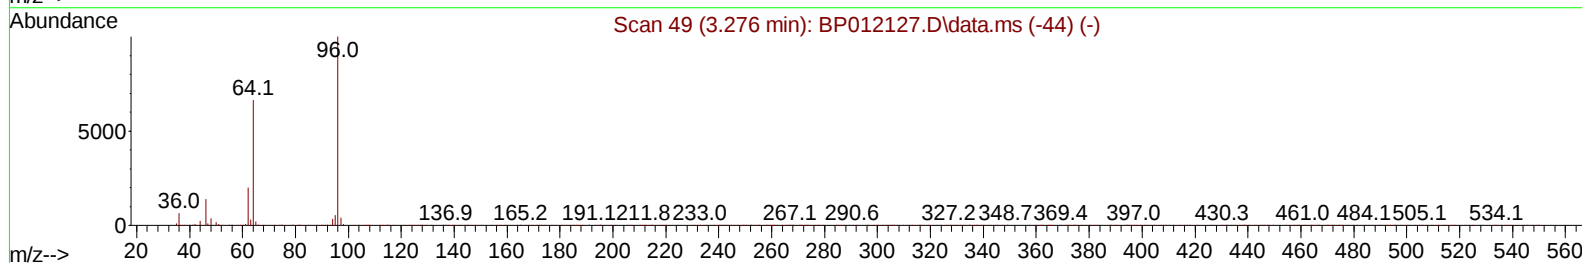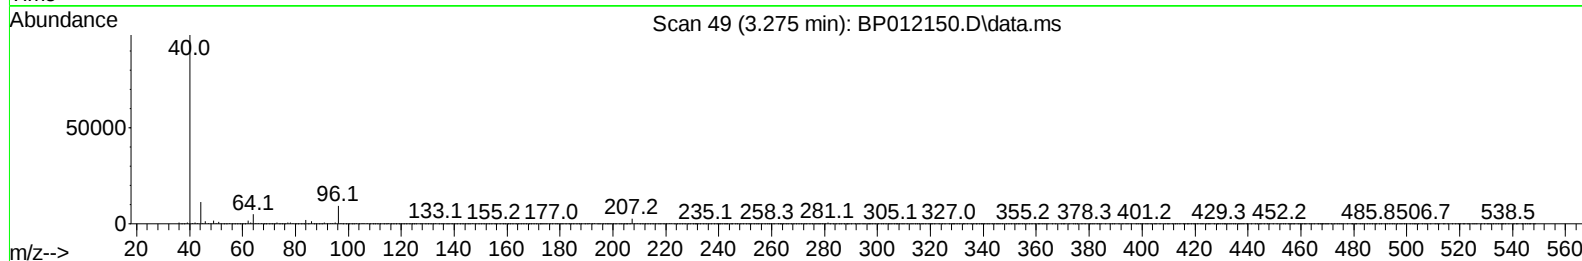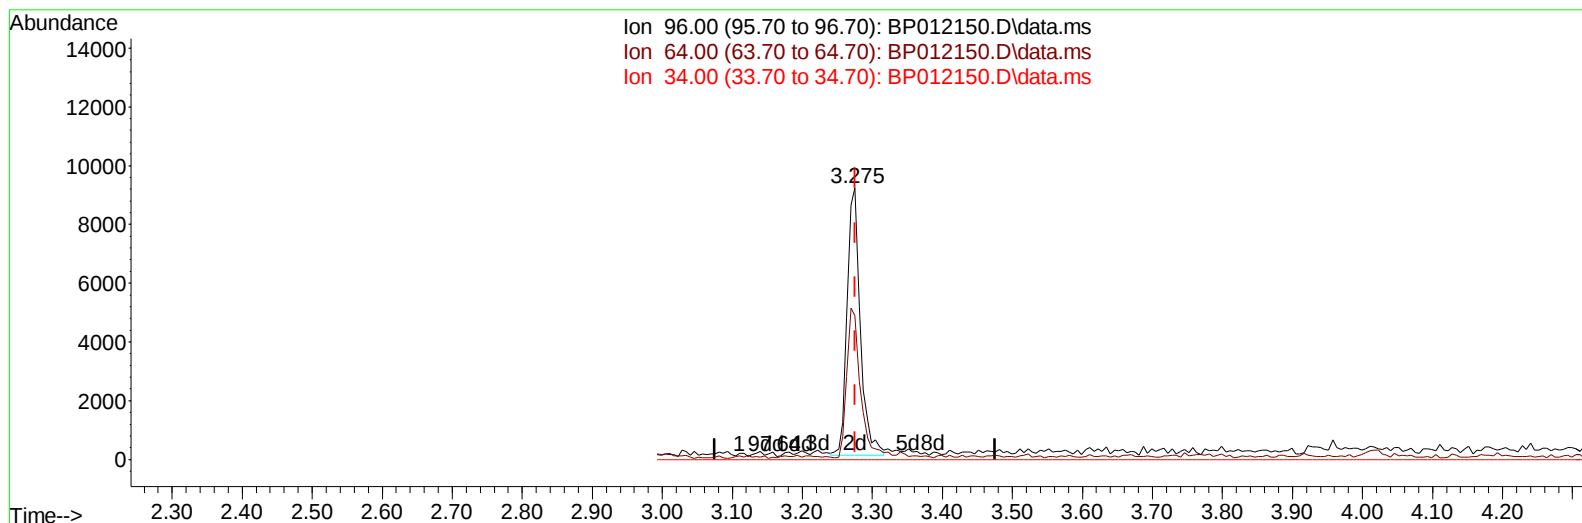

TIC: BP012150.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.275min (-0.000) 2.03 ng/uL m

response 11873

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	52.89#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012150.D
 Acq On : 14 Oct 2022 22:44
 Operator : CG/JU
 Sample : N4984-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGNC4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/15/2022
 Supervised By :mohammad ahmed 10/16/2022

Quant Time: Oct 15 02:14:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	230493	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.646	136	972135	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.492	164	575377	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	1224155	20.000	ng/ul	0.00
79) Chrysene-d12	21.345	240	1223961	20.000	ng/ul	0.00
88) Perylene-d12	23.757	264	1264270	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	11873m	2.031	ng/uL	0.00
4) Pyridine-d5	3.711	84	23199	1.492	ng/ul	0.01
7) Phenol-d5	7.010	99	357943	19.309	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	218193	20.736	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.369	132	292737	19.894	ng/ul	-0.01
15) 4-Methylphenol-d8	8.557	113	273840	19.232	ng/ul	0.00
21) Nitrobenzene-d5	9.010	128	134215	19.549	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.734	143	133166	19.128	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.269	165	245889	18.225	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.793	131	310646	15.624	ng/ul	-0.01
46) Dimethylphthalate-d6	13.904	166	693720	19.038	ng/ul	-0.01
49) Acenaphthylene-d8	14.187	160	862847	19.149	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	58902	8.234	ng/ul	0.00
60) Fluorene-d10	15.486	176	674815	20.468	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.616	200	36473	5.643	ng/ul	0.00
73) Anthracene-d10	17.351	188	1076935	20.259	ng/ul	0.00
81) Pyrene-d10	19.586	212	1257175	20.049	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.604	264	1237013	20.127	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012150.D
Acq On : 14 Oct 2022 22:44
Operator : CG/JU
Sample : N4984-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGNC4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/15/2022
Supervised By :mohammad ahmed 10/16/2022

Quant Time: Oct 15 02:14:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

