

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012132.D
 Acq On : 14 Oct 2022 11:49
 Operator : CG/JU
 Sample : N4976-06DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Y1DL

Quant Time: Oct 14 23:02:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.845	152	209903	20.000	ng/u1	0.00
20) Naphthalene-d8	10.651	136	854235	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.498	164	472666	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.257	188	946759	20.000	ng/u1	0.00
79) Chrysene-d12	21.345	240	1033104	20.000	ng/u1	0.00
88) Perylene-d12	23.762	264	1122830	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	7746	1.455	ng/uL	0.00
4) Pyridine-d5	3.704	84	86135	6.084	ng/u1	0.00
7) Phenol-d5	7.016	99	87762	5.199	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	178310	18.608	ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	222290	16.589	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	149128	11.501	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	126618	20.987	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	126917	20.747	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	224941	18.973	ng/u1	0.00
31) 4-Chloroaniline-d4	10.798	131	101533	5.812	ng/u1	0.00
46) Dimethylphthalate-d6	13.910	166	669824	22.376	ng/u1	0.00
49) Acenaphthylene-d8	14.186	160	809039	21.856	ng/u1	0.00
54) 4-Nitrophenol-d4	14.722	143	21990	3.742	ng/u1	0.01
60) Fluorene-d10	15.492	176	612481	22.615	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	67054	13.413	ng/u1	0.00
73) Anthracene-d10	17.351	188	932599	22.684	ng/u1	0.00
81) Pyrene-d10	19.592	212	1168731	22.082	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.603	264	1240365	22.724	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.310	88	102711	18.334	ng/uL	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012132.D
Acq On : 14 Oct 2022 11:49
Operator : CG/JU
Sample : N4976-06DL 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Y1DL

Quant Time: Oct 14 23:02:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

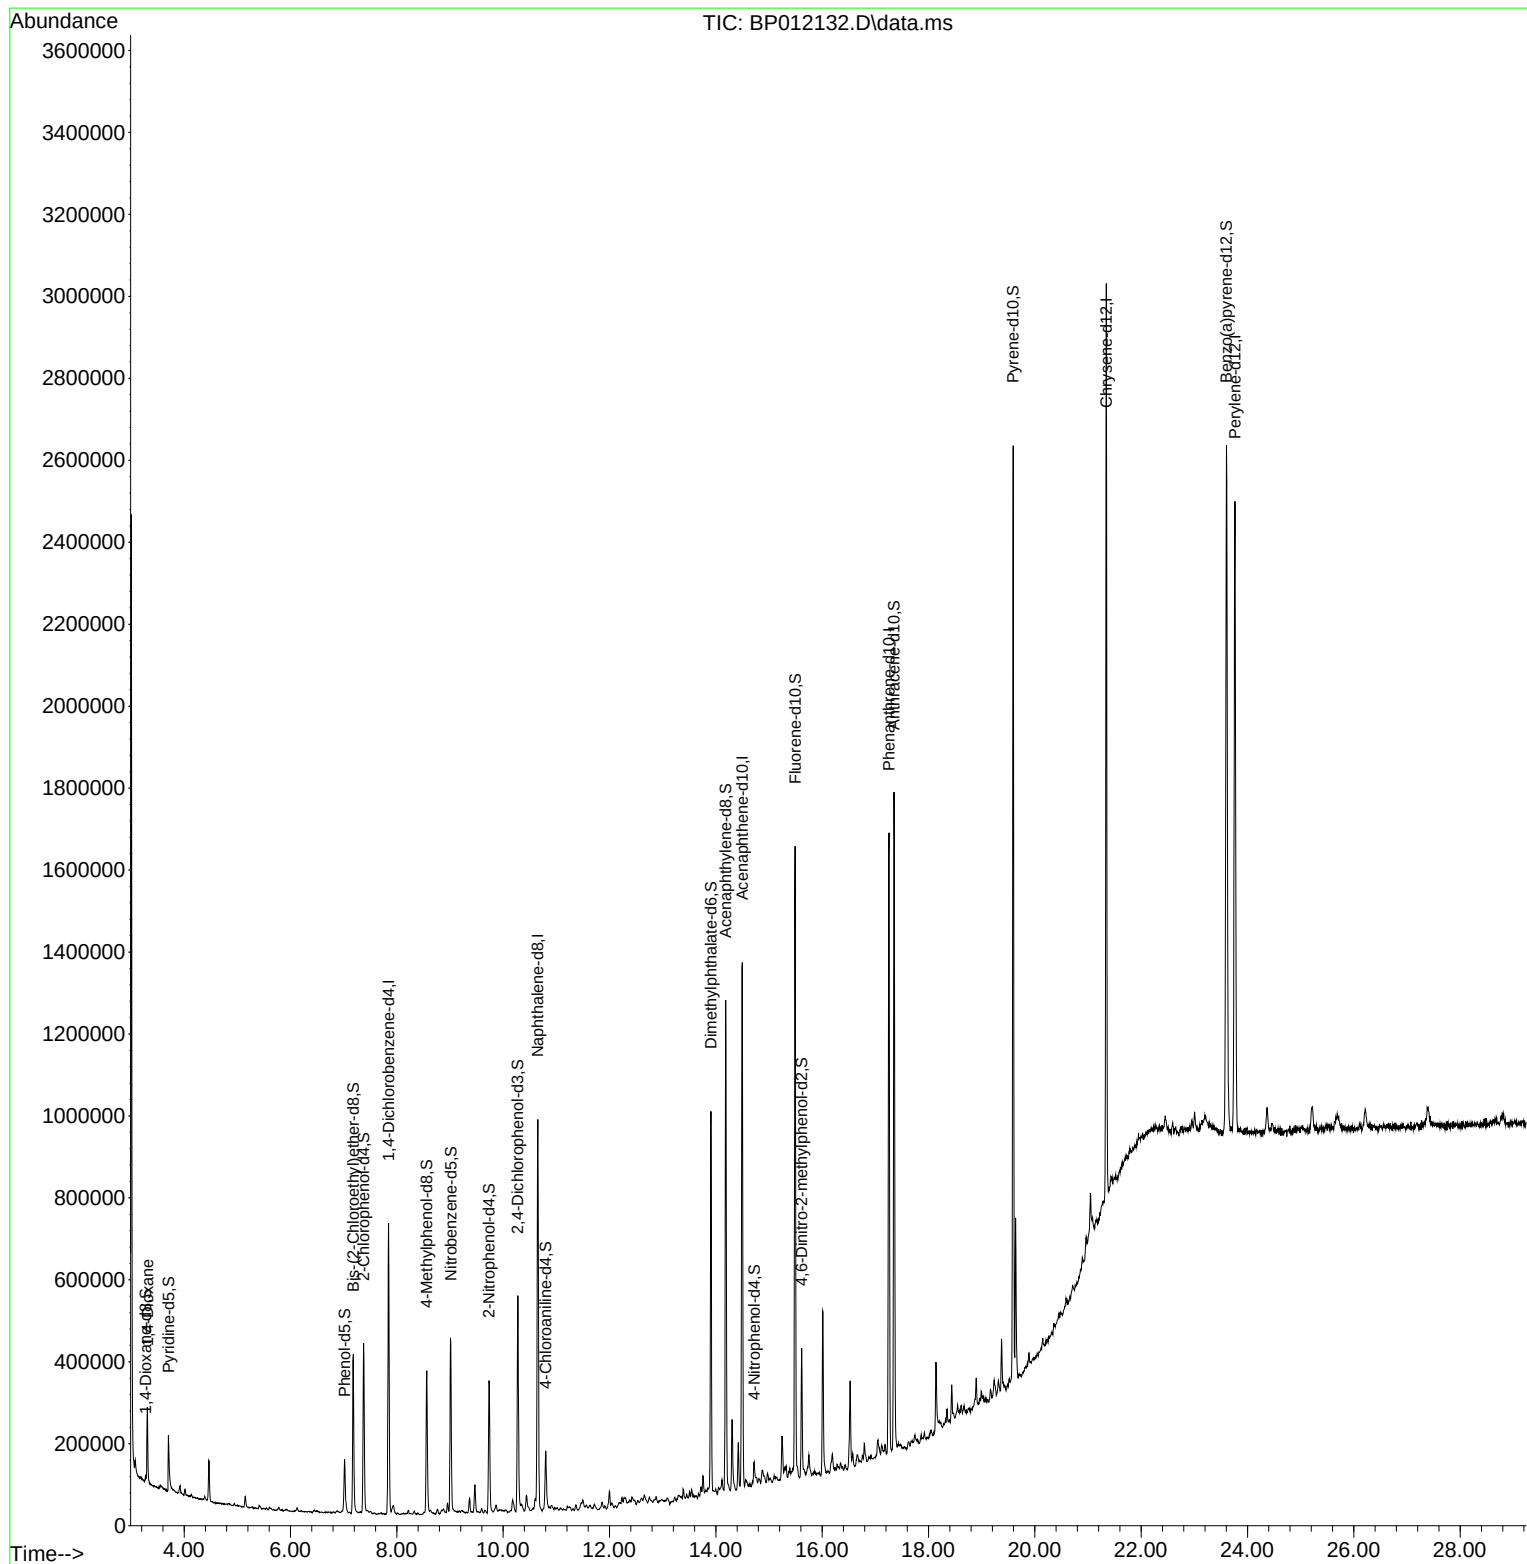

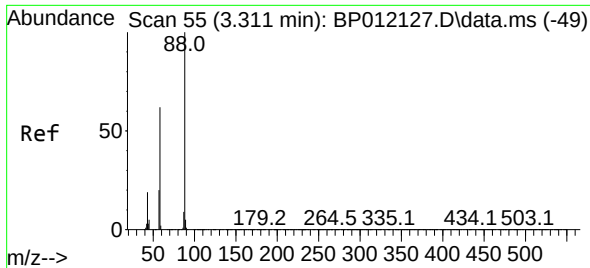

#2
 1,4-Dioxane
 Concen: 18.334 ng/uL
 RT: 3.310 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP012132.D
 Acq: 14 Oct 2022 11:49

Instrument :
 BNA_P
 ClientSampleId :
 CB8Y1DL

Tgt Ion: 88 Resp: 102711
 Ion Ratio Lower Upper
 88 100
 43 18.2 16.6 25.0
 58 62.2 52.6 79.0

