

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012139.D
 Acq On : 14 Oct 2022 15:51
 Operator : CG/JU
 Sample : N4982-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BB9

Quant Time: Oct 14 23:03:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	289200	20.000	ng/u1	0.00
20) Naphthalene-d8	10.652	136	1217248	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.498	164	658878	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.257	188	1318866	20.000	ng/u1	0.00
79) Chrysene-d12	21.345	240	1430488	20.000	ng/u1	0.00
88) Perylene-d12	23.763	264	1538484	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	23125	3.153	ng/uL	0.00
4) Pyridine-d5	3.705	84	98113	5.030	ng/u1	0.00
7) Phenol-d5	7.016	99	143082	6.152	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	342739	25.961	ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	389736	21.110	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	220747	12.356	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	235070	27.344	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	231950	26.609	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	384954	22.787	ng/u1	0.00
31) 4-Chloroaniline-d4	10.799	131	175287	7.041	ng/u1	0.00
46) Dimethylphthalate-d6	13.910	166	1189981	28.518	ng/u1	0.00
49) Acenaphthylene-d8	14.187	160	1405330	27.235	ng/u1	0.00
54) 4-Nitrophenol-d4	14.722	143	35630	4.349	ng/u1	0.01
60) Fluorene-d10	15.492	176	1076906	28.525	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	138056	19.824	ng/u1	0.00
73) Anthracene-d10	17.357	188	1650093	28.812	ng/u1	0.00
81) Pyrene-d10	19.592	212	2066582	28.199	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.610	264	2263994	30.272	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.046	94	24642	1.009	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012139.D
Acq On : 14 Oct 2022 15:51
Operator : CG/JU
Sample : N4982-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB9

Quant Time: Oct 14 23:03:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

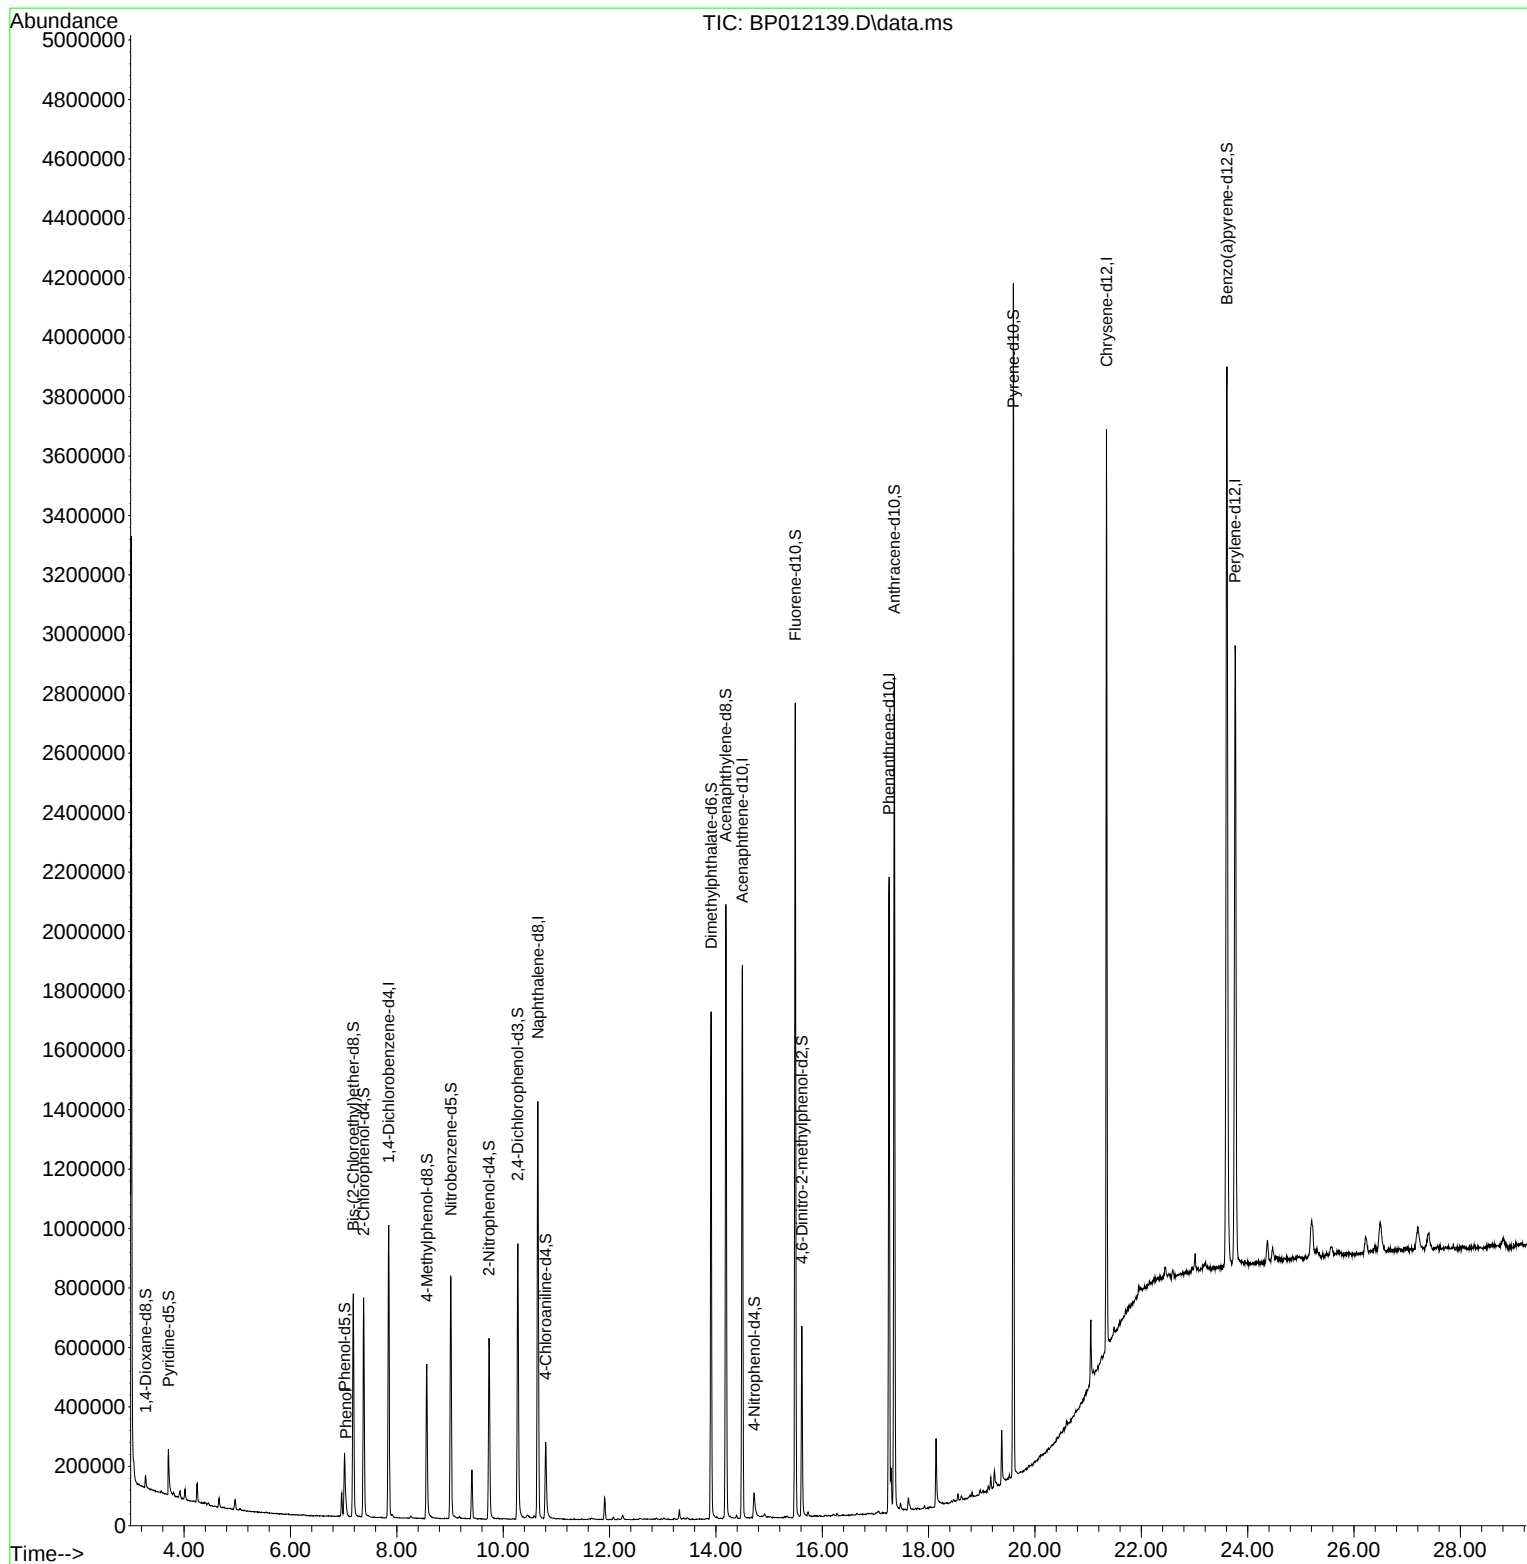

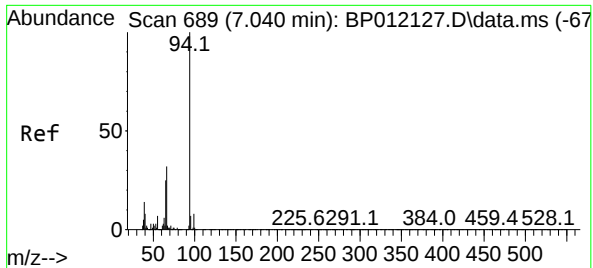

#8
Phenol
Concen: 1.009 ng/ul
RT: 7.046 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP012139.D
Acq: 14 Oct 2022 15:51

Instrument :
BNA_P
ClientSampleId :
C1BB9

Tgt Ion: 94	Resp:	24642
Ion	Ratio	Lower Upper
94	100	
65	28.6	19.4 29.0
66	34.5	24.6 37.0

