

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012151.D
 Acq On : 14 Oct 2022 23:19
 Operator : CG/JU
 Sample : N4984-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGNC5

Quant Time: Oct 15 02:17:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 23:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	248669	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.646	136	1009419	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.492	164	558512	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	1142007	20.000	ng/ul	0.00
79) Chrysene-d12	21.339	240	1201653	20.000	ng/ul	# 0.00
88) Perylene-d12	23.757	264	1269039	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	13668	2.167	ng/uL	0.00
4) Pyridine-d5	3.705	84	37577	2.240	ng/ul	0.00
7) Phenol-d5	7.011	99	481681	24.085	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	285174	25.121	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.369	132	389484	24.534	ng/ul	-0.01
15) 4-Methylphenol-d8	8.557	113	363347	23.653	ng/ul	0.00
21) Nitrobenzene-d5	9.010	128	172791	24.238	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.734	143	179977	24.898	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.269	165	312408	22.300	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.793	131	385924	18.693	ng/ul	-0.01
46) Dimethylphthalate-d6	13.904	166	820995	23.211	ng/ul	-0.01
49) Acenaphthylene-d8	14.187	160	1000431	22.872	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	83813	12.070	ng/ul	0.00
60) Fluorene-d10	15.487	176	757062	23.656	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.616	200	52967	8.784	ng/ul	0.00
73) Anthracene-d10	17.351	188	1225923	24.721	ng/ul	0.00
81) Pyrene-d10	19.586	212	1457867	23.681	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.598	264	1496125	24.252	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.034	94	26265	1.251	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012151.D
Acq On : 14 Oct 2022 23:19
Operator : CG/JU
Sample : N4984-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGNC5

Quant Time: Oct 15 02:17:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 23:03:21 2022
Response via : Initial Calibration

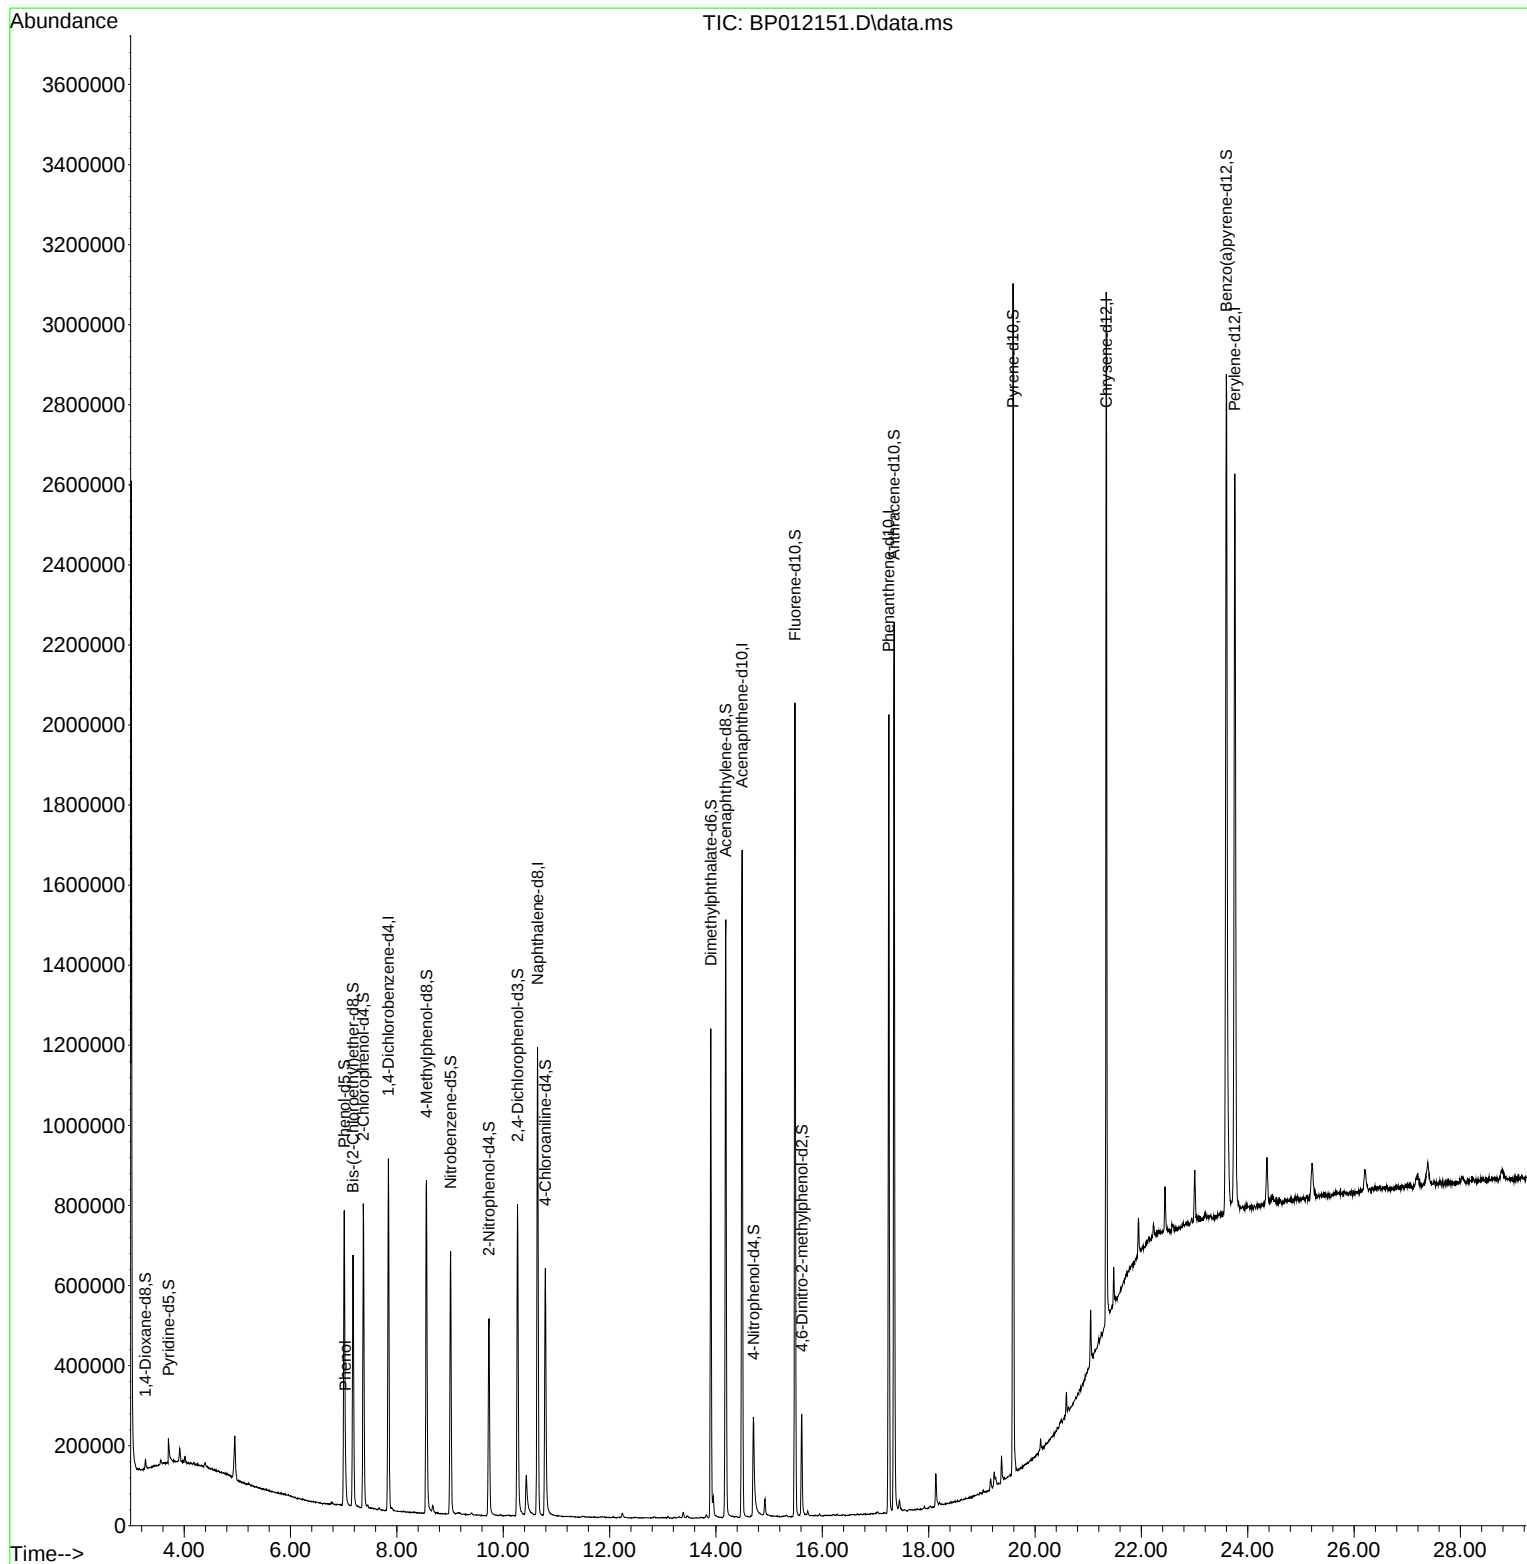

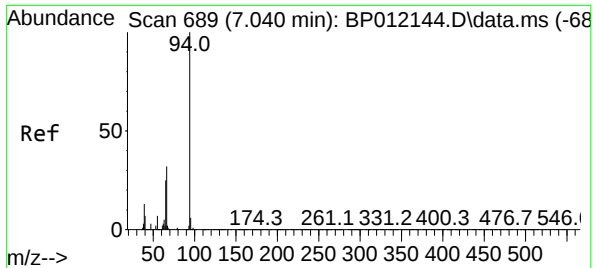

#8
Phenol
Concen: 1.251 ng/ul
RT: 7.034 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP012151.D
Acq: 14 Oct 2022 23:19

Instrument :
BNA_P
ClientSampleId :
BGNC5

Tgt Ion:	94	Resp:	26265
Ion	Ratio	Lower	Upper
94	100		
65	27.6	19.4	29.0
66	45.0	24.6	37.0

