

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012129.D
 Acq On : 14 Oct 2022 10:06
 Operator : CG/JU
 Sample : N5024-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	55	rVB	36284	46560	1.13%	0.112%
2	3.917	154	158	164	rVB	42225	65592	1.59%	0.158%
3	4.017	171	175	181	rVB	35808	48132	1.16%	0.116%
4	4.940	328	332	342	rVB	21956	41645	1.01%	0.100%
5	5.846	482	486	494	rVB8	6640	12258	0.30%	0.029%
6	7.016	679	685	698	rBV	227469	401350	9.71%	0.966%
7	7.181	706	713	730	rBV	443618	749428	18.12%	1.803%
8	7.375	740	746	757	rBV	371226	600828	14.53%	1.446%
9	7.458	757	760	769	rVB3	17371	28468	0.69%	0.068%
10	7.846	817	826	836	rBV	972305	1590242	38.46%	3.826%
11	8.499	931	937	940	rBV7	3569	6519	0.16%	0.016%
12	8.563	942	948	958	rBV	89713	176734	4.27%	0.425%
13	8.681	963	968	980	rVB	28626	57045	1.38%	0.137%
14	9.010	1017	1024	1032	rBV	467751	806416	19.50%	1.940%
15	9.181	1049	1053	1057	rVB7	3963	6303	0.15%	0.015%
16	9.410	1086	1092	1099	rBV3	7912	17328	0.42%	0.042%
17	9.734	1141	1147	1160	rBV	323136	571267	13.82%	1.374%
18	10.275	1232	1239	1258	rBV	330284	644429	15.58%	1.551%
19	10.434	1263	1266	1270	rVB6	4777	6909	0.17%	0.017%
20	10.652	1294	1303	1309	rBV	1388836	2341023	56.61%	5.633%
21	10.699	1309	1311	1321	rVB	62140	94141	2.28%	0.227%
22	10.805	1323	1329	1339	rBV2	69937	159298	3.85%	0.383%
23	12.069	1538	1544	1550	rBV9	7529	14257	0.34%	0.034%
24	12.240	1567	1573	1580	rBV5	9364	19418	0.47%	0.047%
25	12.322	1582	1587	1593	rVB2	17098	31548	0.76%	0.076%
26	12.534	1618	1623	1631	rVB	14411	26367	0.64%	0.063%
27	13.099	1714	1719	1726	rVB	3343	6771	0.16%	0.016%
28	13.310	1750	1755	1763	rBV3	15577	41446	1.00%	0.100%
29	13.387	1766	1768	1773	rVB5	5360	7185	0.17%	0.017%
30	13.669	1814	1816	1822	rVB5	4679	7731	0.19%	0.019%
31	13.816	1835	1841	1846	rBV4	15307	28879	0.70%	0.069%
32	13.904	1850	1856	1872	rVB	921858	1363419	32.97%	3.280%
33	14.051	1877	1881	1884	rVV4	6994	9935	0.24%	0.024%
34	14.081	1884	1886	1892	rVB7	4507	5921	0.14%	0.014%
35	14.187	1894	1904	1923	rBV	1199619	1865457	45.11%	4.488%
36	14.387	1934	1938	1942	rVB2	12225	16865	0.41%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012129.D
 Acq On : 14 Oct 2022 10:06
 Operator : CG/JU
 Sample : N5024-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	14.493	1947	1956	1964	rBV	1878253	2761957	66.79%	6.645%
38	14.557	1964	1967	1975	rVV2	21486	33681	0.81%	0.081%
39	14.640	1975	1981	1984	rVV4	3532	5951	0.14%	0.014%
40	14.745	1993	1999	2003	rBV6	5970	14926	0.36%	0.036%
41	14.898	2020	2025	2030	rBV	42060	70209	1.70%	0.169%
42	15.163	2068	2070	2075	rVB6	4055	5836	0.14%	0.014%
43	15.287	2087	2091	2094	rBV2	10254	13857	0.34%	0.033%
44	15.340	2096	2100	2105	rVB4	13077	19034	0.46%	0.046%
45	15.492	2119	2126	2132	rBV	1540070	2245648	54.31%	5.403%
46	15.545	2132	2135	2142	rVB2	22110	36317	0.88%	0.087%
47	15.616	2142	2147	2155	rBV	65774	103156	2.49%	0.248%
48	15.745	2162	2169	2173	rVB6	9773	23231	0.56%	0.056%
49	15.840	2180	2185	2191	rBV2	16485	26920	0.65%	0.065%
50	15.992	2207	2211	2217	rVB	15570	27844	0.67%	0.067%
51	16.075	2223	2225	2231	rVB6	6133	9025	0.22%	0.022%
52	16.151	2234	2238	2243	rBV3	20102	27400	0.66%	0.066%
53	16.210	2243	2248	2249	rBV2	22247	30320	0.73%	0.073%
54	16.281	2256	2260	2263	rVB6	4458	6828	0.17%	0.016%
55	16.787	2341	2346	2350	rBV5	13809	27836	0.67%	0.067%
56	16.910	2362	2367	2374	rBV	65517	109437	2.65%	0.263%
57	16.981	2376	2379	2380	rVV2	10464	10781	0.26%	0.026%
58	17.004	2380	2383	2387	rVV3	19703	27683	0.67%	0.067%
59	17.069	2389	2394	2402	rVB2	33084	64929	1.57%	0.156%
60	17.251	2419	2425	2429	rBV	1975618	2894400	70.00%	6.964%
61	17.298	2429	2433	2437	rVV	783838	1118376	27.05%	2.691%
62	17.351	2437	2442	2455	rVV	1316652	2044211	49.44%	4.918%
63	17.451	2457	2459	2468	rVB10	22432	40593	0.98%	0.098%
64	17.669	2492	2496	2505	rVB	37227	60892	1.47%	0.147%
65	17.745	2507	2509	2512	rVV3	10977	13154	0.32%	0.032%
66	17.775	2512	2514	2520	rVB5	14490	19845	0.48%	0.048%
67	17.839	2522	2525	2533	rVB8	10119	19909	0.48%	0.048%
68	17.922	2536	2539	2545	rBV7	12706	19339	0.47%	0.047%
69	18.128	2569	2574	2578	rBV	60662	119747	2.90%	0.288%
70	18.169	2578	2581	2586	rVB2	76091	107132	2.59%	0.258%
71	18.310	2600	2605	2609	rBV2	56449	103596	2.51%	0.249%
72	18.345	2609	2611	2620	rVB2	41449	52948	1.28%	0.127%
73	18.416	2621	2623	2628	rBV4	13594	19273	0.47%	0.046%
74	18.610	2652	2656	2659	rBV	51491	70734	1.71%	0.170%
75	18.651	2659	2663	2669	rVB	68594	98848	2.39%	0.238%
76	19.016	2721	2725	2730	rBV6	33789	67361	1.63%	0.162%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012129.D
 Acq On : 14 Oct 2022 10:06
 Operator : CG/JU
 Sample : N5024-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BE8

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

77	19.151	2744	2748	2756	rBV2	59945	127387	3.08%	0.306%
78	19.269	2760	2768	2775	rVV	1197309	1629133	39.40%	3.920%
79	19.592	2817	2823	2826	rBV	2000593	2894236	69.99%	6.964%
80	19.622	2826	2828	2836	rVB	998325	1065838	25.78%	2.564%
81	21.045	3067	3070	3073	rBV2	178646	227767	5.51%	0.548%
82	21.345	3115	3121	3125	rBV	2852654	4135025	100.00%	9.949%
83	21.380	3125	3127	3135	rVB	450123	564466	13.65%	1.358%
84	23.022	3401	3406	3412	rBV2	450271	1073158	25.95%	2.582%
85	23.604	3500	3505	3510	rBV2	892445	1742599	42.14%	4.193%
86	23.763	3526	3532	3539	rVB2	1908705	3612484	87.36%	8.692%




Sum of corrected areas: 41562371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012129\
Data File : BP012129.D
Acq On : 14 Oct 2022 10:06
Operator : CG/JU
Sample : N5024-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

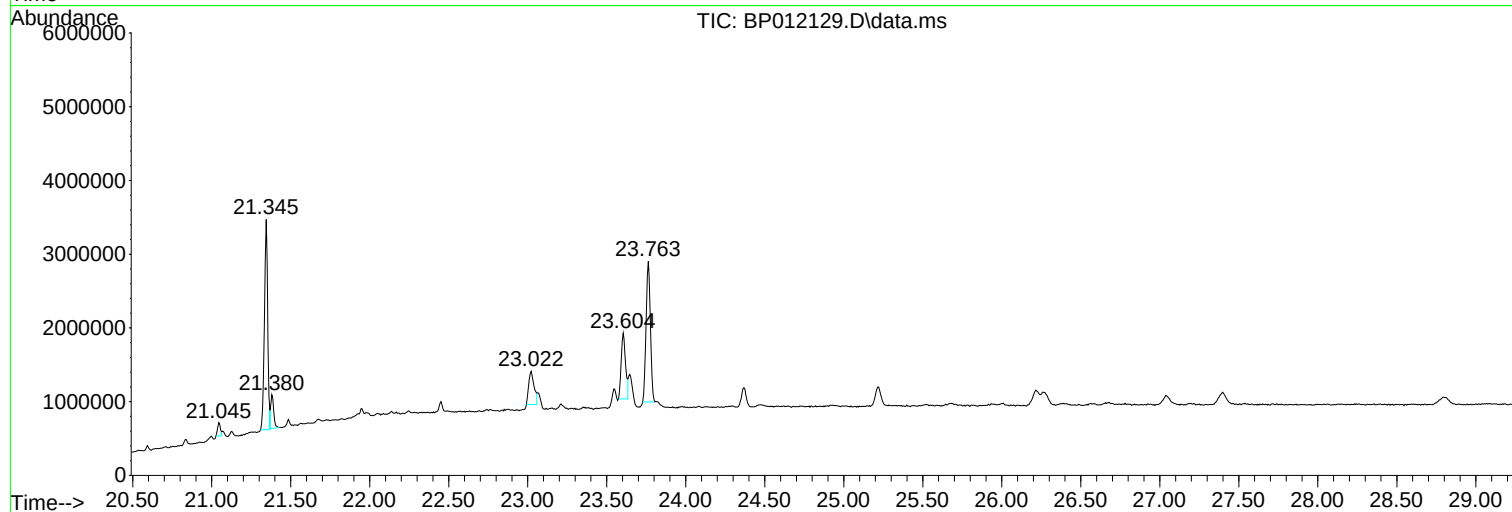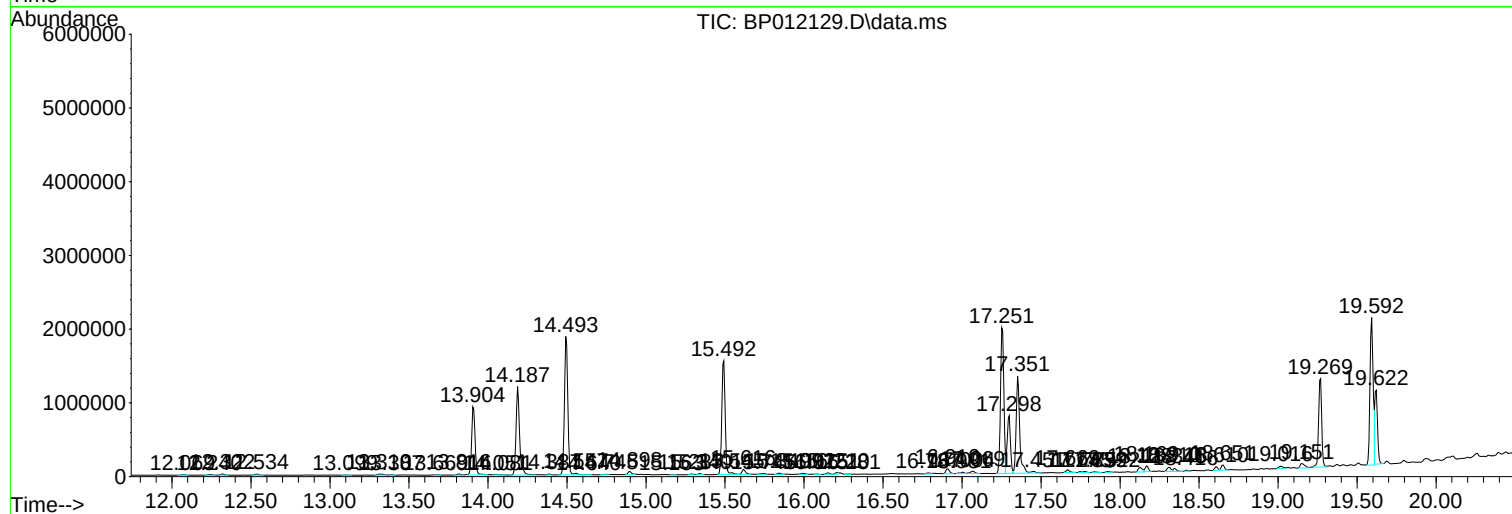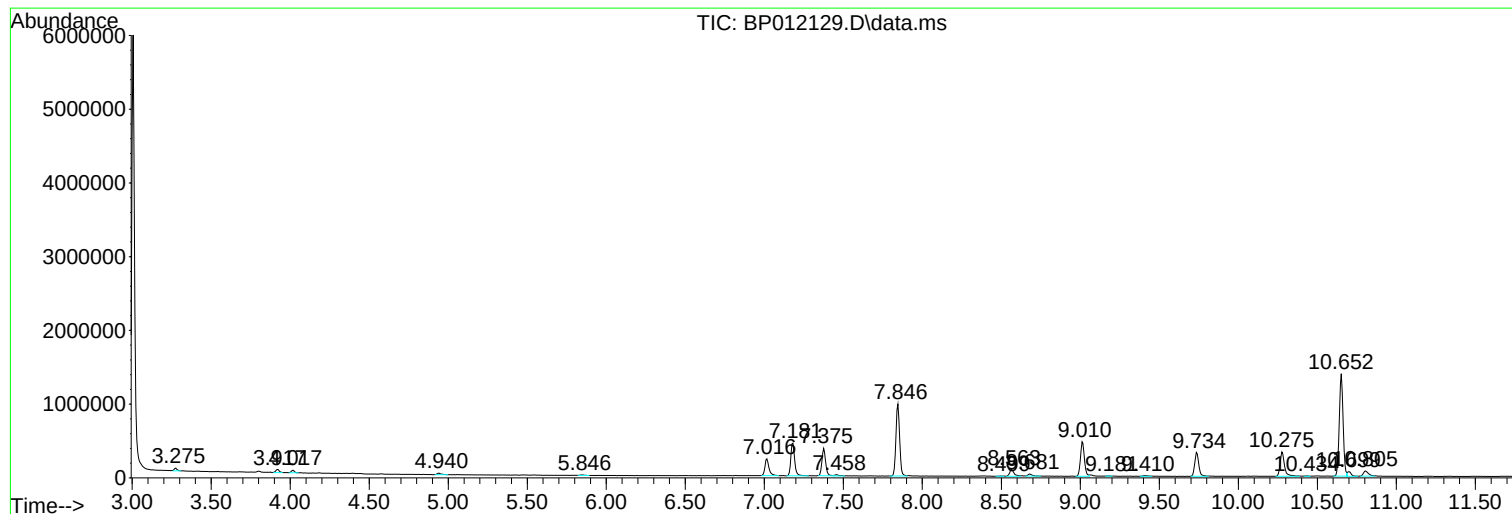

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012129.D
Acq On : 14 Oct 2022 10:06
Operator : CG/JU
Sample : N5024-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012129.D
Acq On : 14 Oct 2022 10:06
Operator : CG/JU
Sample : N5024-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc