

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012130.D
 Acq On : 14 Oct 2022 10:40
 Operator : CG/JU
 Sample : N5024-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	61	rVB2	47337	76095	1.67%	0.148%
2	3.705	120	122	135	rVV	125392	178292	3.91%	0.346%
3	3.799	135	138	144	rVB2	31225	43431	0.95%	0.084%
4	3.916	154	158	164	rVB	45305	68334	1.50%	0.132%
5	4.016	172	175	183	rVB	29312	43710	0.96%	0.085%
6	4.952	328	334	343	rVV2	65932	132205	2.90%	0.256%
7	5.475	418	423	431	rBV2	13757	27559	0.60%	0.053%
8	5.846	480	486	493	rVB3	30326	45104	0.99%	0.087%
9	6.328	564	568	574	rVB8	8311	17605	0.39%	0.034%
10	6.469	588	592	595	rVV5	8813	16288	0.36%	0.032%
11	7.016	676	685	700	rVB	613388	1062059	23.31%	2.059%
12	7.181	706	713	727	rBV	578443	958192	21.03%	1.858%
13	7.375	740	746	756	rBV	693166	1108212	24.32%	2.149%
14	7.457	756	760	763	rVV	23362	36892	0.81%	0.072%
15	7.487	763	765	770	rVB	17827	23309	0.51%	0.045%
16	7.846	816	826	839	rBV	1052665	1697180	37.25%	3.290%
17	8.557	940	947	959	rBV	612282	1071080	23.51%	2.077%
18	8.681	962	968	976	rVB	73236	128154	2.81%	0.248%
19	9.010	1017	1024	1031	rVV	642119	1083150	23.77%	2.100%
20	9.069	1031	1034	1040	rVV	29185	47730	1.05%	0.093%
21	9.181	1049	1053	1062	rVB	9936	24895	0.55%	0.048%
22	9.734	1140	1147	1159	rBV	484547	834430	18.31%	1.618%
23	10.099	1206	1209	1215	rVB5	9901	16787	0.37%	0.033%
24	10.275	1232	1239	1251	rBV	768264	1319881	28.97%	2.559%
25	10.440	1260	1267	1282	rBV	91071	215729	4.73%	0.418%
26	10.651	1293	1303	1309	rBV	1538113	2600123	57.06%	5.041%
27	10.698	1309	1311	1317	rVV	63331	93035	2.04%	0.180%
28	10.798	1321	1328	1350	rVB	469278	922806	20.25%	1.789%
29	11.493	1436	1446	1451	rBV	6280	17951	0.39%	0.035%
30	11.563	1452	1458	1464	rVB8	8632	18636	0.41%	0.036%
31	11.669	1464	1476	1488	rBV4	22070	46833	1.03%	0.091%
32	12.069	1538	1544	1554	rVB	45412	72066	1.58%	0.140%
33	12.240	1568	1573	1579	rBV3	13753	22090	0.48%	0.043%
34	12.316	1579	1586	1594	rVB	90197	145288	3.19%	0.282%
35	12.534	1617	1623	1629	rVB	79349	122953	2.70%	0.238%
36	13.022	1701	1706	1712	rVB	17822	29033	0.64%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012130.D
 Acq On : 14 Oct 2022 10:40
 Operator : CG/JU
 Sample : N5024-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	13.310	1750	1755	1763	rBV2	45416	83564	1.83%	0.162%
38	13.657	1807	1814	1815	rBV2	30852	47943	1.05%	0.093%
39	13.810	1835	1840	1845	rBV	75957	135923	2.98%	0.264%
40	13.869	1845	1850	1852	rVV	63925	105638	2.32%	0.205%
41	13.910	1852	1857	1863	rVV	1216808	1753588	38.48%	3.400%
42	13.969	1863	1867	1871	rVV	39380	62348	1.37%	0.121%
43	14.010	1871	1874	1877	rVV4	9869	16528	0.36%	0.032%
44	14.051	1877	1881	1884	rVV	46553	71530	1.57%	0.139%
45	14.081	1884	1886	1892	rVB4	22885	29600	0.65%	0.057%
46	14.187	1897	1904	1921	rVB	1616218	2393541	52.53%	4.641%
47	14.387	1933	1938	1944	rBV	43714	56307	1.24%	0.109%
48	14.492	1946	1956	1963	rBV	2056014	3132720	68.75%	6.074%
49	14.557	1963	1967	1975	rVB3	30596	64621	1.42%	0.125%
50	14.710	1987	1993	2002	rBV	227336	462090	10.14%	0.896%
51	14.892	2018	2024	2033	rBV2	72627	148251	3.25%	0.287%
52	14.969	2033	2037	2041	rVB	33648	48378	1.06%	0.094%
53	15.004	2041	2043	2053	rVB9	10314	23314	0.51%	0.045%
54	15.110	2056	2061	2066	rBV	32726	55205	1.21%	0.107%
55	15.163	2066	2070	2075	rVB	28773	41054	0.90%	0.080%
56	15.281	2082	2090	2094	rBV4	45521	93716	2.06%	0.182%
57	15.316	2094	2096	2097	rVV	24057	23221	0.51%	0.045%
58	15.339	2097	2100	2105	rVB	46981	62265	1.37%	0.121%
59	15.428	2107	2115	2118	rBV8	7668	17071	0.37%	0.033%
60	15.492	2119	2126	2131	rVV	1959922	2869118	62.96%	5.563%
61	15.534	2131	2133	2139	rVB2	88505	117778	2.58%	0.228%
62	15.616	2141	2147	2155	rVV	279157	396264	8.70%	0.768%
63	15.751	2166	2170	2178	rVB4	26770	51649	1.13%	0.100%
64	15.839	2180	2185	2192	rVB	55569	94761	2.08%	0.184%
65	15.922	2192	2199	2200	rBV7	8140	16363	0.36%	0.032%
66	15.957	2201	2205	2206	rVV4	20000	25898	0.57%	0.050%
67	15.992	2206	2211	2218	rVV	56970	123642	2.71%	0.240%
68	16.081	2221	2226	2233	rVB2	25408	47600	1.04%	0.092%
69	16.228	2243	2251	2257	rBV2	100654	217453	4.77%	0.422%
70	16.357	2269	2273	2277	rBV2	16188	24162	0.53%	0.047%
71	16.551	2304	2306	2312	rVB6	12951	19037	0.42%	0.037%
72	16.786	2340	2346	2350	rBV3	59071	113740	2.50%	0.221%
73	16.910	2363	2367	2373	rBV3	25639	47255	1.04%	0.092%
74	17.004	2375	2383	2386	rVV3	67326	126665	2.78%	0.246%
75	17.069	2390	2394	2398	rVB3	19366	33163	0.73%	0.064%
76	17.257	2419	2426	2430	rBV	2022920	3003144	65.90%	5.822%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012130.D
 Acq On : 14 Oct 2022 10:40
 Operator : CG/JU
 Sample : N5024-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

77	17.298	2430	2433	2437	rVV	351507	467670	10.26%	0.907%
78	17.351	2437	2442	2453	rVB2	1679213	2529910	55.52%	4.905%
79	17.663	2492	2495	2502	rBV4	22478	42944	0.94%	0.083%
80	17.745	2506	2509	2513	rVB	62540	68575	1.50%	0.133%
81	18.133	2569	2575	2578	rBV2	117882	232996	5.11%	0.452%
82	18.169	2578	2581	2586	rVB	139708	195364	4.29%	0.379%
83	18.245	2591	2594	2599	rVV	22550	35663	0.78%	0.069%
84	18.304	2600	2604	2608	rVV3	88390	155765	3.42%	0.302%
85	18.345	2608	2611	2618	rVB	72088	106054	2.33%	0.206%
86	18.422	2620	2624	2628	rVV	74172	90108	1.98%	0.175%
87	18.545	2643	2645	2650	rVB6	22599	26106	0.57%	0.051%
88	18.610	2652	2656	2660	rBV2	41967	62867	1.38%	0.122%
89	19.010	2720	2724	2725	rBV	89487	107939	2.37%	0.209%
90	19.098	2737	2739	2743	rVB	48987	45451	1.00%	0.088%
91	19.163	2744	2750	2755	rVV5	46242	114100	2.50%	0.221%
92	19.263	2763	2767	2775	rVB	417120	548982	12.05%	1.064%
93	19.369	2782	2785	2789	rBV3	66141	85791	1.88%	0.166%
94	19.592	2818	2823	2827	rBV	2523267	3443858	75.58%	6.677%
95	20.104	2908	2910	2915	rVB2	124118	141103	3.10%	0.274%
96	20.592	2991	2993	2997	rVB2	103355	97895	2.15%	0.190%
97	21.045	3067	3070	3074	rBV	283842	354227	7.77%	0.687%
98	21.345	3115	3121	3125	rBV	2703483	3616962	79.38%	7.012%
99	23.604	3499	3505	3522	rVB2	1913127	4556784	100.00%	8.835%
100	23.762	3526	3532	3545	rVB2	1905951	3828697	84.02%	7.423%




Sum of corrected areas: 51579036

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP0101422\
Data File : BP012130.D
Acq On : 14 Oct 2022 10:40
Operator : CG/JU
Sample : N5024-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

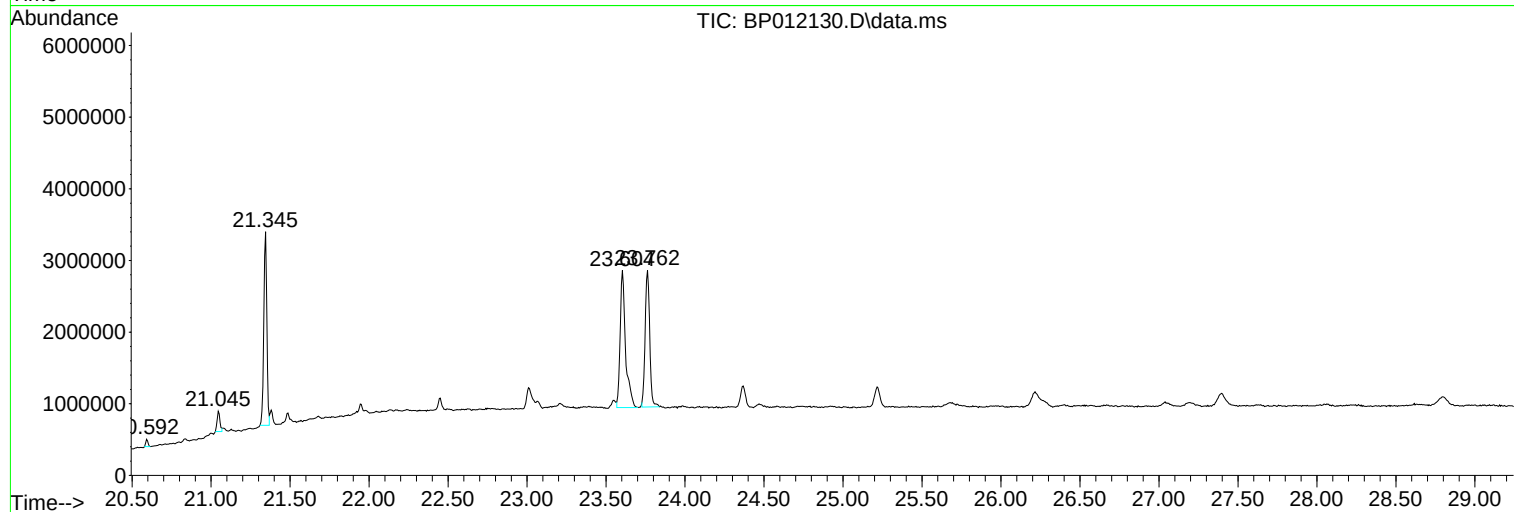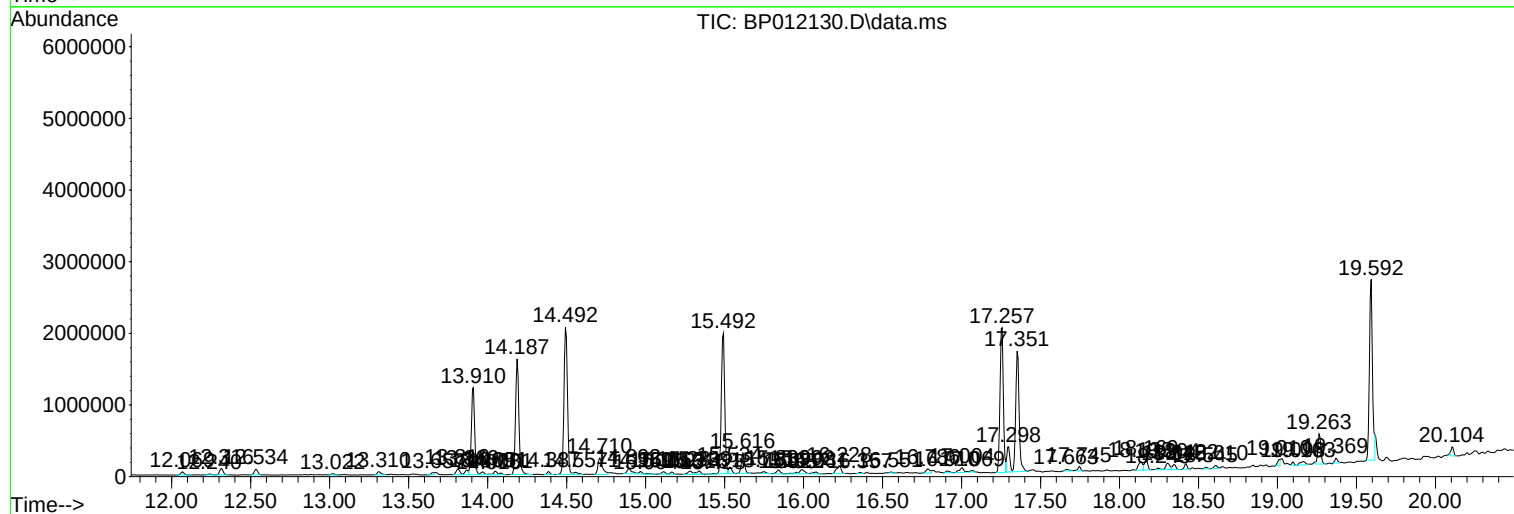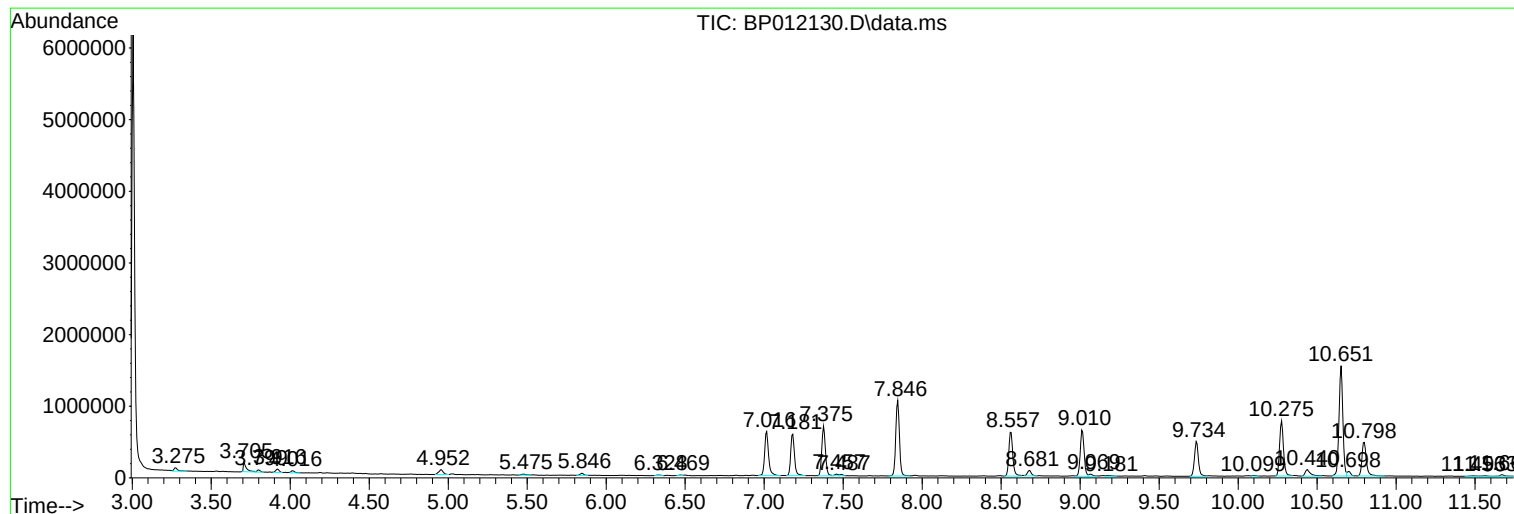

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012130.D
Acq On : 14 Oct 2022 10:40
Operator : CG/JU
Sample : N5024-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012130.D
Acq On : 14 Oct 2022 10:40
Operator : CG/JU
Sample : N5024-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc