

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012133.D
 Acq On : 14 Oct 2022 12:23
 Operator : CG/JU
 Sample : N4982-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	57	rVB	47258	65916	1.15%	0.128%
2	3.705	120	122	132	rBV	190255	285281	4.96%	0.554%
3	3.917	155	158	163	rVB2	21127	30931	0.54%	0.060%
4	4.017	172	175	180	rVB	16697	22508	0.39%	0.044%
5	4.958	330	335	340	rVB2	42221	63180	1.10%	0.123%
6	7.016	679	685	697	rBV	183038	322659	5.61%	0.626%
7	7.181	706	713	730	rBV	637020	1064021	18.50%	2.065%
8	7.375	739	746	757	rBV	641031	1045559	18.18%	2.029%
9	7.846	819	826	836	rBV	856427	1361302	23.67%	2.642%
10	8.563	940	948	969	rBV	492176	863281	15.01%	1.675%
11	9.010	1017	1024	1037	rBV	684448	1202352	20.90%	2.333%
12	9.410	1087	1092	1098	rBV	18376	29980	0.52%	0.058%
13	9.734	1139	1147	1163	rBV	528591	917757	15.96%	1.781%
14	10.275	1231	1239	1256	rBV	791405	1413100	24.57%	2.743%
15	10.652	1295	1303	1320	rVB	1222634	2028585	35.27%	3.937%
16	10.799	1320	1328	1347	rBV	555139	1068565	18.58%	2.074%
17	11.910	1510	1517	1526	rVB3	6673	15366	0.27%	0.030%
18	12.075	1538	1545	1551	rVB7	4997	8245	0.14%	0.016%
19	12.251	1569	1575	1581	rBV2	12213	26132	0.45%	0.051%
20	13.310	1751	1755	1762	rVB	15227	24171	0.42%	0.047%
21	13.469	1777	1782	1787	rVB7	3507	7165	0.12%	0.014%
22	13.904	1850	1856	1872	rBV	1386912	2082318	36.20%	4.041%
23	14.187	1894	1904	1922	rBV	1872710	2787083	48.46%	5.409%
24	14.387	1935	1938	1942	rVB4	5668	7427	0.13%	0.014%
25	14.492	1949	1956	1972	rBV	1731677	2626338	45.66%	5.097%
26	14.716	1988	1994	2012	rBV2	71285	206137	3.58%	0.400%
27	15.492	2119	2126	2140	rBV	2562274	3607643	62.72%	7.002%
28	15.616	2141	2147	2156	rBV	632576	886129	15.41%	1.720%
29	15.734	2162	2167	2171	rBV2	11031	16573	0.29%	0.032%
30	16.281	2257	2260	2265	rVB7	5148	6633	0.12%	0.013%
31	17.257	2419	2426	2436	rBV	2293726	3299099	57.36%	6.403%
32	17.351	2436	2442	2455	rBV	2917519	4128888	71.78%	8.013%
33	18.139	2572	2576	2585	rBV2	64046	103794	1.80%	0.201%
34	18.551	2643	2646	2650	rBV5	14076	17150	0.30%	0.033%
35	19.169	2748	2751	2757	rBV3	37631	48839	0.85%	0.095%
36	19.239	2759	2763	2768	rBV	39423	63229	1.10%	0.123%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012133.D
Acq On : 14 Oct 2022 12:23
Operator : CG/JU
Sample : N4982-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Title : SVOA CALIBRATION

37	19.375	2783	2786	2790	rBV3	48344	64294	1.12%	0.125%
38	19.592	2817	2823	2835	rBV	3958601	5314891	92.40%	10.315%
39	21.045	3067	3070	3074	rBV3	136489	177984	3.09%	0.345%
40	21.345	3116	3121	3132	rBV	3335083	4163805	72.39%	8.081%
41	23.604	3499	3505	3519	rVB2	2790956	5751887	100.00%	11.163%
42	23.763	3526	3532	3541	rVB2	2068857	4299575	74.75%	8.345%




Sum of corrected areas: 51525772

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012133.D
Acq On : 14 Oct 2022 12:23
Operator : CG/JU
Sample : N4982-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

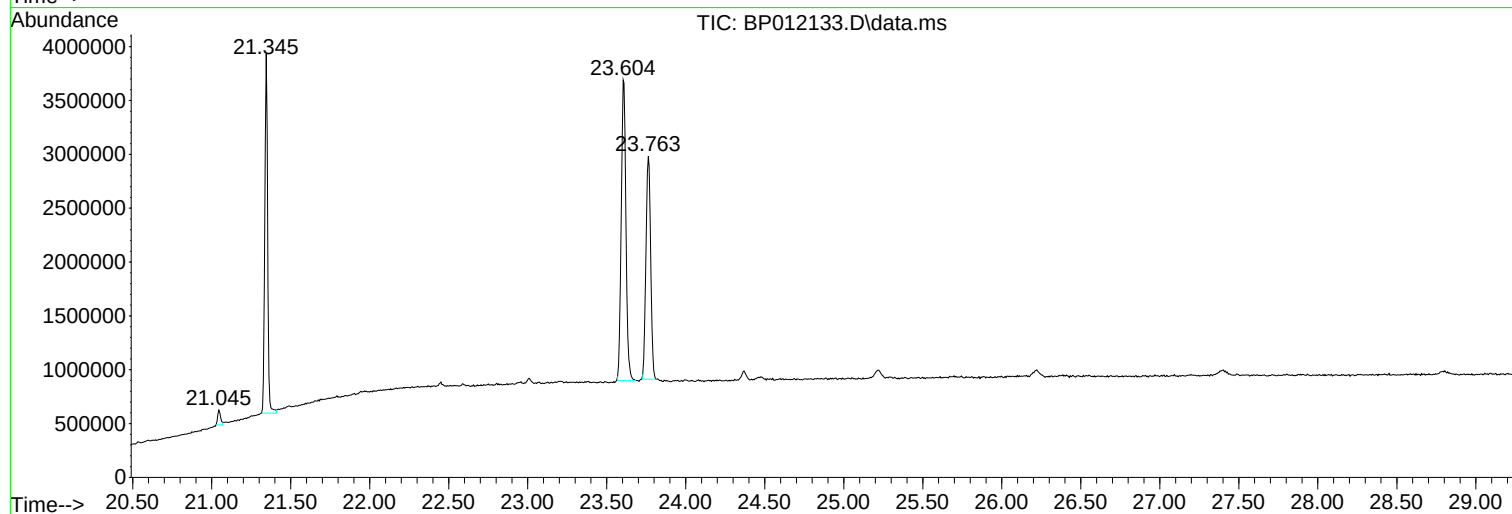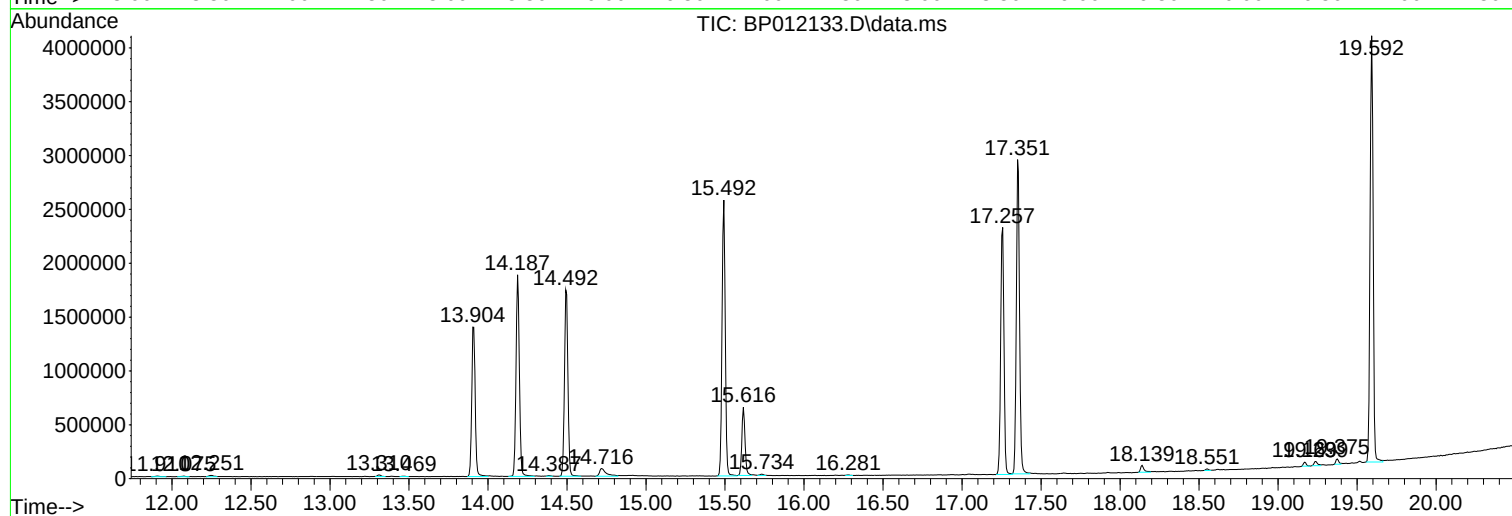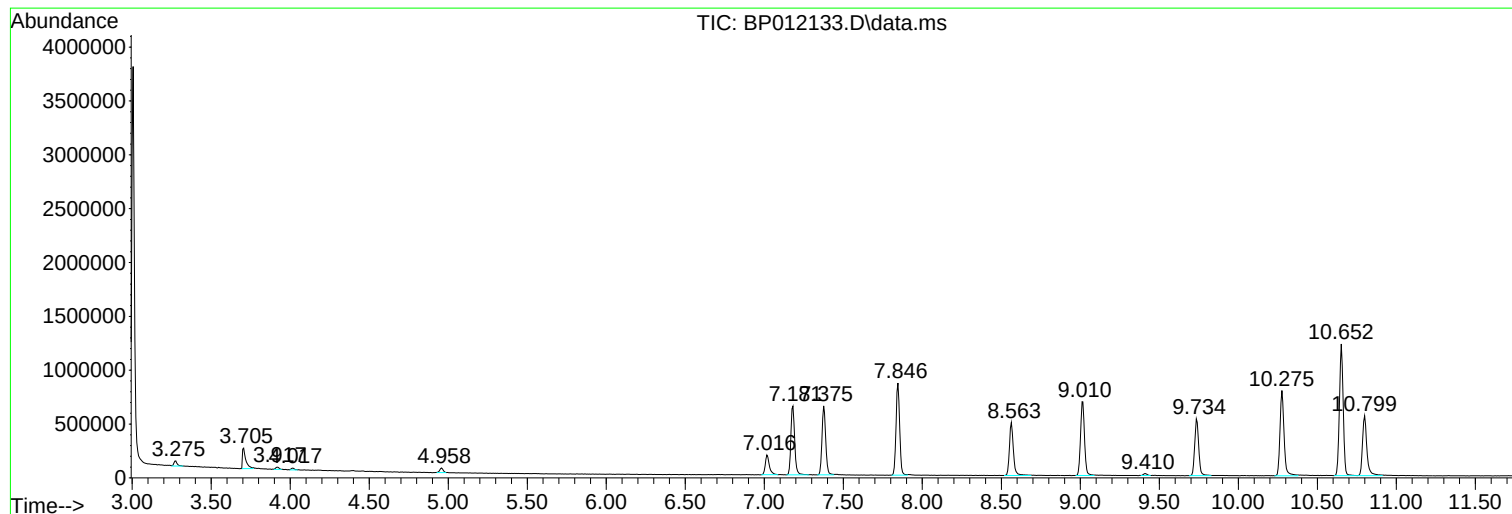

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012133.D
Acq On : 14 Oct 2022 12:23
Operator : CG/JU
Sample : N4982-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012133.D
Acq On : 14 Oct 2022 12:23
Operator : CG/JU
Sample : N4982-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc