

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012135.D
 Acq On : 14 Oct 2022 13:32
 Operator : CG/JU
 Sample : N4982-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	58	rVB	47906	63698	1.16%	0.145%
2	3.705	119	122	134	rBV	137618	212745	3.88%	0.484%
3	4.010	172	174	180	rVB2	16072	21040	0.38%	0.048%
4	4.957	331	335	342	rVB	45246	66162	1.21%	0.151%
5	6.963	671	676	679	rBV3	8243	13921	0.25%	0.032%
6	7.016	679	685	700	rVB	195664	355216	6.48%	0.808%
7	7.181	706	713	727	rBV	782073	1289449	23.54%	2.934%
8	7.375	739	746	758	rBV	746232	1219167	22.26%	2.774%
9	7.846	819	826	835	rBV	638238	1037501	18.94%	2.361%
10	7.928	835	840	850	rVB5	13719	28817	0.53%	0.066%
11	8.563	938	948	967	rBV	494644	876586	16.00%	1.994%
12	9.010	1017	1024	1044	rBV	853346	1454884	26.56%	3.310%
13	9.410	1086	1092	1097	rBV	37548	57535	1.05%	0.131%
14	9.734	1140	1147	1161	rBV	620555	1061760	19.38%	2.416%
15	10.275	1231	1239	1254	rBV	881294	1573215	28.72%	3.579%
16	10.651	1295	1303	1318	rVB	900375	1534380	28.01%	3.491%
17	10.798	1320	1328	1347	rBV	463073	920935	16.81%	2.095%
18	11.645	1468	1472	1474	rBV3	5445	8562	0.16%	0.019%
19	11.910	1508	1517	1522	rBV	19129	32075	0.59%	0.073%
20	12.075	1540	1545	1552	rBV9	5755	11552	0.21%	0.026%
21	12.245	1569	1574	1581	rBV	14437	27326	0.50%	0.062%
22	13.310	1751	1755	1760	rBV3	13420	19805	0.36%	0.045%
23	13.469	1777	1782	1788	rVB8	4087	7269	0.13%	0.017%
24	13.910	1850	1857	1871	rBV	1467871	2142367	39.11%	4.874%
25	14.004	1871	1873	1879	rVB6	4409	7575	0.14%	0.017%
26	14.186	1897	1904	1915	rBV	1937165	2883165	52.63%	6.560%
27	14.386	1935	1938	1942	rVB4	5314	6617	0.12%	0.015%
28	14.492	1950	1956	1965	rBV	1206645	1785313	32.59%	4.062%
29	14.722	1990	1995	2015	rBV	51610	159702	2.92%	0.363%
30	14.910	2025	2027	2036	rVB10	6278	11163	0.20%	0.025%
31	15.492	2119	2126	2140	rBV	2461968	3568008	65.14%	8.118%
32	15.616	2141	2147	2160	rVV	532259	762315	13.92%	1.734%
33	15.733	2163	2167	2172	rVB3	12242	20405	0.37%	0.046%
34	16.274	2257	2259	2263	rVB5	4086	5807	0.11%	0.013%
35	16.580	2307	2311	2317	rVB8	3355	6350	0.12%	0.014%
36	17.257	2419	2426	2436	rBV	1299905	1922672	35.10%	4.374%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012135.D
 Acq On : 14 Oct 2022 13:32
 Operator : CG/JU
 Sample : N4982-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BB1

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	17.357	2436	2443	2458	rVV	2431410	3644974	66.54%	8.293%
38	18.139	2572	2576	2581	rBV	56290	80568	1.47%	0.183%
39	19.168	2748	2751	2758	rBV2	32396	42353	0.77%	0.096%
40	19.239	2760	2763	2769	rVV	31612	47240	0.86%	0.107%
41	19.374	2783	2786	2792	rBV6	37737	59783	1.09%	0.136%
42	19.592	2818	2823	2832	rBV	3668741	4632092	84.56%	10.539%
43	21.345	3117	3121	3127	rBV	1850942	2308648	42.15%	5.253%
44	23.609	3499	3506	3518	rVB2	2678261	5477845	100.00%	12.463%
45	23.762	3527	3532	3540	rVB2	1296467	2483376	45.33%	5.650%




Sum of corrected areas: 43951938

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012135.D
Acq On : 14 Oct 2022 13:32
Operator : CG/JU
Sample : N4982-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

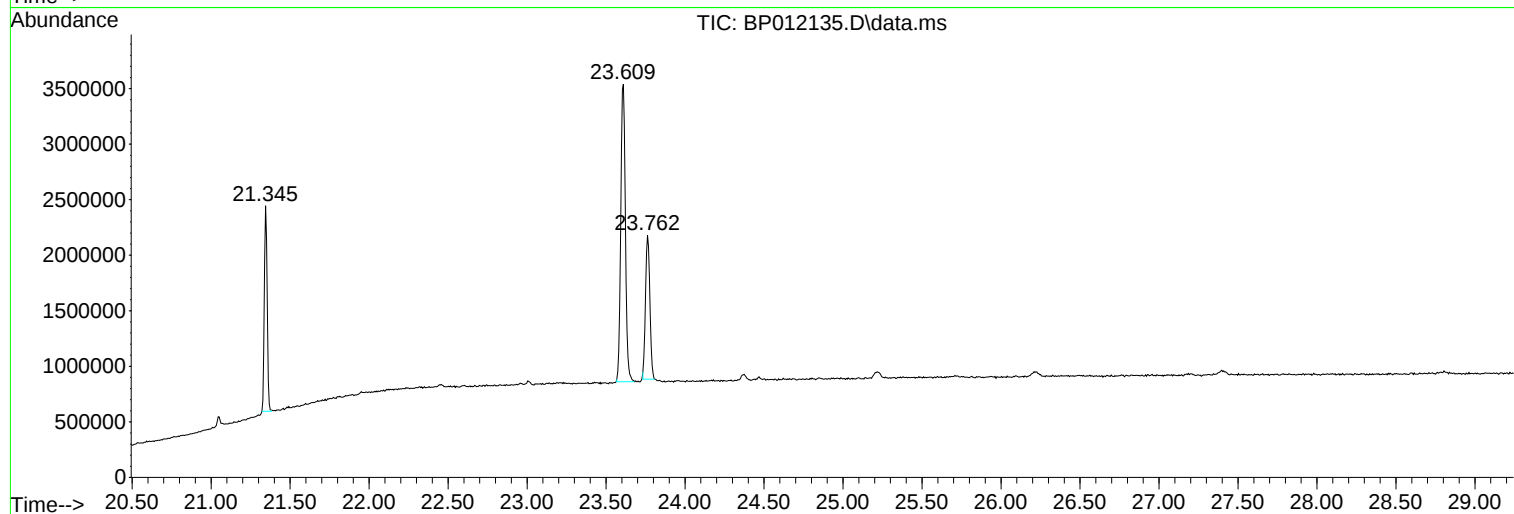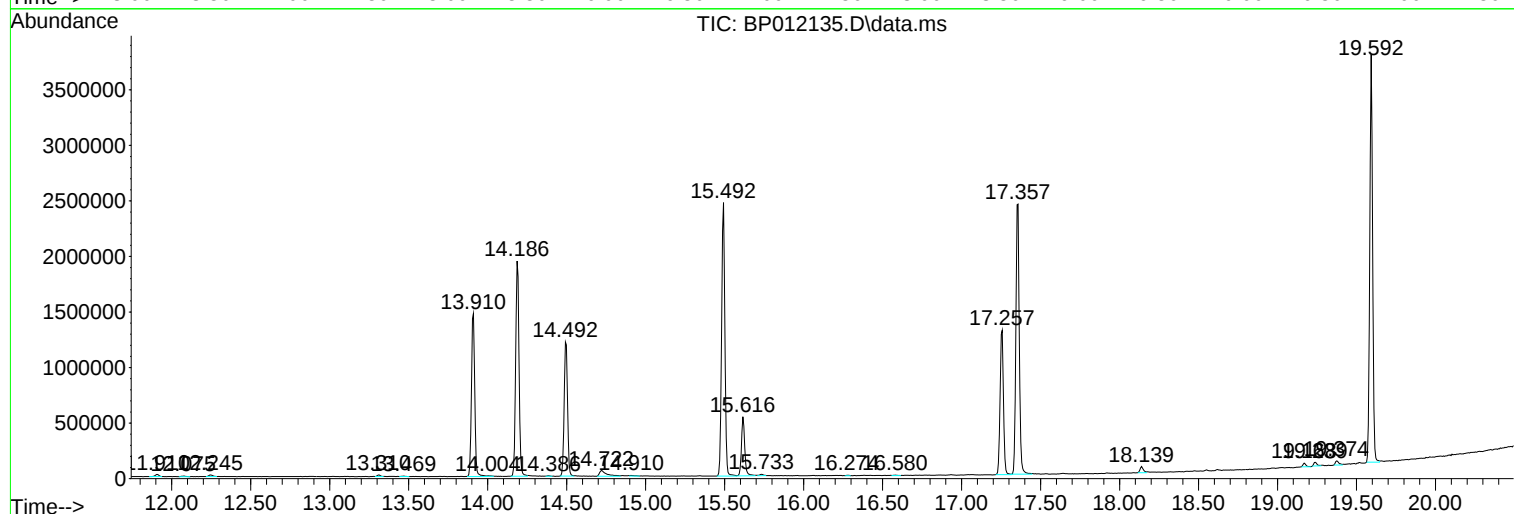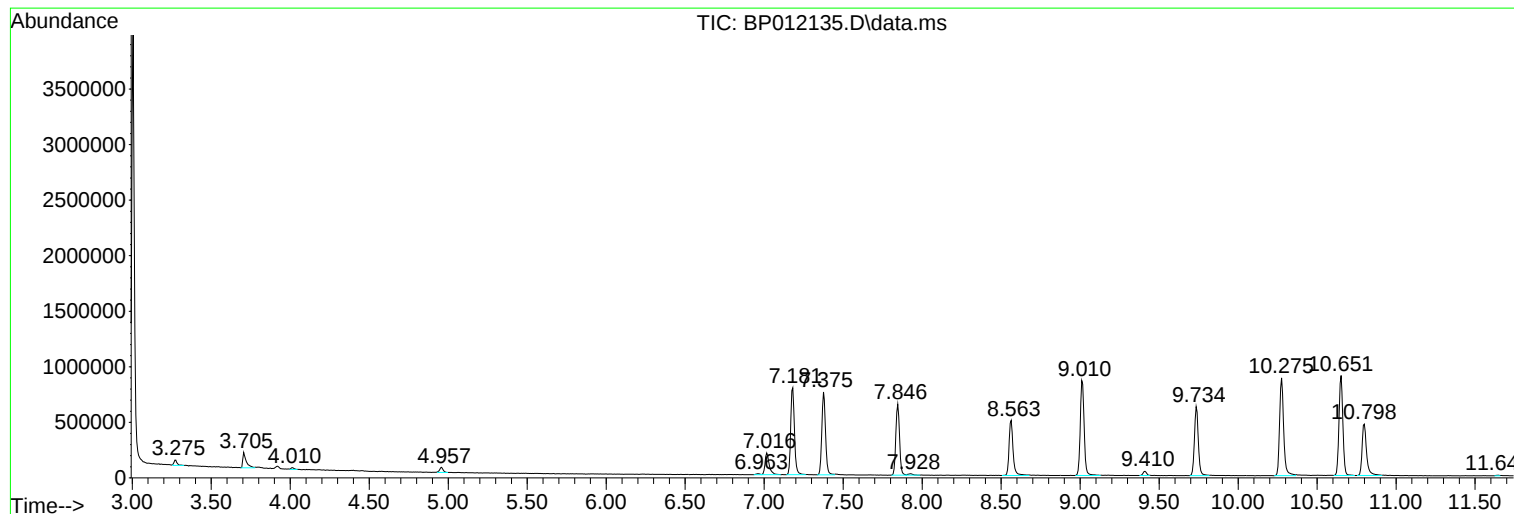

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012135.D
Acq On : 14 Oct 2022 13:32
Operator : CG/JU
Sample : N4982-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012135.D
Acq On : 14 Oct 2022 13:32
Operator : CG/JU
Sample : N4982-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
