

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012136.D
 Acq On : 14 Oct 2022 14:07
 Operator : CG/JU
 Sample : N4982-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	55	rVB	48370	60094	0.89%	0.102%
2	3.705	119	122	137	rBV	175302	266633	3.95%	0.451%
3	4.958	331	335	342	rVB	49601	72571	1.08%	0.123%
4	6.964	672	676	679	rBV	9273	12668	0.19%	0.021%
5	7.016	679	685	696	rVB	223235	395284	5.86%	0.669%
6	7.181	706	713	726	rBV	855492	1421143	21.05%	2.404%
7	7.375	739	746	756	rBV	848963	1351177	20.02%	2.286%
8	7.846	819	826	835	rBV	875592	1432714	21.22%	2.424%
9	8.563	941	948	965	rBV	625543	1084328	16.06%	1.834%
10	9.010	1017	1024	1039	rBV	939930	1628795	24.13%	2.755%
11	9.410	1085	1092	1098	rBV	78471	122483	1.81%	0.207%
12	9.734	1140	1147	1158	rBV	704233	1202311	17.81%	2.034%
13	10.275	1231	1239	1257	rBV	1042814	1845358	27.34%	3.122%
14	10.587	1285	1292	1294	rBV7	4533	8765	0.13%	0.015%
15	10.652	1295	1303	1320	rVB	1228543	2155458	31.93%	3.646%
16	10.799	1320	1328	1347	rBV	724082	1383160	20.49%	2.340%
17	11.910	1509	1517	1522	rBV	43329	68186	1.01%	0.115%
18	12.069	1540	1544	1550	rBV8	6367	9320	0.14%	0.016%
19	12.246	1568	1574	1583	rBV2	17718	35517	0.53%	0.060%
20	13.310	1750	1755	1762	rBV	19924	28790	0.43%	0.049%
21	13.393	1764	1769	1774	rVB8	4473	7184	0.11%	0.012%
22	13.457	1777	1780	1786	rVB7	4859	8480	0.13%	0.014%
23	13.910	1850	1857	1872	rBV	1869259	2706200	40.09%	4.578%
24	14.187	1891	1904	1921	rBV	2491601	3641720	53.95%	6.160%
25	14.387	1934	1938	1942	rVB4	7395	10160	0.15%	0.017%
26	14.493	1949	1956	1974	rBV	1831844	2730095	40.44%	4.618%
27	14.716	1988	1994	2012	rBV2	84590	228492	3.38%	0.387%
28	14.910	2023	2027	2036	rVB10	7094	17970	0.27%	0.030%
29	15.492	2118	2126	2140	rBV	3149064	4563767	67.61%	7.720%
30	15.616	2141	2147	2161	rVV	778964	1093130	16.19%	1.849%
31	15.728	2163	2166	2174	rVB5	14551	26596	0.39%	0.045%
32	17.251	2418	2425	2435	rBV	2224728	3236833	47.95%	5.476%
33	17.351	2436	2442	2459	rVV	3490308	5082908	75.30%	8.598%
34	17.634	2488	2490	2496	rBV7	6583	11573	0.17%	0.020%
35	18.139	2571	2576	2582	rBV	73160	109279	1.62%	0.185%
36	19.169	2747	2751	2757	rBV3	45472	66027	0.98%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012136.D
Acq On : 14 Oct 2022 14:07
Operator : CG/JU
Sample : N4982-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Title : SVOA CALIBRATION

37	19.233	2759	2762	2768	rBV2	45661	72508	1.07%	0.123%
38	19.375	2782	2786	2791	rBV3	50101	78145	1.16%	0.132%
39	19.592	2817	2823	2833	rBV	4702395	6215185	92.07%	10.514%
40	21.345	3116	3121	3130	rBV	2961677	3814200	56.50%	6.452%
41	23.610	3499	3506	3518	rVB2	3315464	6750271	100.00%	11.419%
42	23.763	3526	3532	3542	rVB2	2025042	4059119	60.13%	6.867%




Sum of corrected areas: 59114597

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012136.D
Acq On : 14 Oct 2022 14:07
Operator : CG/JU
Sample : N4982-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

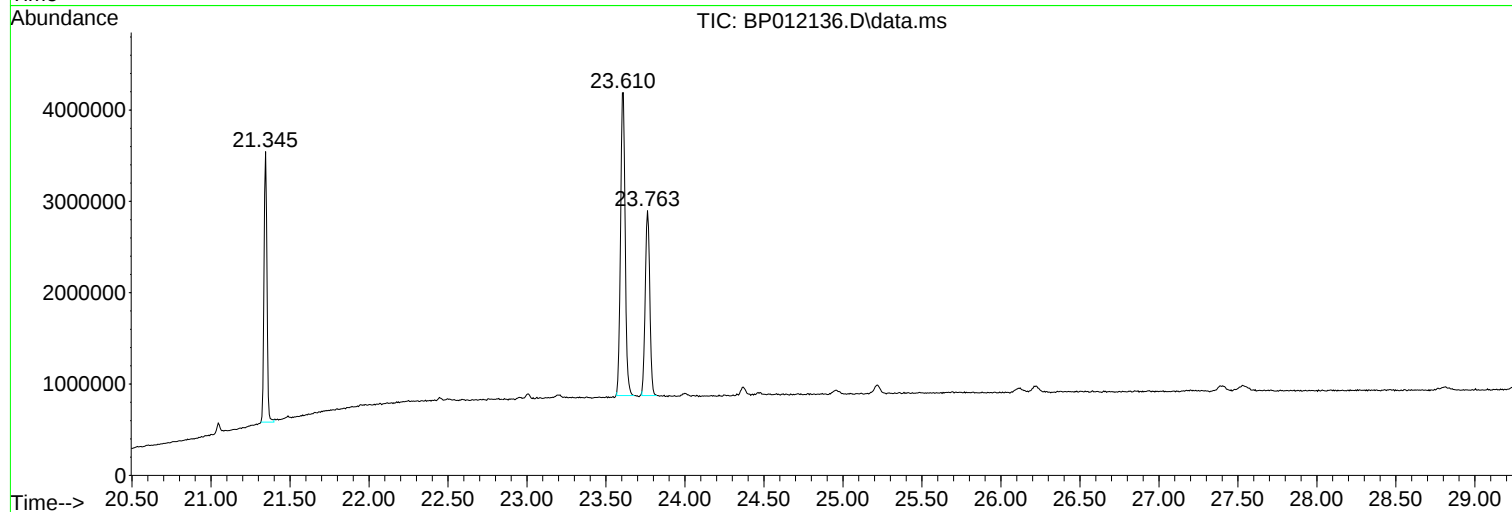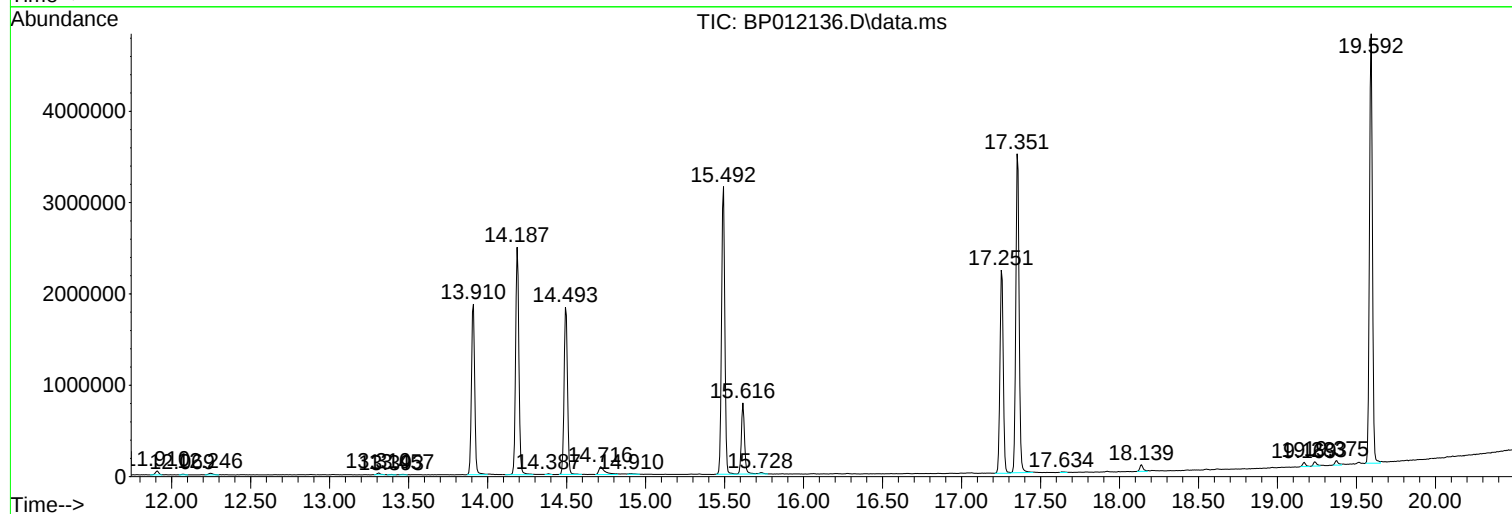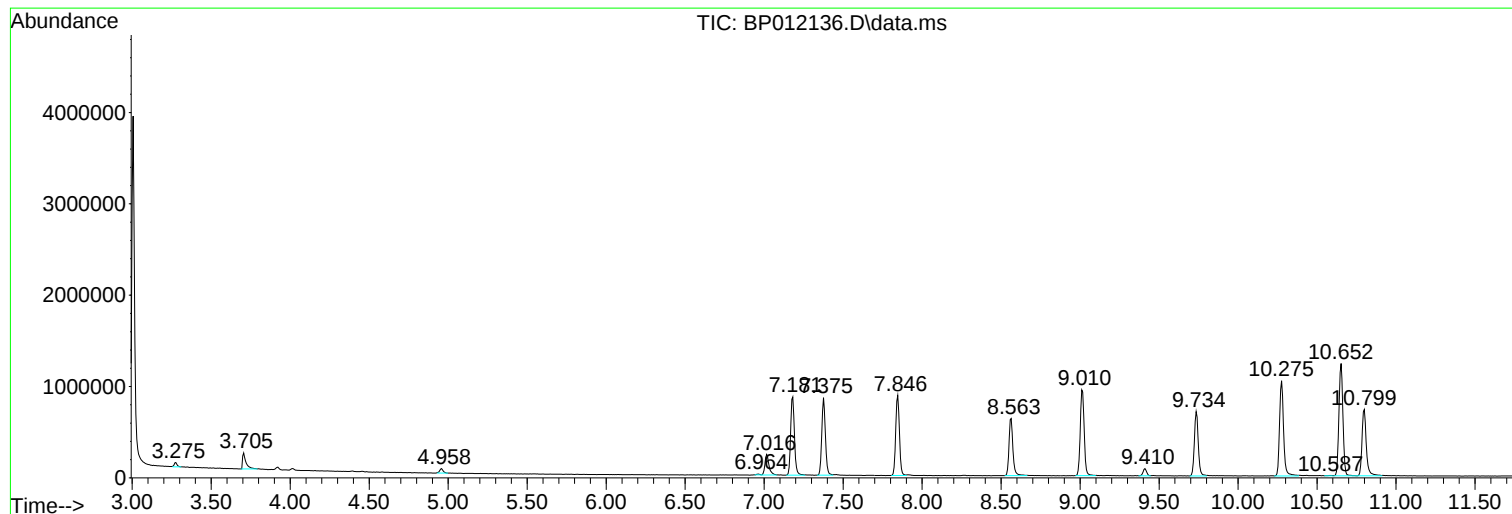

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012136.D
Acq On : 14 Oct 2022 14:07
Operator : CG/JU
Sample : N4982-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012136.D
Acq On : 14 Oct 2022 14:07
Operator : CG/JU
Sample : N4982-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
