

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012137.D
 Acq On : 14 Oct 2022 14:41
 Operator : CG/JU
 Sample : N4982-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	45	48	57	rVB2	51106	73671	1.07%	0.126%
2	3.705	120	122	131	rBV	170632	257758	3.75%	0.440%
3	3.917	155	158	165	rVB2	32566	50035	0.73%	0.085%
4	4.017	172	175	181	rVB2	20946	27337	0.40%	0.047%
5	7.016	679	685	698	rVB	242965	419648	6.10%	0.716%
6	7.181	706	713	727	rBV	886615	1471781	21.39%	2.512%
7	7.375	739	746	757	rBV	874187	1413732	20.55%	2.413%
8	7.846	818	826	835	rBV	887361	1421564	20.66%	2.426%
9	7.910	835	837	842	rVB4	6093	9430	0.14%	0.016%
10	8.563	939	948	963	rBV	652432	1144467	16.64%	1.953%
11	9.010	1016	1024	1039	rBV	955787	1669668	24.27%	2.850%
12	9.410	1086	1092	1098	rVB2	21378	33390	0.49%	0.057%
13	9.734	1140	1147	1161	rBV	726910	1239235	18.01%	2.115%
14	10.275	1232	1239	1261	rBV	1076041	1903835	27.67%	3.249%
15	10.652	1295	1303	1318	rVB	1223896	2091650	30.40%	3.570%
16	10.799	1320	1328	1348	rBV	705108	1354690	19.69%	2.312%
17	11.904	1511	1516	1524	rVB2	8515	15557	0.23%	0.027%
18	12.069	1540	1544	1550	rBV6	6915	11166	0.16%	0.019%
19	12.246	1568	1574	1582	rBV2	17724	35175	0.51%	0.060%
20	13.022	1701	1706	1711	rVB9	4777	7233	0.11%	0.012%
21	13.310	1745	1755	1764	rBV	21288	39745	0.58%	0.068%
22	13.398	1764	1770	1773	rVV7	4054	7608	0.11%	0.013%
23	13.463	1777	1781	1785	rVB6	4132	8093	0.12%	0.014%
24	13.910	1849	1857	1871	rBV	1821458	2648862	38.50%	4.521%
25	14.004	1871	1873	1885	rVB	6695	15748	0.23%	0.027%
26	14.187	1897	1904	1917	rBV	2382150	3544648	51.52%	6.050%
27	14.387	1932	1938	1943	rVB7	6563	10290	0.15%	0.018%
28	14.492	1948	1956	1968	rBV	1705009	2585214	37.58%	4.412%
29	14.716	1988	1994	2005	rBV2	90487	218372	3.17%	0.373%
30	14.910	2024	2027	2035	rVB10	6056	14807	0.22%	0.025%
31	15.492	2118	2126	2140	rBV	3180771	4462351	64.86%	7.616%
32	15.616	2141	2147	2158	rVV	756856	1081641	15.72%	1.846%
33	15.734	2162	2167	2172	rVB3	15140	28192	0.41%	0.048%
34	16.281	2256	2260	2263	rBV6	5222	7148	0.10%	0.012%
35	17.257	2419	2426	2436	rBV	2056025	3035149	44.12%	5.180%
36	17.357	2436	2443	2458	rVV	3346991	4938563	71.78%	8.429%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012137.D
 Acq On : 14 Oct 2022 14:41
 Operator : CG/JU
 Sample : N4982-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

37	17.922	2537	2539	2544	rVB4	8059	7935	0.12%	0.014%
38	18.139	2572	2576	2585	rBV3	62701	101148	1.47%	0.173%
39	19.169	2748	2751	2756	rVB2	39943	51808	0.75%	0.088%
40	19.233	2759	2762	2768	rBV	43422	65924	0.96%	0.113%
41	19.375	2783	2786	2790	rBV2	48022	60856	0.88%	0.104%
42	19.592	2817	2823	2834	rBV	4779543	6184575	89.90%	10.556%
43	21.045	3067	3070	3074	rBV2	147724	203666	2.96%	0.348%
44	21.345	3116	3121	3130	rBV	2985985	3773324	54.85%	6.440%
45	23.610	3499	3506	3517	rVB2	3411235	6879756	100.00%	11.742%
46	23.763	3526	3532	3541	rVB2	1948085	3962384	57.59%	6.763%




Sum of corrected areas: 58588829

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP0101422\
Data File : BP012137.D
Acq On : 14 Oct 2022 14:41
Operator : CG/JU
Sample : N4982-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

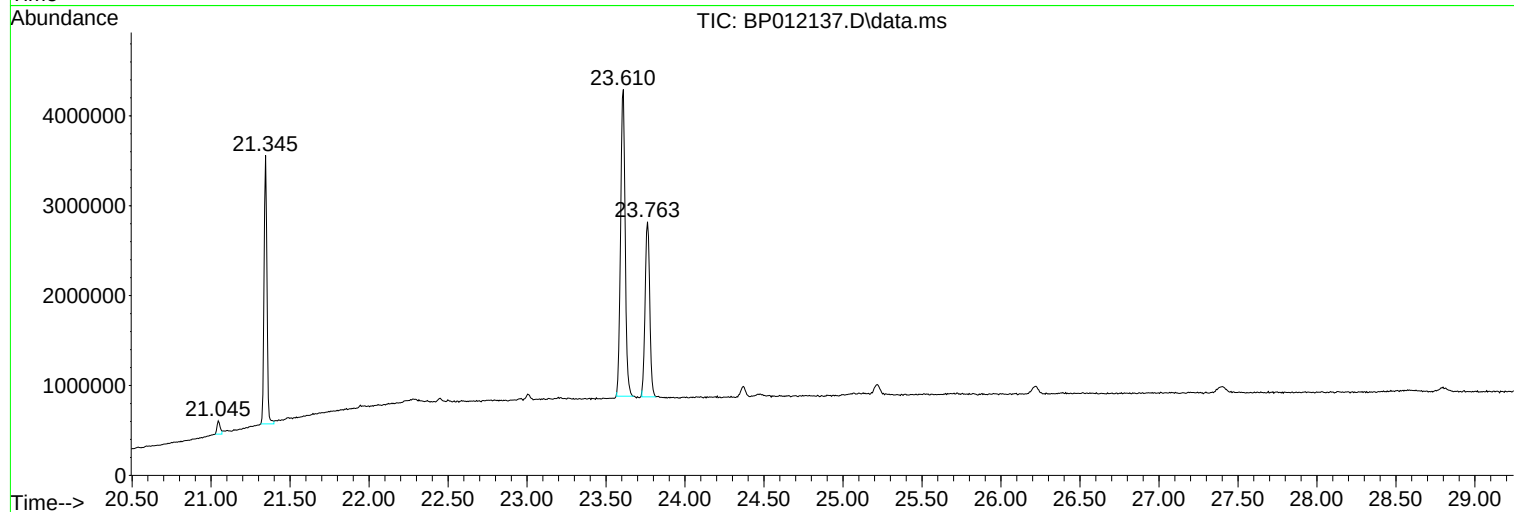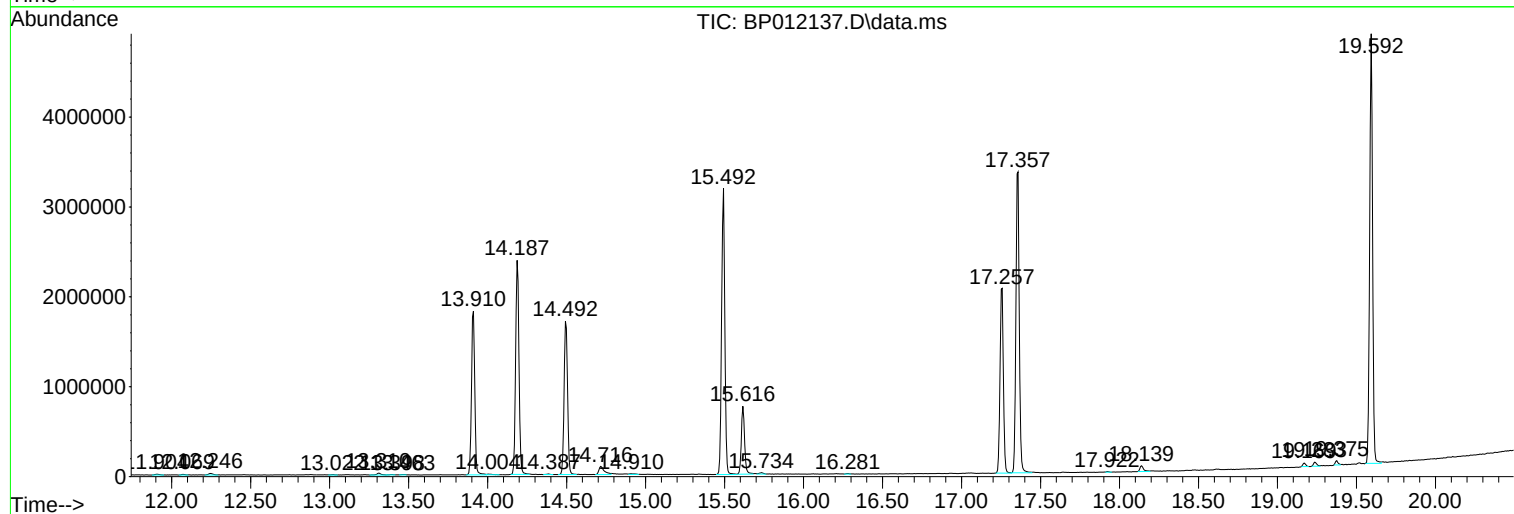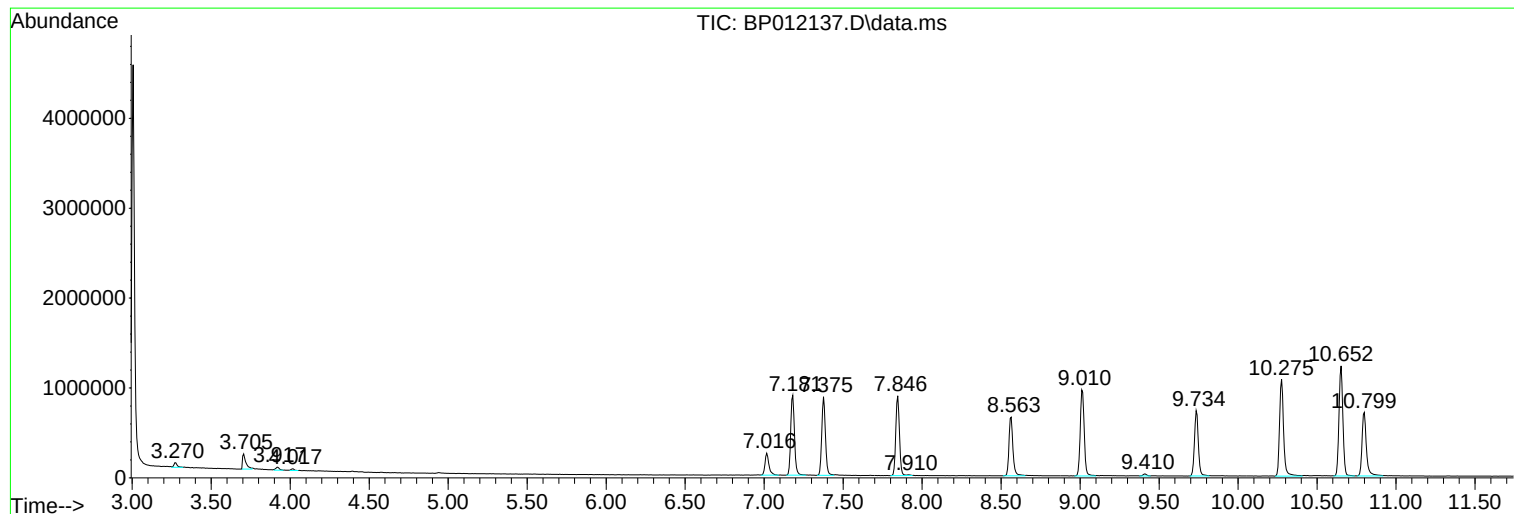

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012137.D
Acq On : 14 Oct 2022 14:41
Operator : CG/JU
Sample : N4982-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012137.D
Acq On : 14 Oct 2022 14:41
Operator : CG/JU
Sample : N4982-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
