

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012140.D
 Acq On : 14 Oct 2022 16:25
 Operator : CG/JU
 Sample : N4982-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	46	49	53	rVB	46573	51925	0.72%	0.087%
2	3.699	119	121	136	rBV	254367	389384	5.40%	0.653%
3	4.017	172	175	180	rVB	42426	55430	0.77%	0.093%
4	4.958	330	335	344	rVB	81691	126468	1.75%	0.212%
5	6.964	671	676	680	rBV	22978	34064	0.47%	0.057%
6	7.017	680	685	698	rVB	254978	433294	6.01%	0.727%
7	7.181	706	713	730	rBV	910564	1514830	21.00%	2.542%
8	7.375	739	746	757	rBV	906610	1473796	20.43%	2.473%
9	7.458	757	760	769	rVB10	8377	15031	0.21%	0.025%
10	7.846	818	826	835	rBV	851939	1379781	19.13%	2.315%
11	8.563	941	948	965	rBV	659696	1164979	16.15%	1.955%
12	9.011	1016	1024	1040	rBV	1011977	1721989	23.88%	2.890%
13	9.411	1087	1092	1100	rVB	47503	75134	1.04%	0.126%
14	9.734	1140	1147	1162	rBV	758039	1286364	17.84%	2.159%
15	10.275	1230	1239	1261	rBV	1082369	1946156	26.98%	3.266%
16	10.587	1286	1292	1295	rBV4	4857	8706	0.12%	0.015%
17	10.652	1295	1303	1318	rVB	1210601	2028853	28.13%	3.405%
18	10.799	1321	1328	1344	rBV	717093	1366403	18.95%	2.293%
19	11.910	1511	1517	1523	rVB	26538	44358	0.62%	0.074%
20	12.069	1540	1544	1549	rBV8	4834	7469	0.10%	0.013%
21	12.252	1568	1575	1582	rBV	15897	32622	0.45%	0.055%
22	13.310	1748	1755	1764	rBV2	12363	22466	0.31%	0.038%
23	13.463	1775	1781	1788	rVB7	5502	9972	0.14%	0.017%
24	13.904	1849	1856	1871	rBV	1860887	2704427	37.50%	4.538%
25	14.004	1871	1873	1878	rVB6	4630	7273	0.10%	0.012%
26	14.187	1892	1904	1923	rBV	2438940	3623839	50.25%	6.081%
27	14.493	1949	1956	1974	rBV	1652866	2464961	34.18%	4.137%
28	14.716	1987	1994	2014	rBV	98652	269234	3.73%	0.452%
29	14.922	2023	2029	2034	rVB10	7621	17103	0.24%	0.029%
30	15.493	2118	2126	2140	rBV	3082375	4531475	62.83%	7.604%
31	15.616	2140	2147	2160	rVV	813164	1152673	15.98%	1.934%
32	15.728	2163	2166	2175	rVB4	14813	27918	0.39%	0.047%
33	17.251	2418	2425	2436	rBV	1964642	2905043	40.28%	4.875%
34	17.357	2436	2443	2458	rVV	3510525	5136252	71.22%	8.619%
35	18.139	2571	2576	2584	rBV	107225	169182	2.35%	0.284%
36	19.169	2747	2751	2757	rBV3	45103	66124	0.92%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012140.D
Acq On : 14 Oct 2022 16:25
Operator : CG/JU
Sample : N4982-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BC0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Title : SVOA CALIBRATION

37	19.239	2759	2763	2769	rBV2	51650	84544	1.17%	0.142%
38	19.375	2782	2786	2793	rBV2	104361	162455	2.25%	0.273%
39	19.592	2817	2823	2835	rBV	5028500	6460283	89.57%	10.841%
40	21.345	3116	3121	3128	rBV	2882074	3578609	49.62%	6.005%
41	23.610	3499	3506	3520	rVB2	3605029	7212249	100.00%	12.103%
42	23.763	3526	3532	3549	rVB2	1836534	3826324	53.05%	6.421%




Sum of corrected areas: 59589442

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP0121422\
Data File : BP012140.D
Acq On : 14 Oct 2022 16:25
Operator : CG/JU
Sample : N4982-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

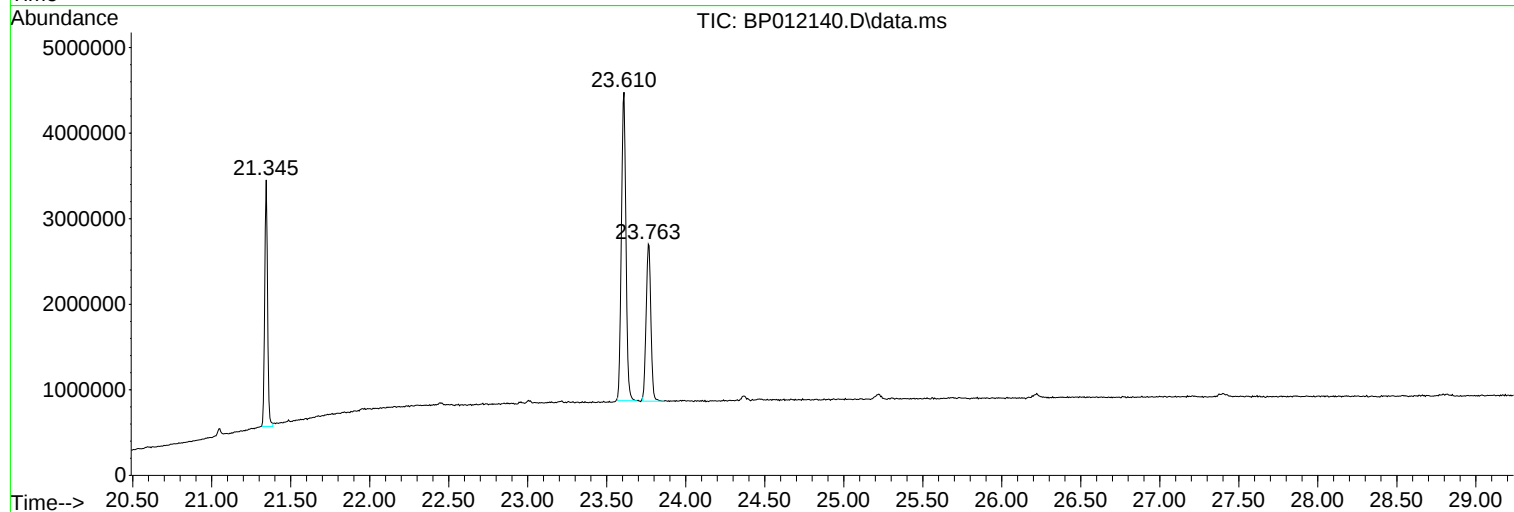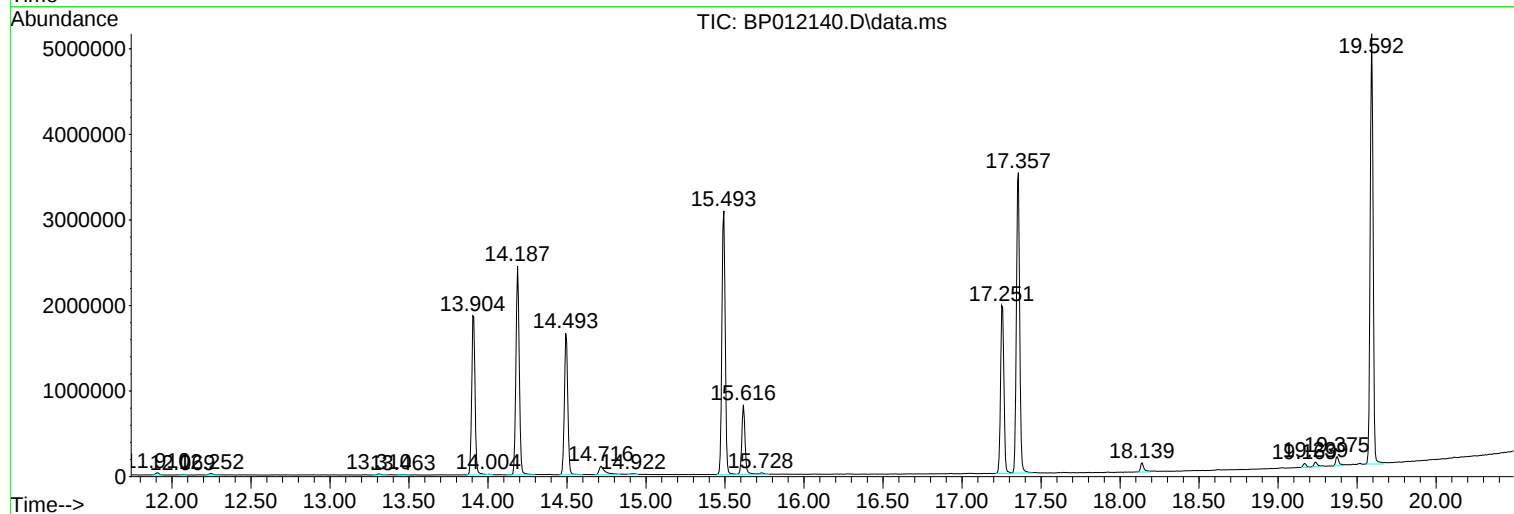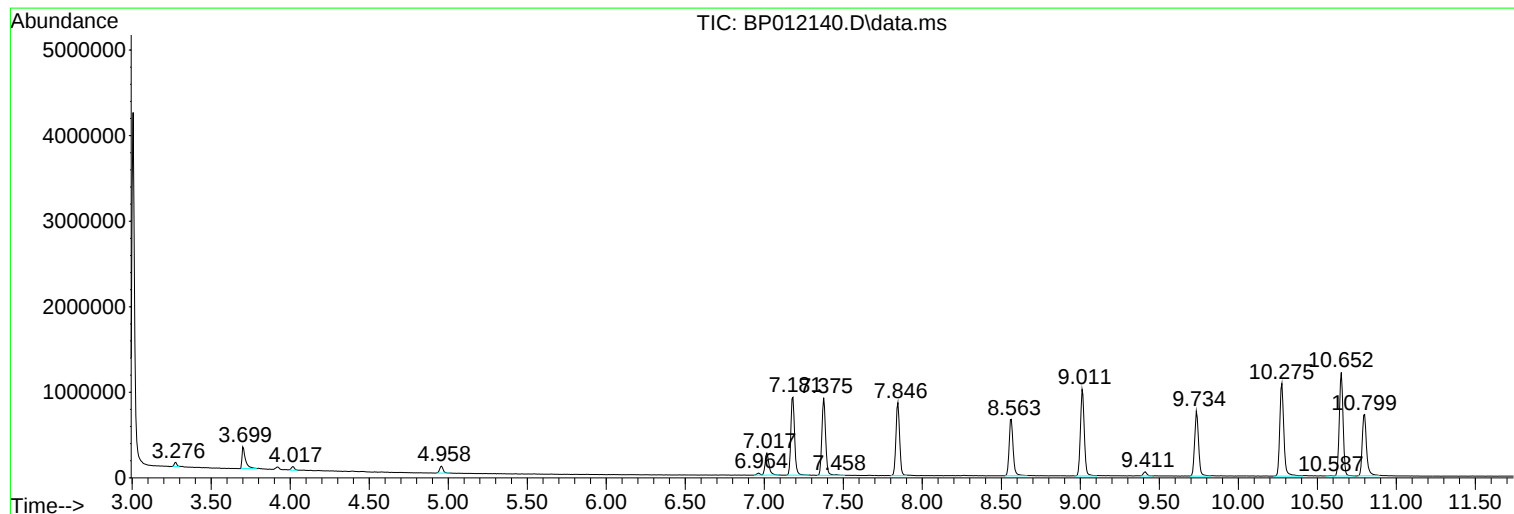

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012140.D
Acq On : 14 Oct 2022 16:25
Operator : CG/JU
Sample : N4982-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012140.D
Acq On : 14 Oct 2022 16:25
Operator : CG/JU
Sample : N4982-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
