

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012145.D
 Acq On : 14 Oct 2022 19:53
 Operator : CG/JU
 Sample : PB148236BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	46	48	54	rVB	50728	56668	1.05%	0.100%
2	3.693	117	120	141	rBV	652016	987133	18.35%	1.734%
3	7.011	678	684	703	rVV	957827	1563125	29.06%	2.746%
4	7.175	706	712	732	rVB	817524	1340395	24.92%	2.355%
5	7.375	739	746	764	rBV	1003816	1623013	30.18%	2.851%
6	7.840	818	825	836	rBV	945448	1531126	28.47%	2.690%
7	8.558	940	947	963	rBV	1180165	1939361	36.06%	3.407%
8	9.010	1017	1024	1038	rBV	890577	1494369	27.78%	2.625%
9	9.734	1138	1147	1162	rBV	698102	1169453	21.74%	2.055%
10	10.269	1230	1238	1256	rBV	1011014	1841921	34.25%	3.236%
11	10.646	1292	1302	1315	rBV	1322127	2305184	42.86%	4.050%
12	10.793	1318	1327	1352	rBV	1029506	1932537	35.93%	3.395%
13	12.246	1568	1574	1587	rBV4	13788	35579	0.66%	0.063%
14	13.904	1849	1856	1869	rBV	1568041	2274475	42.29%	3.996%
15	14.187	1894	1904	1916	rBV	2117125	3137140	58.33%	5.512%
16	14.492	1948	1956	1968	rBV	1883307	2761280	51.34%	4.851%
17	14.704	1986	1992	2015	rBV	535413	1037058	19.28%	1.822%
18	15.487	2118	2125	2137	rBV	2605744	3759820	69.90%	6.606%
19	15.616	2141	2147	2161	rVV	573789	840874	15.63%	1.477%
20	15.728	2162	2166	2171	rVB4	10564	17948	0.33%	0.032%
21	16.063	2218	2223	2227	rBV8	2998	7136	0.13%	0.013%
22	17.039	2385	2389	2394	rBV4	4769	8227	0.15%	0.014%
23	17.251	2419	2425	2435	rBV	2203973	3101404	57.66%	5.449%
24	17.351	2435	2442	2459	rVV	2779577	3993553	74.25%	7.016%
25	19.169	2747	2751	2756	rBV4	33661	49717	0.92%	0.087%
26	19.233	2759	2762	2768	rVV	31744	49076	0.91%	0.086%
27	19.592	2817	2823	2833	rBV	3639304	4911124	91.31%	8.628%
28	21.345	3116	3121	3129	rBV	2888603	3772293	70.14%	6.628%
29	23.604	3498	3505	3519	rVB2	2640594	5378565	100.00%	9.450%
30	23.763	3525	3532	3543	rVB2	1929208	3998744	74.35%	7.025%




Sum of corrected areas: 56918298

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012145.D
Acq On : 14 Oct 2022 19:53
Operator : CG/JU
Sample : PB148236BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

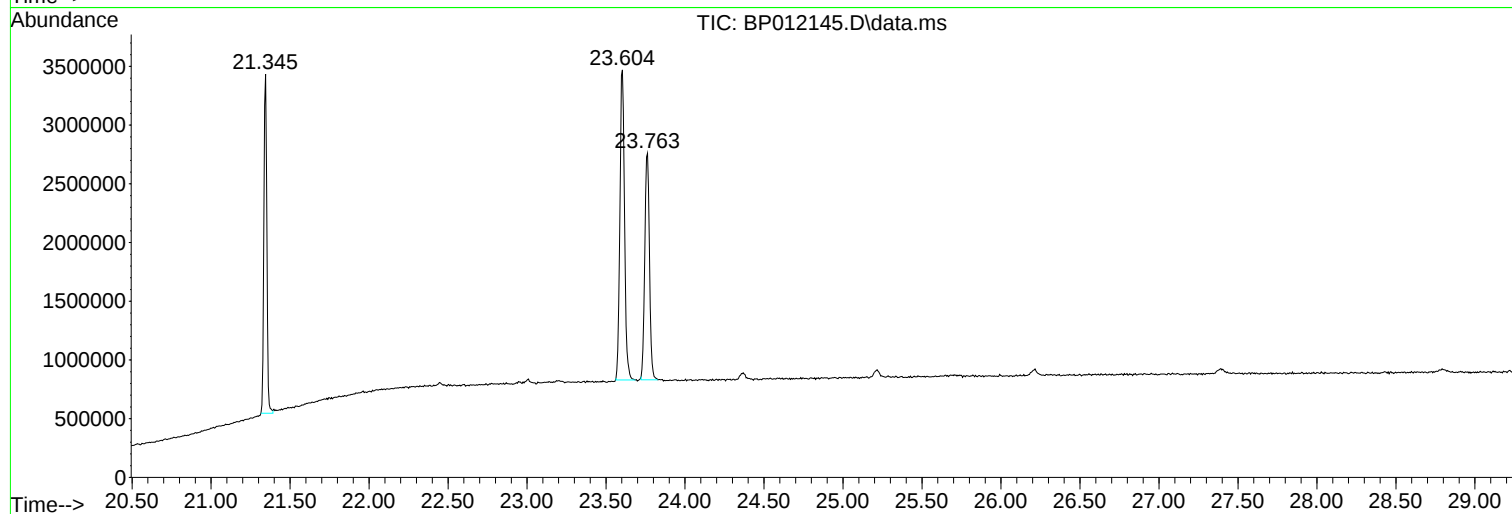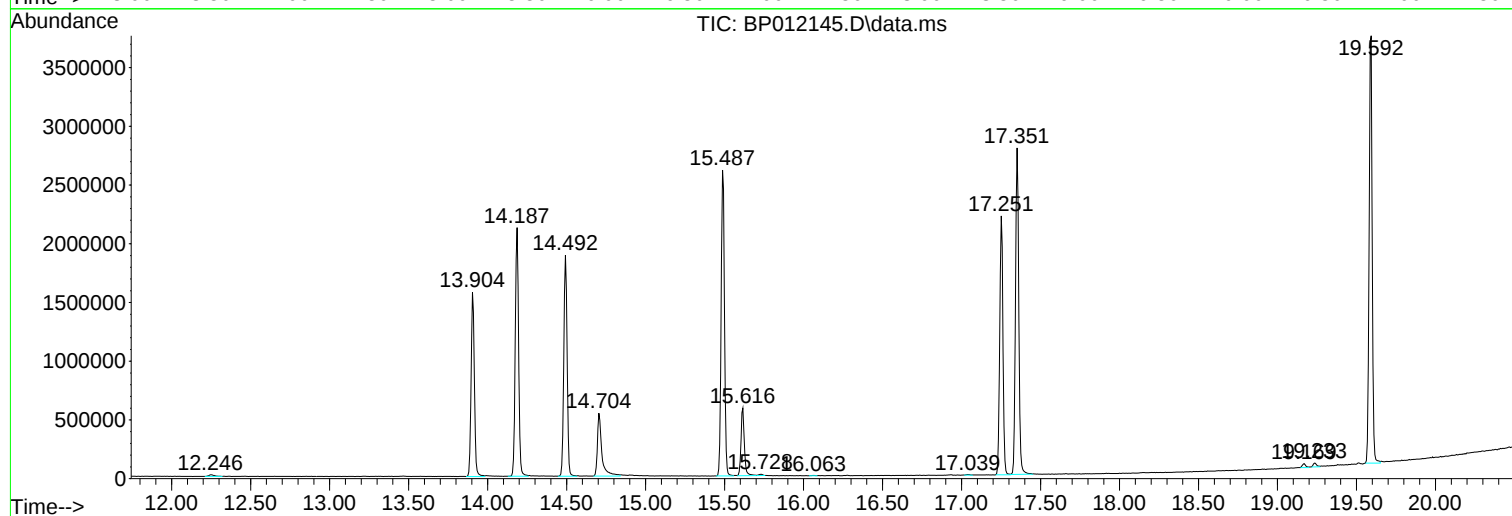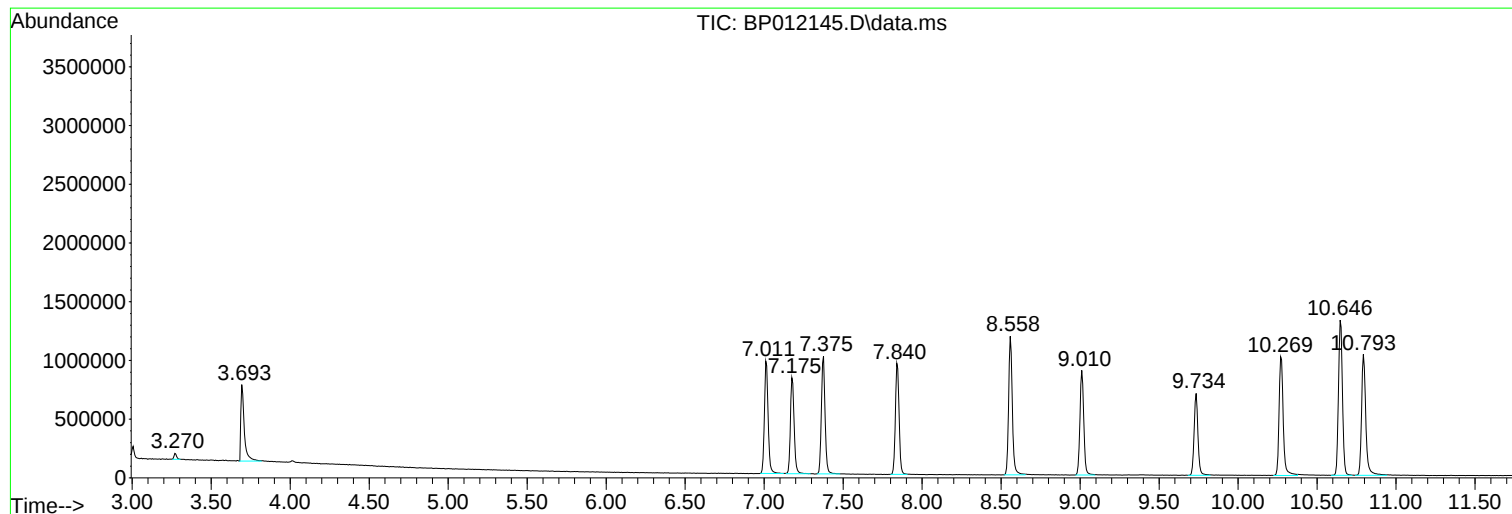

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012145.D
Acq On : 14 Oct 2022 19:53
Operator : CG/JU
Sample : PB148236BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012145.D
Acq On : 14 Oct 2022 19:53
Operator : CG/JU
Sample : PB148236BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc