

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
 Data File : BP012146.D
 Acq On : 14 Oct 2022 20:27
 Operator : CG/JU
 Sample : PB148313BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK313

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	46	48	54	rVB	42862	52070	0.98%	0.097%
2	3.693	118	120	138	rBV	560789	847172	15.95%	1.580%
3	7.010	678	684	700	rBV	897994	1475411	27.77%	2.751%
4	7.175	706	712	729	rVB	783913	1254899	23.62%	2.340%
5	7.375	739	746	758	rBV	919912	1500698	28.25%	2.798%
6	7.840	819	825	836	rBV	915046	1501416	28.26%	2.799%
7	8.557	939	947	965	rBV	1081764	1814703	34.16%	3.383%
8	9.010	1017	1024	1043	rBV	834205	1402977	26.41%	2.616%
9	9.734	1138	1147	1159	rBV	619622	1073669	20.21%	2.002%
10	10.269	1231	1238	1260	rBV	965732	1710670	32.20%	3.189%
11	10.646	1294	1302	1314	rBV	1273663	2136416	40.21%	3.983%
12	10.793	1320	1327	1347	rBV	939169	1714848	32.28%	3.197%
13	12.251	1567	1575	1586	rBV3	11896	30330	0.57%	0.057%
14	12.457	1605	1610	1615	rBV9	3116	6756	0.13%	0.013%
15	13.904	1850	1856	1870	rBV	1527349	2146088	40.39%	4.001%
16	14.187	1897	1904	1920	rBV	1971440	2914884	54.86%	5.435%
17	14.492	1949	1956	1968	rBV	1710469	2547756	47.95%	4.750%
18	14.704	1985	1992	2024	rBV	503563	1039214	19.56%	1.938%
19	15.487	2116	2125	2139	rBV	2448119	3565487	67.11%	6.648%
20	15.616	2141	2147	2156	rBV	538802	787370	14.82%	1.468%
21	15.728	2163	2166	2173	rVB6	11913	16704	0.31%	0.031%
22	17.039	2386	2389	2395	rVB6	3973	6207	0.12%	0.012%
23	17.251	2418	2425	2435	rBV	2022122	2856868	53.77%	5.326%
24	17.351	2435	2442	2461	rVV	2746802	3939572	74.15%	7.345%
25	19.169	2747	2751	2756	rBV4	30608	47038	0.89%	0.088%
26	19.233	2760	2762	2769	rVB2	28186	36730	0.69%	0.068%
27	19.586	2817	2822	2832	rBV	3522226	4755349	89.51%	8.866%
28	21.339	3116	3120	3129	rBV	2579156	3469112	65.30%	6.468%
29	23.598	3498	3504	3517	rVB2	2598231	5312880	100.00%	9.906%
30	23.757	3525	3531	3543	rVB2	1861458	3671917	69.11%	6.846%




Sum of corrected areas: 53635211

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP0121422\
Data File : BP012146.D
Acq On : 14 Oct 2022 20:27
Operator : CG/JU
Sample : PB148313BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK313

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

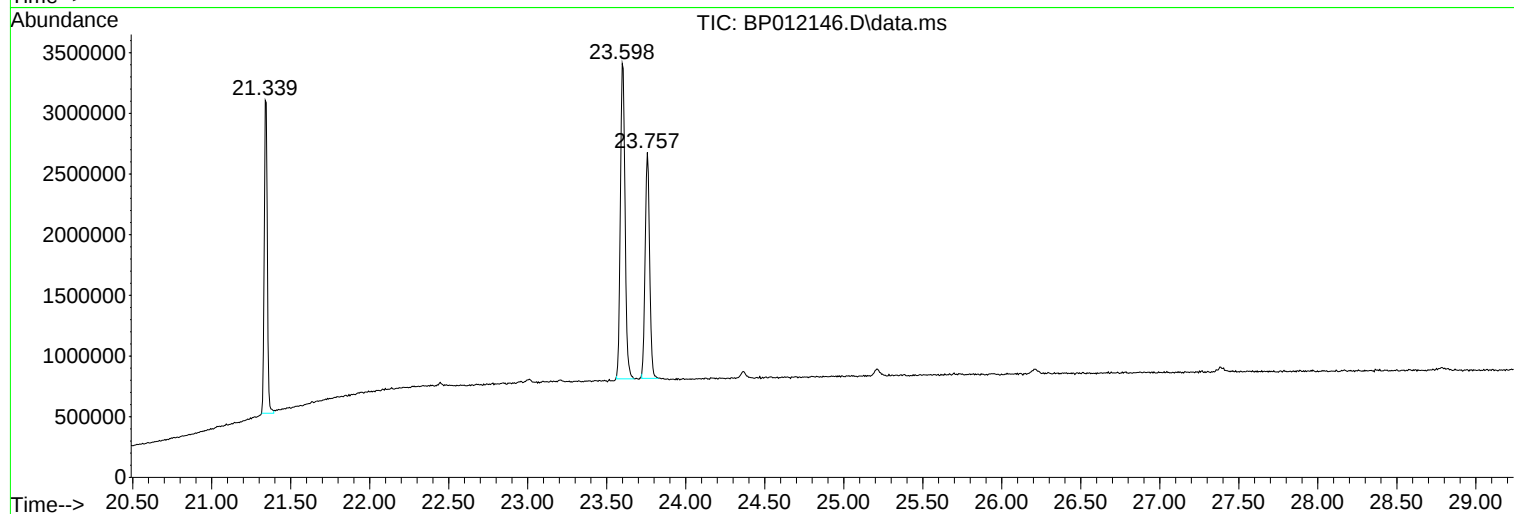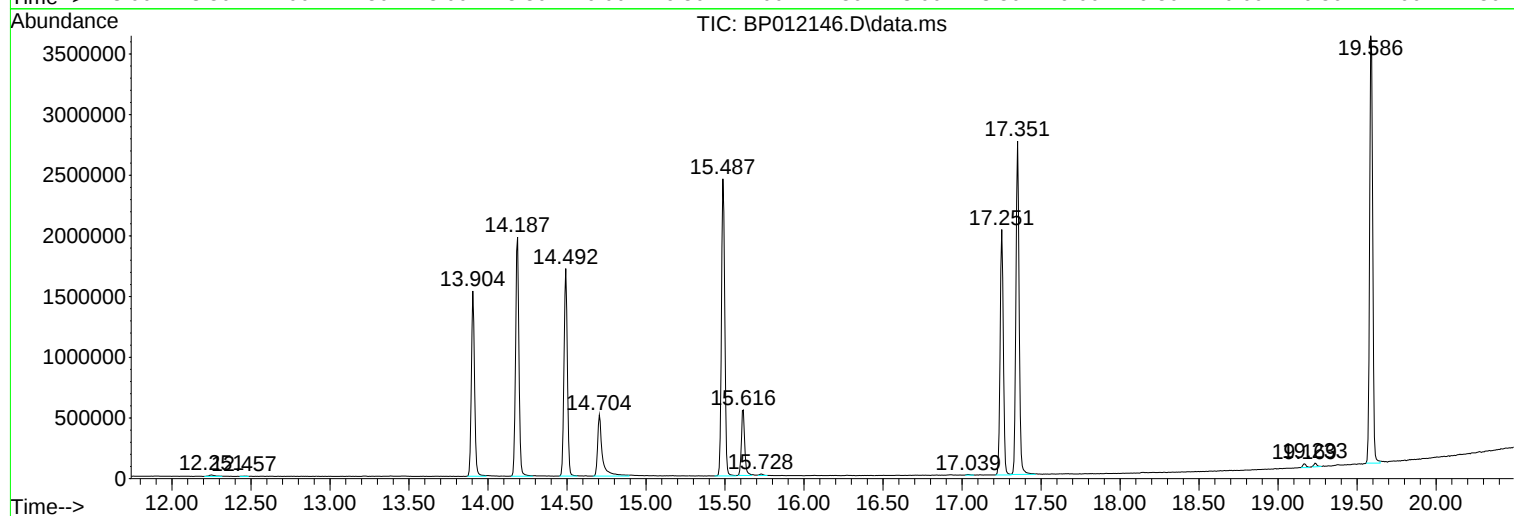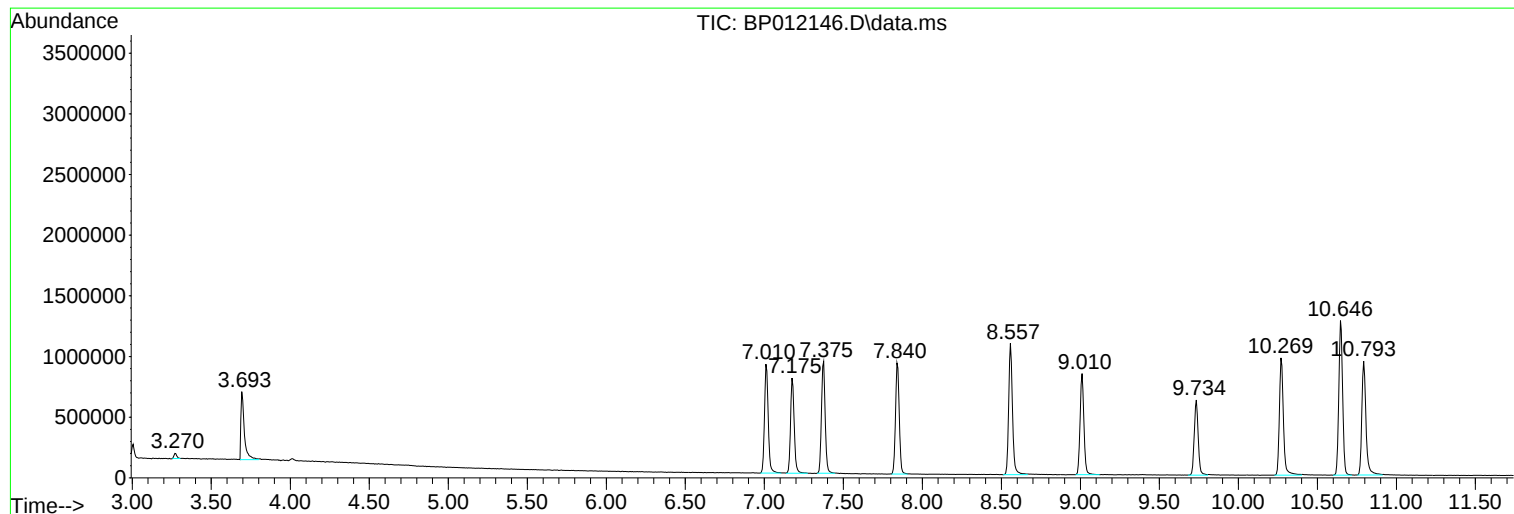

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012146.D
Acq On : 14 Oct 2022 20:27
Operator : CG/JU
Sample : PB148313BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK313

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101422\
Data File : BP012146.D
Acq On : 14 Oct 2022 20:27
Operator : CG/JU
Sample : PB148313BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK313

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
