




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022394.D
 Acq On : 15 Oct 2024 18:19
 Operator : RC/JU
 Sample : P4349-11
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAG4

Manual IntegrationsAPPROVED

Quant Time: Oct 16 02:29:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 14 11:01:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :mohammad ahmed 10/22/2024

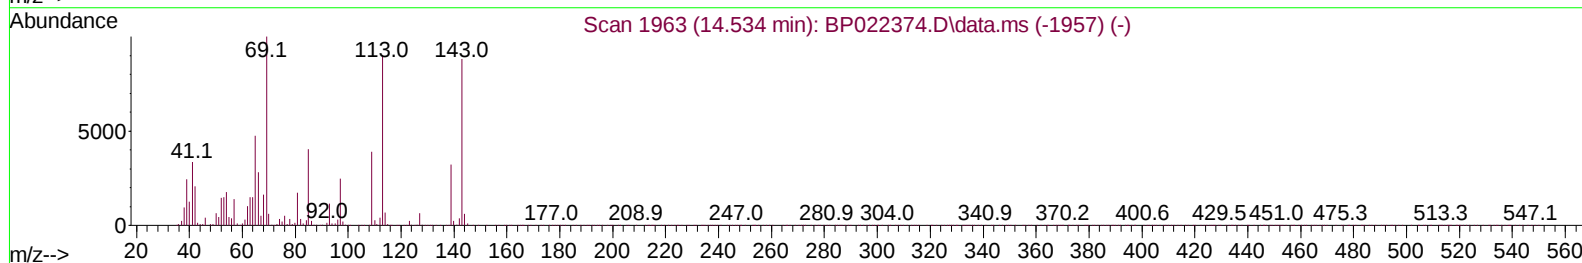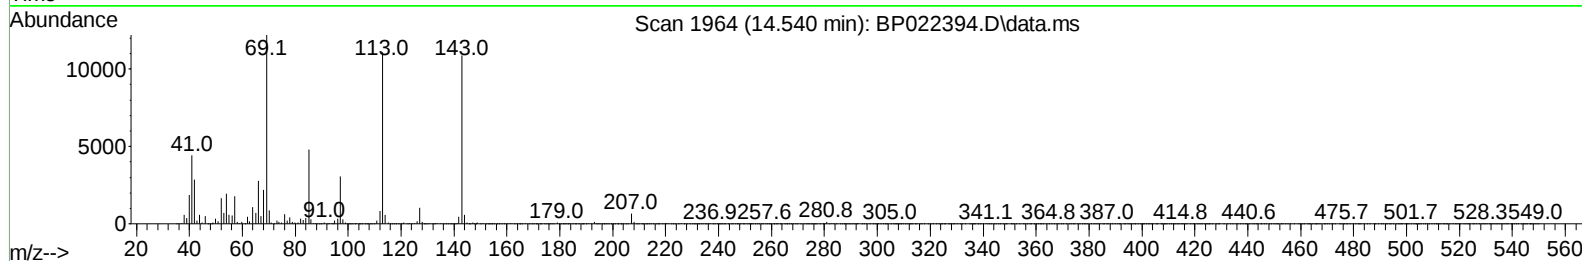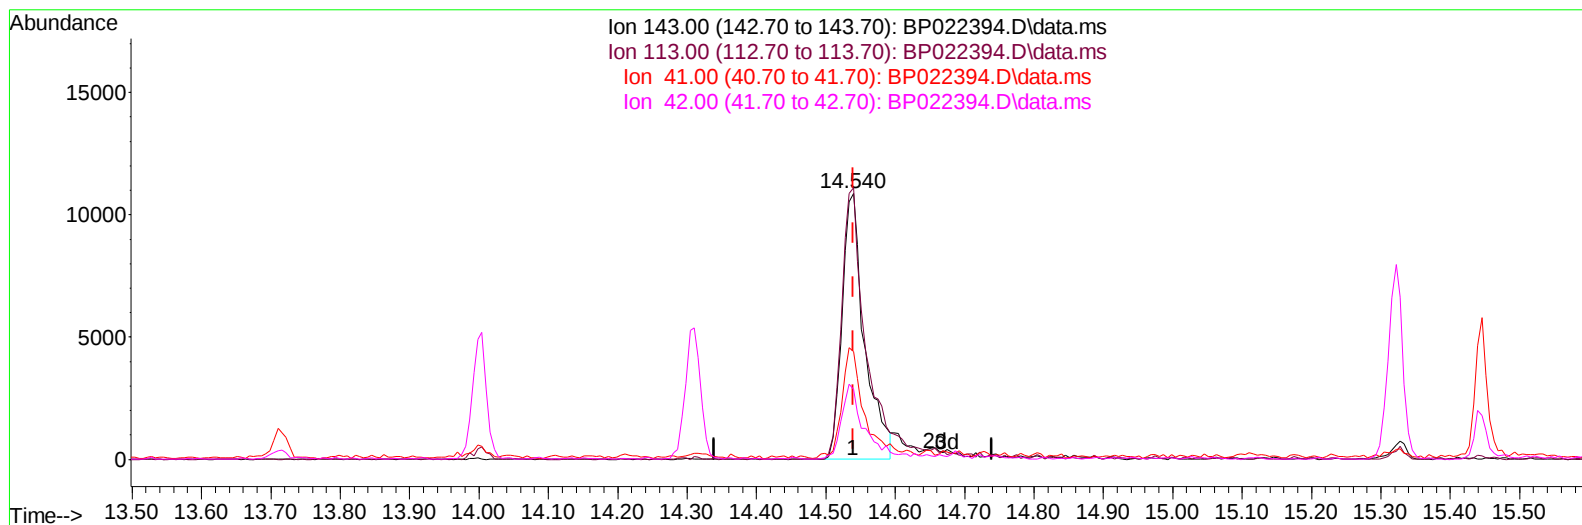

TIC: BP022394.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.540min (+ 0.000) 6.57 ng/u1

response 24207

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	102.06
41.00	35.90	40.60
42.00	23.70	26.34




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022394.D
Acq On : 15 Oct 2024 18:19
Operator : RC/JU
Sample : P4349-11
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG4

Manual IntegrationsAPPROVED

Quant Time: Oct 16 02:29:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 14 11:01:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :mohammad ahmed 10/22/2024

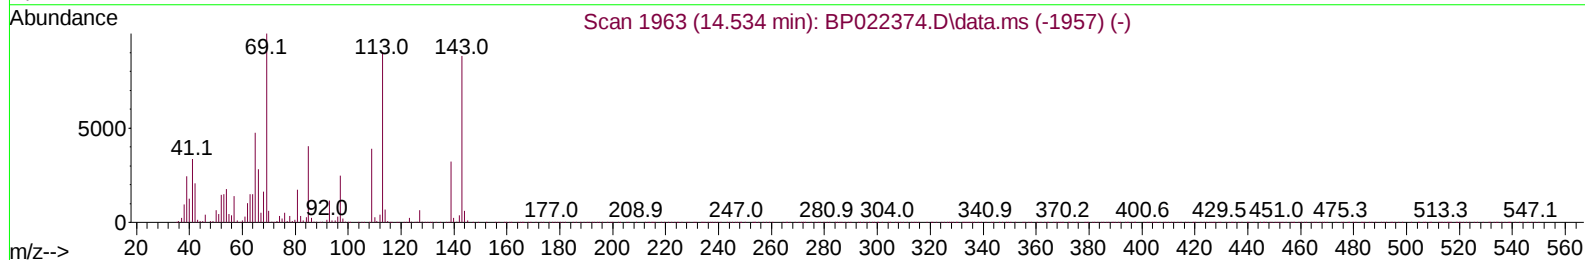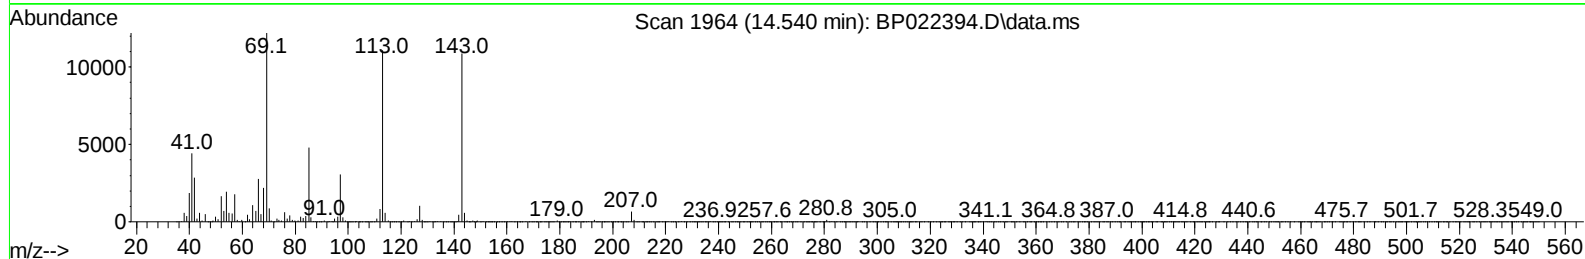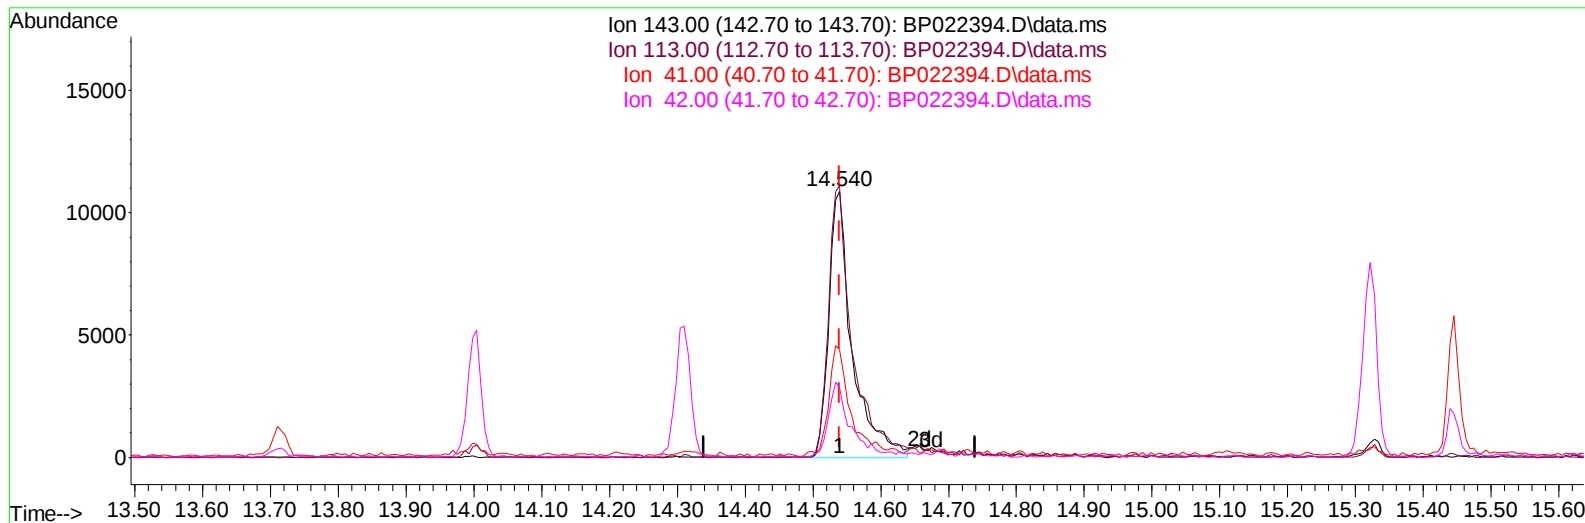

TIC: BP022394.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.540min (+ 0.000) 7.08 ng/ul m

response 26075

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	102.06
41.00	35.90	40.60
42.00	23.70	26.34

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022394.D
 Acq On : 15 Oct 2024 18:19
 Operator : RC/JU
 Sample : P4349-11
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAG4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :mohammad ahmed 10/22/2024

Quant Time: Oct 16 02:30:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 14 11:01:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	90774	20.000	ng/ul	0.00
20) Naphthalene-d8	10.452	136	352561	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	276316	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	701316	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	786206	20.000	ng/ul	-0.01
88) Perylene-d12	24.839	264	892397	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	10021	4.290	ng/uL	0.00
4) Pyridine-d5	3.640	84	31417	4.899	ng/ul	0.00
7) Phenol-d5	6.881	99	88234	11.547	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	111893	24.915	ng/ul	0.00
11) 2-Chlorophenol-d4	7.234	132	139072	25.650	ng/ul	0.00
15) 4-Methylphenol-d8	8.393	113	134595	22.072	ng/ul	0.00
21) Nitrobenzene-d5	8.834	128	73622	27.158	ng/ul	0.00
24) 2-Nitrophenol-d4	9.546	143	88398	28.166	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	179454	26.903	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	135560	17.199	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166	603648	27.496	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	627296	26.902	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	26075m	7.080	ng/ul	0.00
60) Fluorene-d10	15.322	176	539188	28.316	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	112287	24.344	ng/ul	0.00
73) Anthracene-d10	17.210	188	969919	29.399	ng/ul	0.00
81) Pyrene-d10	19.592	212	1259530	30.295	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.598	264	1445343	30.327	ng/ul	-0.04

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022394.D
Acq On : 15 Oct 2024 18:19
Operator : RC/JU
Sample : P4349-11
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG4

Manual IntegrationsAPPROVED

Quant Time: Oct 16 02:30:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 14 11:01:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :mohammad ahmed 10/22/2024

