

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022350.D
 Acq On : 14 Oct 2024 11:10
 Operator : RC/JU
 Sample : PB163884BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK884

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	47	rVB	26380	35739	1.04%	0.107%
2	3.634	106	110	125	rBV	318879	487846	14.13%	1.466%
3	3.958	161	165	170	rBV	13393	17915	0.52%	0.054%
4	6.887	653	663	675	rBV	406687	661564	19.16%	1.987%
5	7.040	682	689	701	rBV	297851	471367	13.65%	1.416%
6	7.246	715	724	736	rBV	414384	658499	19.08%	1.978%
7	7.699	793	801	811	rBV	462079	744639	21.57%	2.237%
8	8.399	913	920	932	rBV	483588	821004	23.78%	2.466%
9	8.840	987	995	1005	rBV	428425	642141	18.60%	1.929%
10	9.257	1059	1066	1071	rVB8	3827	6562	0.19%	0.020%
11	9.551	1109	1116	1126	rBV	349817	564745	16.36%	1.697%
12	10.093	1199	1208	1222	rBV	505606	914356	26.49%	2.747%
13	10.463	1263	1271	1284	rVB	597159	1008735	29.22%	3.030%
14	10.593	1286	1293	1307	rBV	480216	826589	23.94%	2.483%
15	12.051	1537	1541	1550	rBV2	6751	14266	0.41%	0.043%
16	13.728	1817	1826	1837	rBV	820699	1421387	41.17%	4.270%
17	14.010	1866	1874	1883	rBV	995661	1635251	47.37%	4.912%
18	14.316	1918	1926	1935	rBV	1062883	1565310	45.34%	4.702%
19	14.545	1959	1965	1975	rBV	480652	691521	20.03%	2.077%
20	14.681	1986	1988	1995	rVV8	2242	3483	0.10%	0.010%
21	14.728	1995	1996	2004	rVB8	2736	4826	0.14%	0.014%
22	15.328	2091	2098	2105	rBV	1599789	2177792	63.09%	6.542%
23	15.457	2112	2120	2135	rBV	351151	659956	19.12%	1.983%
24	15.581	2135	2141	2145	rVB6	6229	11163	0.32%	0.034%
25	15.981	2203	2209	2214	rBV4	6155	8590	0.25%	0.026%
26	16.045	2214	2220	2226	rBV5	7533	12485	0.36%	0.038%
27	16.116	2228	2232	2237	rBV8	2628	4626	0.13%	0.014%
28	16.375	2272	2276	2282	rBV5	5493	8830	0.26%	0.027%
29	16.439	2282	2287	2291	rVV3	9561	15379	0.45%	0.046%
30	16.486	2291	2295	2300	rVB3	7051	11131	0.32%	0.033%
31	16.598	2310	2314	2317	rBV5	2557	4233	0.12%	0.013%
32	16.775	2340	2344	2351	rVB10	3566	7922	0.23%	0.024%
33	16.904	2359	2366	2368	rBV6	3976	7142	0.21%	0.021%
34	17.116	2396	2402	2412	rBV	1608804	2189316	63.42%	6.577%
35	17.216	2412	2419	2430	rVV	1738619	2589314	75.01%	7.779%
36	17.316	2434	2436	2444	rVB9	2469	4008	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022350.D
Acq On : 14 Oct 2024 11:10
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK884

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	18.051	2558	2561	2563	rBV4	3717	4445	0.13%	0.013%
38	19.151	2743	2748	2753	rBV3	26373	45770	1.33%	0.137%
39	19.222	2756	2760	2764	rVV	25849	37138	1.08%	0.112%
40	19.598	2819	2824	2834	rBV	2490852	3355291	97.19%	10.080%
41	21.557	3151	3157	3165	rBV2	1660548	2732906	79.17%	8.210%
42	24.633	3672	3680	3694	rVB	1344425	3452132	100.00%	10.371%
43	24.857	3710	3718	3730	rVB	1064908	2750370	79.67%	8.262%




Sum of corrected areas: 33287684

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022350.D
Acq On : 14 Oct 2024 11:10
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK884

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

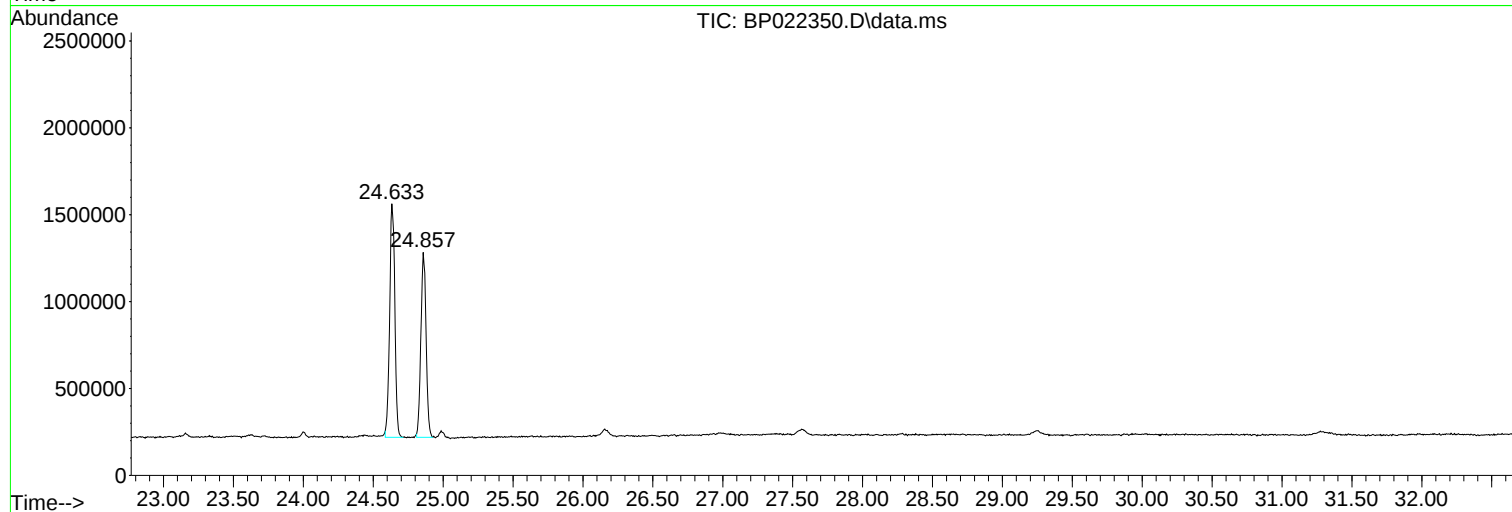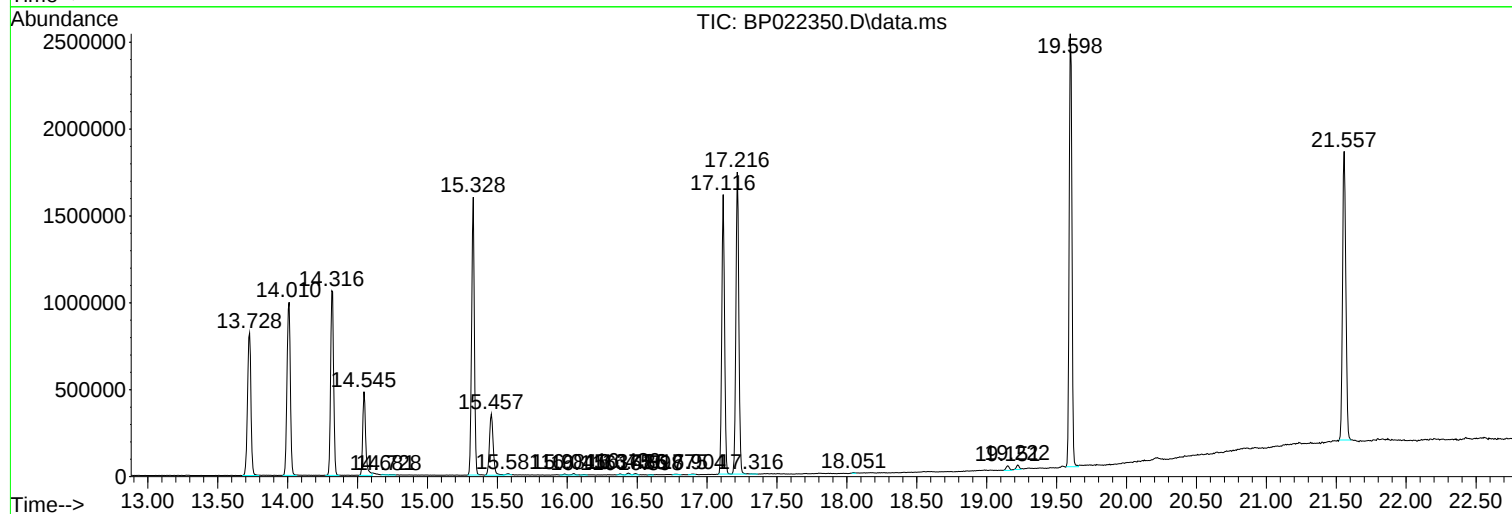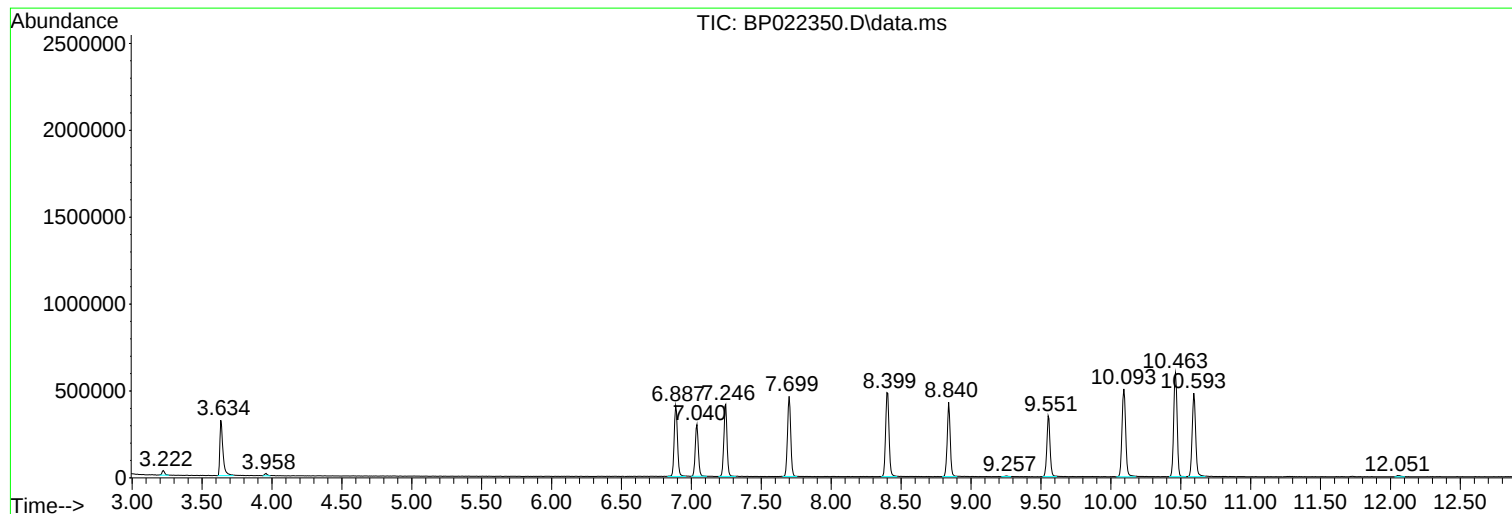

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022350.D
Acq On : 14 Oct 2024 11:10
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK884

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022350.D
Acq On : 14 Oct 2024 11:10
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK884

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc