

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022351.D
 Acq On : 14 Oct 2024 11:51
 Operator : RC/JU
 Sample : PB163924BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK924

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	50	rVB	26727	38638	1.10%	0.113%
2	3.634	107	110	126	rBV	327332	497514	14.20%	1.460%
3	3.958	160	165	171	rBV	11116	15572	0.44%	0.046%
4	6.887	652	663	676	rBV	418910	685511	19.56%	2.011%
5	7.046	681	690	701	rVV	302085	489861	13.98%	1.437%
6	7.246	717	724	735	rBV	429136	690754	19.71%	2.027%
7	7.705	793	802	813	rBV	430347	714528	20.39%	2.096%
8	8.399	913	920	931	rBV	504177	868692	24.79%	2.549%
9	8.840	988	995	1008	rBV	397316	684575	19.53%	2.009%
10	9.252	1060	1065	1072	rVB8	2499	4901	0.14%	0.014%
11	9.558	1110	1117	1126	rBV	375786	608942	17.38%	1.787%
12	10.093	1198	1208	1220	rBV	540527	965283	27.54%	2.832%
13	10.463	1262	1271	1284	rVB	540556	994774	28.39%	2.919%
14	10.593	1284	1293	1309	rBV	526765	897809	25.62%	2.634%
15	11.734	1481	1487	1495	rVB7	3020	5559	0.16%	0.016%
16	12.052	1535	1541	1547	rBV3	7554	14998	0.43%	0.044%
17	13.716	1817	1824	1834	rBV	1103464	1532336	43.73%	4.496%
18	14.010	1864	1874	1885	rBV	1141793	1796995	51.28%	5.272%
19	14.328	1919	1928	1936	rBV	1012655	1573794	44.91%	4.617%
20	14.545	1958	1965	1979	rBV	383866	768538	21.93%	2.255%
21	15.328	2090	2098	2111	rBV	1431576	2338556	66.73%	6.861%
22	15.445	2112	2118	2133	rVV	509589	733817	20.94%	2.153%
23	15.569	2133	2139	2145	rVB6	6109	13396	0.38%	0.039%
24	16.892	2358	2364	2369	rBV2	3518	6429	0.18%	0.019%
25	17.116	2395	2402	2412	rBV	1688036	2180190	62.21%	6.397%
26	17.222	2412	2420	2432	rVB	1598937	2733940	78.01%	8.021%
27	18.057	2559	2562	2566	rBV6	2951	4954	0.14%	0.015%
28	19.139	2743	2746	2752	rVB2	26487	34185	0.98%	0.100%
29	19.216	2755	2759	2766	rVV2	28927	42816	1.22%	0.126%
30	19.592	2817	2823	2832	rBV	2517728	3439478	98.15%	10.091%
31	21.551	3150	3156	3167	rVB2	1629155	2580778	73.64%	7.572%
32	24.627	3670	3679	3691	rVB	1247037	3504393	100.00%	10.282%
33	24.851	3709	3717	3728	rVB	981425	2620851	74.79%	7.690%




Sum of corrected areas: 34083357

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022351.D
Acq On : 14 Oct 2024 11:51
Operator : RC/JU
Sample : PB163924BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

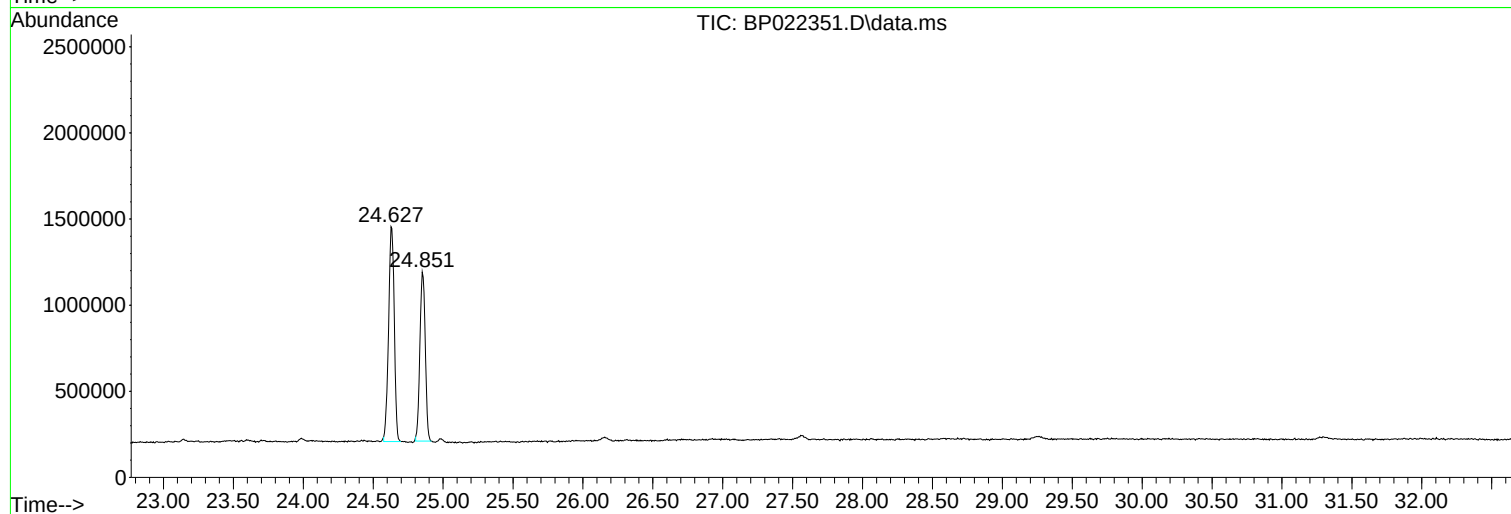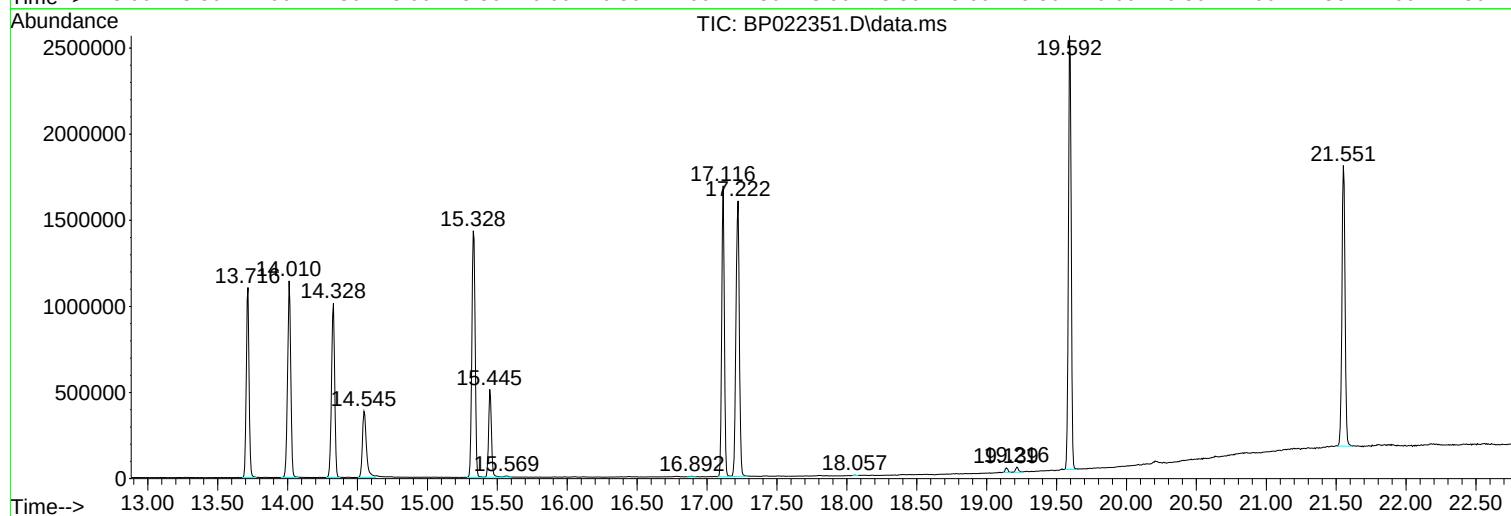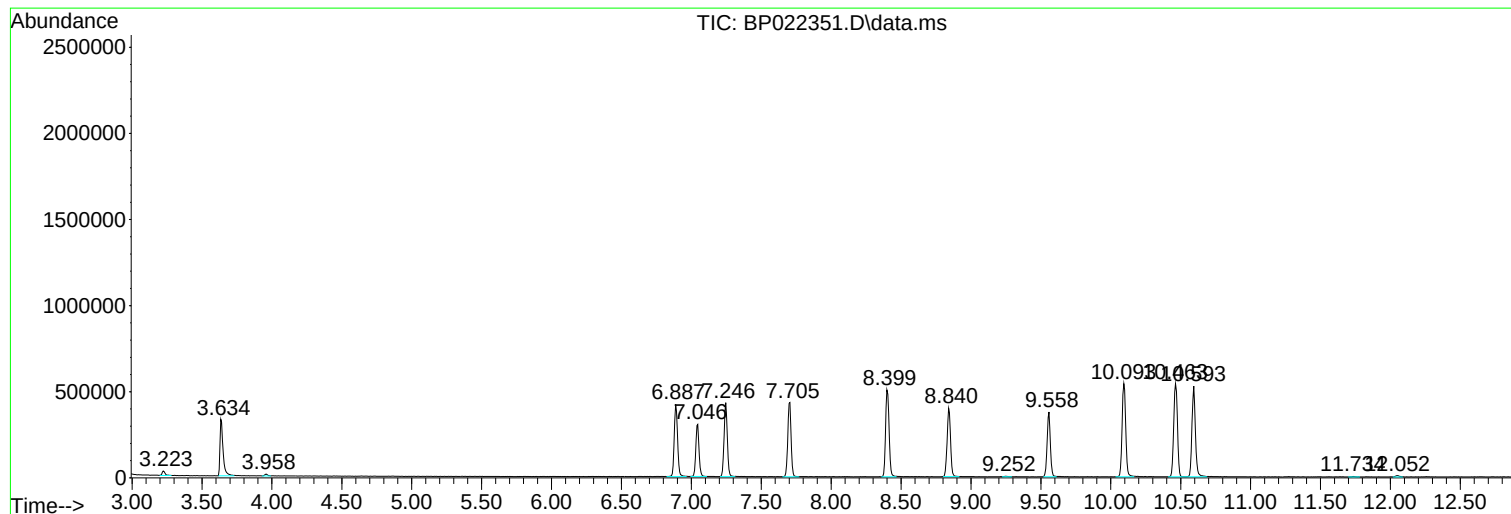

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022351.D
Acq On : 14 Oct 2024 11:51
Operator : RC/JU
Sample : PB163924BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022351.D
Acq On : 14 Oct 2024 11:51
Operator : RC/JU
Sample : PB163924BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc