

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022360.D
 Acq On : 14 Oct 2024 18:01
 Operator : RC/JU
 Sample : PB163830BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK830

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	46	rVB	21657	25968	0.93%	0.096%
2	3.634	106	110	124	rBV	279257	413881	14.75%	1.535%
3	3.957	161	165	172	rVB2	6488	9670	0.34%	0.036%
4	6.887	652	663	678	rVB	335902	571144	20.36%	2.119%
5	7.040	681	689	698	rBV	248778	395790	14.11%	1.468%
6	7.240	716	723	737	rBV	355422	565072	20.14%	2.096%
7	7.698	794	801	810	rBV	387513	618042	22.03%	2.293%
8	8.398	911	920	931	rBV	418126	700063	24.95%	2.597%
9	8.839	987	995	1005	rBV	325526	545228	19.43%	2.022%
10	9.257	1059	1066	1069	rVB8	2797	4858	0.17%	0.018%
11	9.551	1108	1116	1130	rBV	291736	477617	17.02%	1.772%
12	10.092	1199	1208	1220	rBV	418479	758875	27.05%	2.815%
13	10.463	1261	1271	1280	rBV	491523	839424	29.92%	3.114%
14	10.592	1286	1293	1310	rBV	395929	695147	24.78%	2.579%
15	12.057	1537	1542	1546	rBV4	4829	8874	0.32%	0.033%
16	13.716	1816	1824	1833	rBV	723357	1107062	39.46%	4.106%
17	14.010	1866	1874	1890	rBB	935023	1350980	48.15%	5.011%
18	14.321	1918	1927	1936	rBV	911745	1263844	45.05%	4.688%
19	14.551	1959	1966	1983	rBV	367603	579007	20.64%	2.148%
20	15.327	2090	2098	2112	rBV	1144170	1794038	63.95%	6.655%
21	15.445	2112	2118	2134	rVV	321377	521573	18.59%	1.935%
22	15.574	2136	2140	2147	rVB8	6126	11290	0.40%	0.042%
23	16.780	2344	2345	2349	rVB3	2610	2865	0.10%	0.011%
24	16.910	2362	2367	2369	rBV5	1916	3571	0.13%	0.013%
25	17.115	2395	2402	2413	rBV	1152134	1752354	62.46%	6.500%
26	17.221	2413	2420	2431	rVV	1331712	2098953	74.81%	7.786%
27	17.745	2507	2509	2512	rBV3	3013	3928	0.14%	0.015%
28	17.804	2517	2519	2523	rVB4	2905	3455	0.12%	0.013%
29	18.051	2557	2561	2564	rBV5	4804	7781	0.28%	0.029%
30	19.151	2744	2748	2753	rBV3	19468	29556	1.05%	0.110%
31	19.221	2756	2760	2767	rVV	21425	33664	1.20%	0.125%
32	19.598	2819	2824	2832	rBV	2132034	2673394	95.29%	9.917%
33	21.556	3151	3157	3166	rVB	1218996	2122167	75.64%	7.872%
34	24.621	3669	3678	3690	rVB	1131782	2805530	100.00%	10.407%
35	24.844	3707	3716	3730	rVB	755695	2164222	77.14%	8.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022360.D
Acq On : 14 Oct 2024 18:01
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 26958887

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022360.D
Acq On : 14 Oct 2024 18:01
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

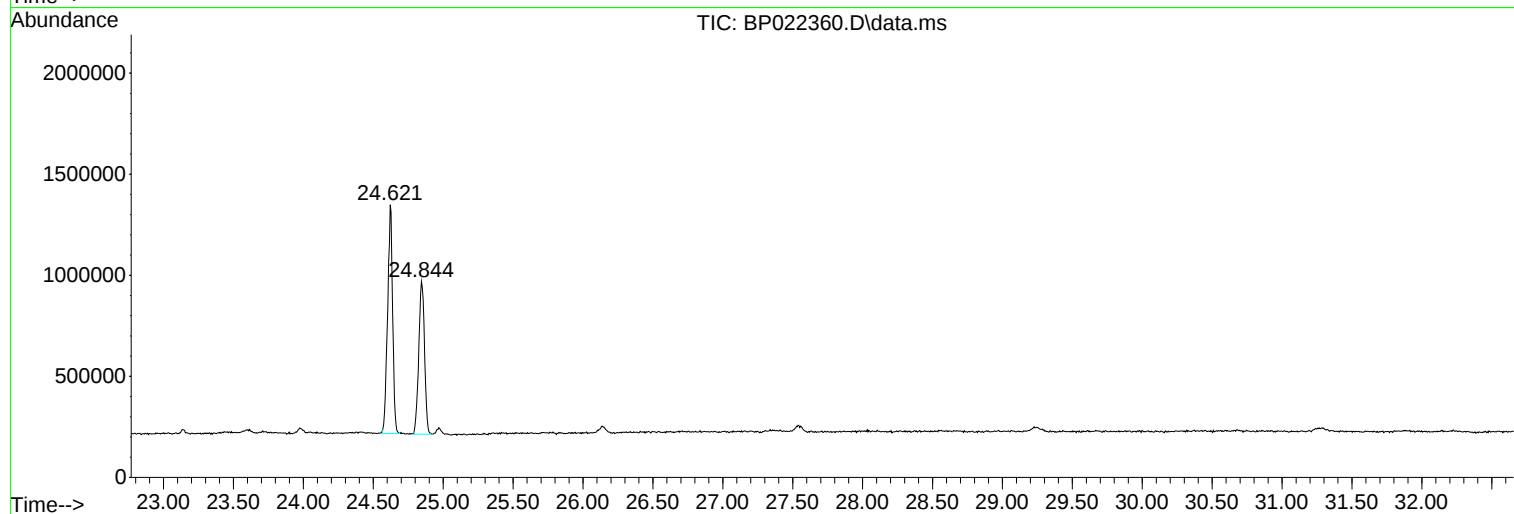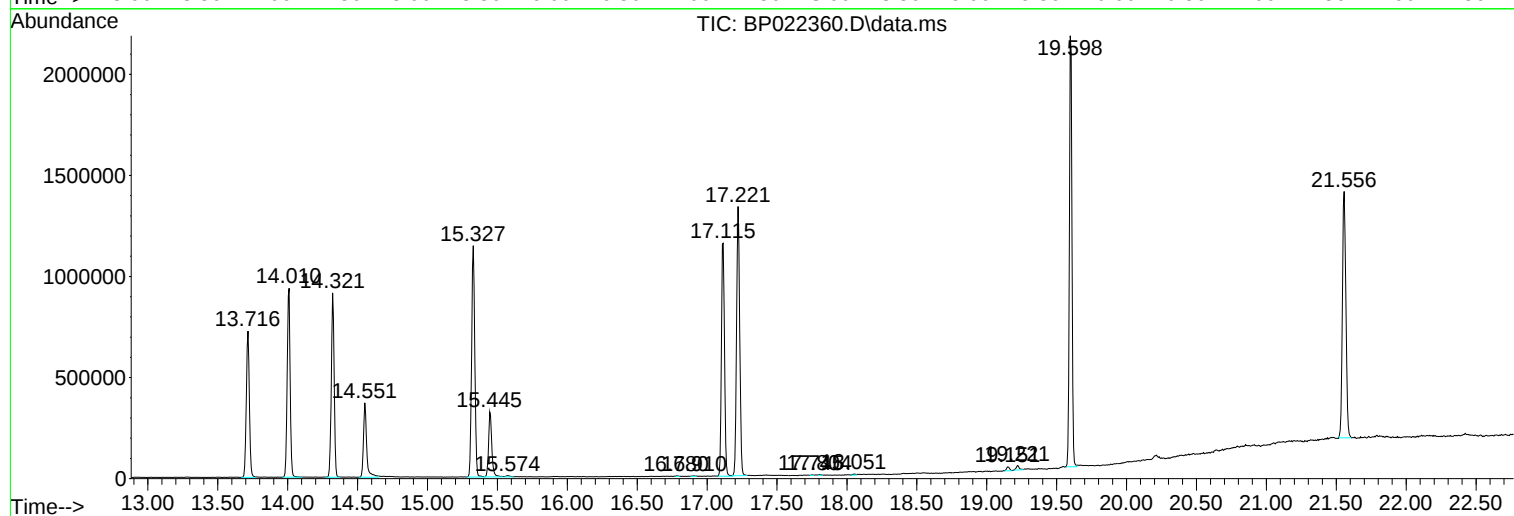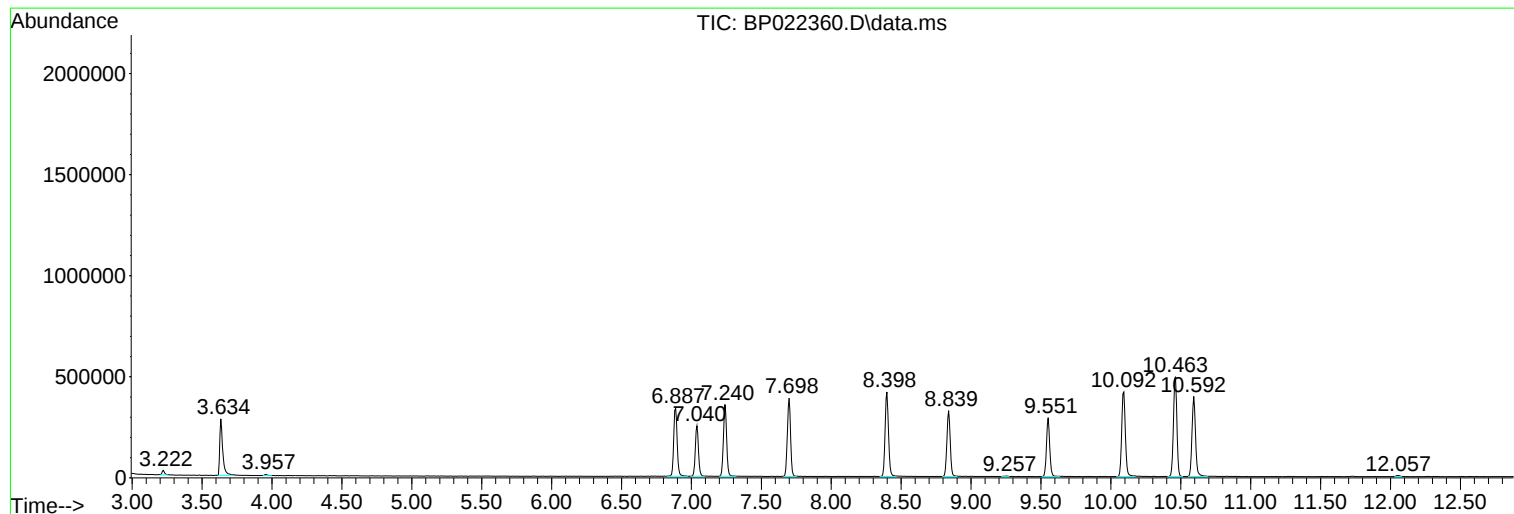

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022360.D
Acq On : 14 Oct 2024 18:01
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022360.D
Acq On : 14 Oct 2024 18:01
Operator : RC/JU
Sample : PB163830BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK830

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc