

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022376.D
 Acq On : 15 Oct 2024 05:37
 Operator : RC/JU
 Sample : PB164091BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK091

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	50	rVB	24848	33597	1.09%	0.117%
2	3.634	106	110	128	rBV	308094	458850	14.84%	1.598%
3	3.958	160	165	170	rVB2	4985	7631	0.25%	0.027%
4	6.887	652	663	672	rBV	357442	603815	19.53%	2.103%
5	7.040	682	689	698	rBV	260253	420763	13.61%	1.466%
6	7.240	714	723	736	rBV	362425	604263	19.54%	2.105%
7	7.699	792	801	811	rBV	374071	587440	19.00%	2.046%
8	8.399	911	920	937	rBV	456414	763825	24.70%	2.660%
9	8.840	986	995	1005	rBV	345365	598705	19.36%	2.085%
10	9.252	1060	1065	1071	rVB8	2948	5906	0.19%	0.021%
11	9.552	1105	1116	1128	rBV	332647	529655	17.13%	1.845%
12	10.093	1199	1208	1221	rBV	461538	839349	27.14%	2.923%
13	10.458	1262	1270	1280	rBV	466848	808199	26.14%	2.815%
14	10.587	1283	1292	1306	rBV	434899	766411	24.78%	2.669%
15	12.046	1536	1540	1548	rVB2	7628	12277	0.40%	0.043%
16	13.716	1816	1824	1838	rBV	764299	1254407	40.57%	4.369%
17	13.999	1863	1872	1883	rBV	930860	1471252	47.58%	5.124%
18	14.310	1916	1925	1937	rBV	785519	1246649	40.32%	4.342%
19	14.528	1955	1962	1984	rBV	416758	682326	22.07%	2.377%
20	15.310	2087	2095	2107	rBV	1106783	1936382	62.62%	6.744%
21	15.451	2112	2119	2130	rBV	425412	603773	19.53%	2.103%
22	15.557	2133	2137	2143	rVB6	6238	11447	0.37%	0.040%
23	15.893	2191	2194	2201	rBV9	1731	3370	0.11%	0.012%
24	16.781	2342	2345	2350	rVB6	2568	4142	0.13%	0.014%
25	16.898	2360	2365	2370	rBV6	3650	5105	0.17%	0.018%
26	17.110	2394	2401	2410	rBV	1045778	1752401	56.67%	6.104%
27	17.216	2412	2419	2434	rVV	1659989	2341650	75.73%	8.156%
28	19.139	2742	2746	2750	rVB3	21155	28023	0.91%	0.098%
29	19.216	2755	2759	2764	rBV2	21281	31411	1.02%	0.109%
30	19.598	2817	2824	2831	rBV	2127121	2940613	95.10%	10.242%
31	21.551	3150	3156	3164	rBV2	1400314	2104194	68.05%	7.329%
32	24.621	3669	3678	3693	rVB	1133571	3092241	100.00%	10.770%
33	24.863	3709	3719	3730	rVB	781839	2160940	69.88%	7.527%




Sum of corrected areas: 28711012

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022376.D
Acq On : 15 Oct 2024 05:37
Operator : RC/JU
Sample : PB164091BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK091

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

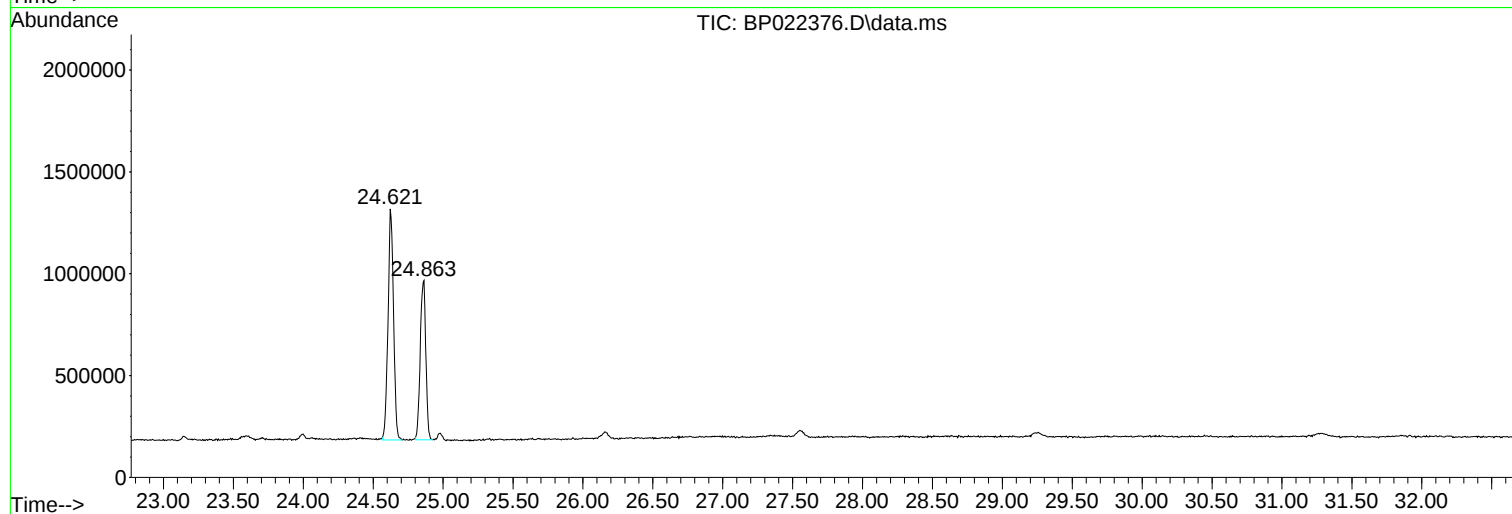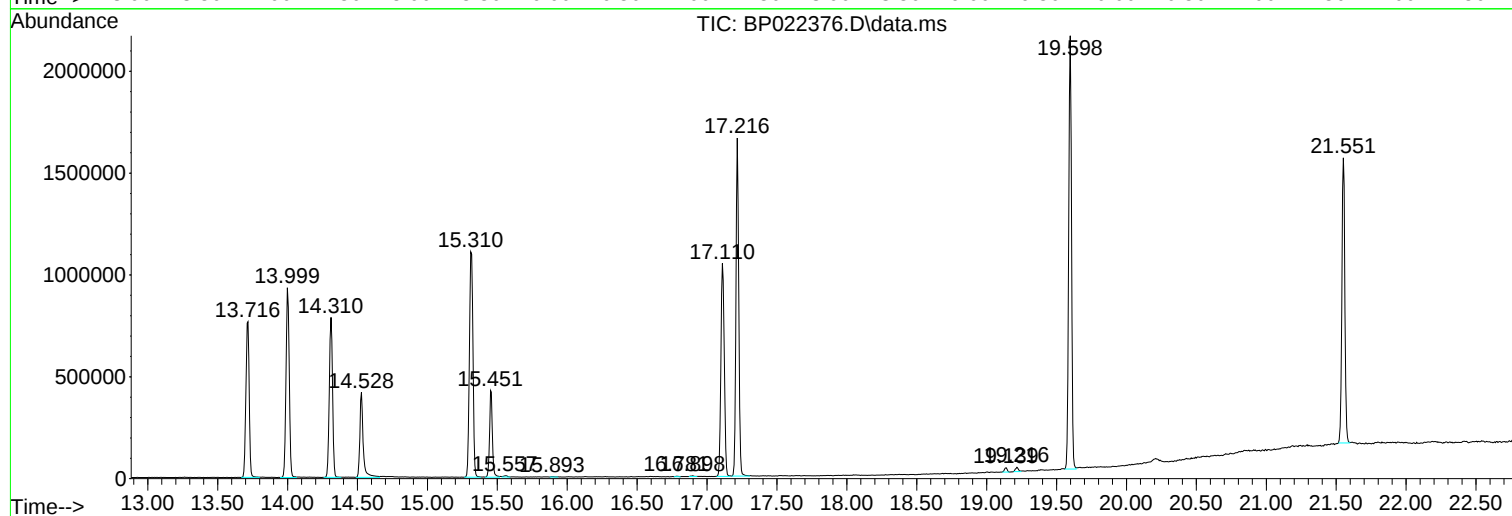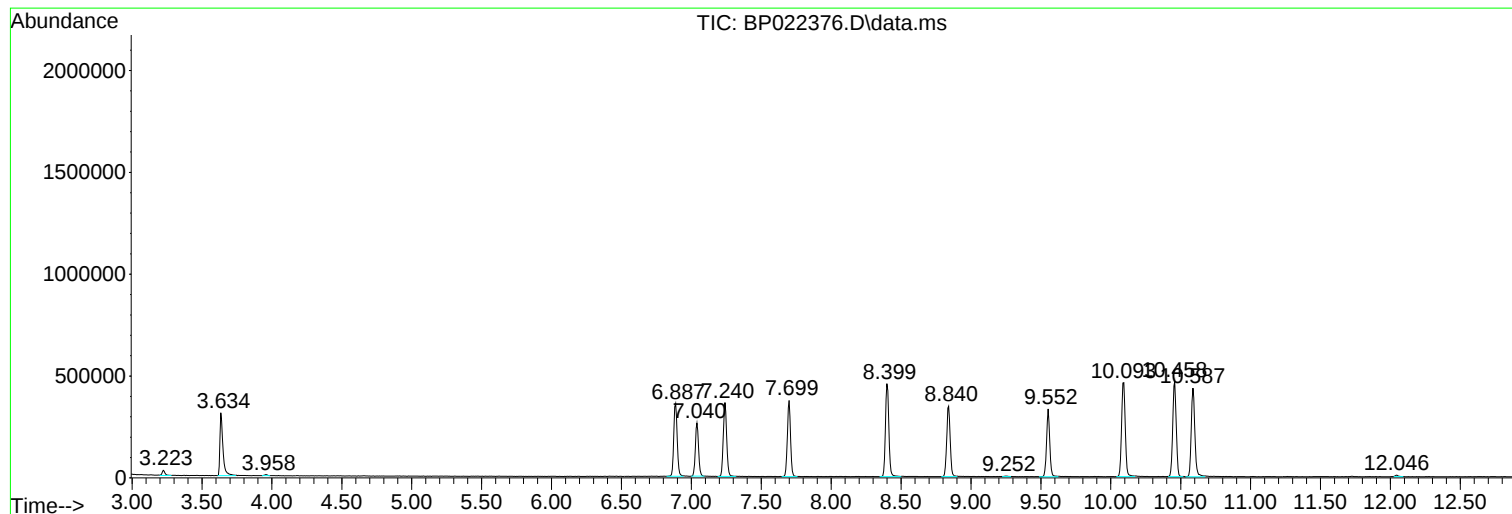

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022376.D
Acq On : 15 Oct 2024 05:37
Operator : RC/JU
Sample : PB164091BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK091

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022376.D
Acq On : 15 Oct 2024 05:37
Operator : RC/JU
Sample : PB164091BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK091

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------