

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022385.D
 Acq On : 15 Oct 2024 11:44
 Operator : RC/JU
 Sample : P4349-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	29	rVB7	5358	6882	0.18%	0.023%
2	3.222	36	40	46	rBV	18420	24276	0.63%	0.082%
3	3.958	161	165	170	rVB	12169	17542	0.45%	0.059%
4	4.322	223	227	234	rVB7	4651	8025	0.21%	0.027%
5	4.399	234	240	245	rVB3	3864	6901	0.18%	0.023%
6	4.458	245	250	254	rBV5	4366	6756	0.17%	0.023%
7	4.505	254	258	265	rVB2	9287	14770	0.38%	0.050%
8	5.387	404	408	409	rBV4	3468	4380	0.11%	0.015%
9	5.546	429	435	439	rBV7	3198	5362	0.14%	0.018%
10	5.740	462	468	476	rBV5	10829	23891	0.62%	0.081%
11	5.993	508	511	516	rVB6	2809	4234	0.11%	0.014%
12	6.110	520	531	538	rVB3	31979	66558	1.72%	0.224%
13	6.305	559	564	569	rBV7	2839	6868	0.18%	0.023%
14	6.463	586	591	597	rBV8	2537	5079	0.13%	0.017%
15	6.528	597	602	605	rVV7	3631	5962	0.15%	0.020%
16	6.575	605	610	615	rVB4	7986	12126	0.31%	0.041%
17	6.846	650	656	657	rBV3	5939	6754	0.17%	0.023%
18	6.887	657	663	674	rVB	167230	270378	6.98%	0.912%
19	7.040	683	689	699	rBV	281174	445857	11.51%	1.503%
20	7.240	716	723	732	rBV	387169	620353	16.02%	2.092%
21	7.440	752	757	764	rVB8	4386	7411	0.19%	0.025%
22	7.699	794	801	809	rBV	368794	567464	14.65%	1.913%
23	8.399	911	920	931	rBV	383373	642973	16.60%	2.168%
24	8.840	987	995	1003	rBV	388940	640431	16.53%	2.159%
25	9.257	1058	1066	1069	rBV7	3767	8383	0.22%	0.028%
26	9.551	1108	1116	1123	rBV	346110	586494	15.14%	1.978%
27	9.604	1123	1125	1132	rVB5	7080	10726	0.28%	0.036%
28	10.087	1199	1207	1227	rBV	529071	930667	24.03%	3.138%
29	10.457	1262	1270	1282	rBV	442929	790796	20.42%	2.667%
30	10.604	1286	1295	1301	rBV3	10027	21219	0.55%	0.072%
31	11.110	1375	1381	1387	rBV	7135	14686	0.38%	0.050%
32	11.728	1478	1486	1493	rBV	2460	5477	0.14%	0.018%
33	11.810	1496	1500	1506	rVV7	2272	4244	0.11%	0.014%
34	12.045	1532	1540	1545	rBV	8194	15878	0.41%	0.054%
35	12.251	1571	1575	1582	rVB10	3002	5324	0.14%	0.018%
36	12.657	1641	1644	1651	rVB8	2470	4217	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022385.D
 Acq On : 15 Oct 2024 11:44
 Operator : RC/JU
 Sample : P4349-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	12.910	1681	1687	1694	rVB9	4036	8120	0.21%	0.027%
38	13.710	1817	1823	1832	rBV	1058429	1457993	37.64%	4.916%
39	14.004	1865	1873	1884	rBV	1018743	1550891	40.04%	5.230%
40	14.316	1918	1926	1935	rBV	790767	1253891	32.37%	4.228%
41	14.551	1958	1966	1985	rBV2	163479	369361	9.54%	1.245%
42	14.998	2034	2042	2045	rBV10	2605	5444	0.14%	0.018%
43	15.075	2048	2055	2057	rBV3	4002	5527	0.14%	0.019%
44	15.145	2063	2067	2072	rVB3	5277	9883	0.26%	0.033%
45	15.328	2091	2098	2112	rBV	1644991	2303743	59.48%	7.768%
46	15.445	2112	2118	2131	rVV	587414	813875	21.01%	2.744%
47	15.563	2133	2138	2144	rVB6	6694	13795	0.36%	0.047%
48	15.704	2156	2162	2169	rVB6	4443	8408	0.22%	0.028%
49	16.039	2213	2219	2230	rBV	64249	94413	2.44%	0.318%
50	16.780	2340	2345	2350	rVB9	3949	6341	0.16%	0.021%
51	16.886	2360	2363	2372	rVB5	3240	6582	0.17%	0.022%
52	17.116	2394	2402	2411	rBV	1365858	1765034	45.57%	5.952%
53	17.216	2411	2419	2429	rBV	1792961	2835588	73.21%	9.561%
54	17.410	2448	2452	2456	rBV	10476	14554	0.38%	0.049%
55	17.804	2516	2519	2525	rBV7	4280	7184	0.19%	0.024%
56	18.051	2557	2561	2569	rBV2	29978	42044	1.09%	0.142%
57	18.398	2616	2620	2622	rBV5	3680	5609	0.14%	0.019%
58	18.551	2642	2646	2648	rBV5	5263	6882	0.18%	0.023%
59	19.145	2742	2747	2752	rBV4	22973	36075	0.93%	0.122%
60	19.222	2756	2760	2763	rBV	30555	42541	1.10%	0.143%
61	19.380	2783	2787	2792	rVB4	22953	30064	0.78%	0.101%
62	19.533	2809	2813	2817	rVB4	16004	24475	0.63%	0.083%
63	19.598	2818	2824	2831	rBV	2773079	3700078	95.53%	12.476%
64	19.851	2862	2867	2874	rVB	204116	268746	6.94%	0.906%
65	21.539	3148	3154	3164	rVB2	1388898	2187571	56.48%	7.376%
66	24.609	3667	3676	3689	rVB	1500195	3873248	100.00%	13.060%
67	24.821	3705	3712	3713	rBV	812382	1089171	28.12%	3.673%




Sum of corrected areas: 29656475

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022385.D
Acq On : 15 Oct 2024 11:44
Operator : RC/JU
Sample : P4349-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

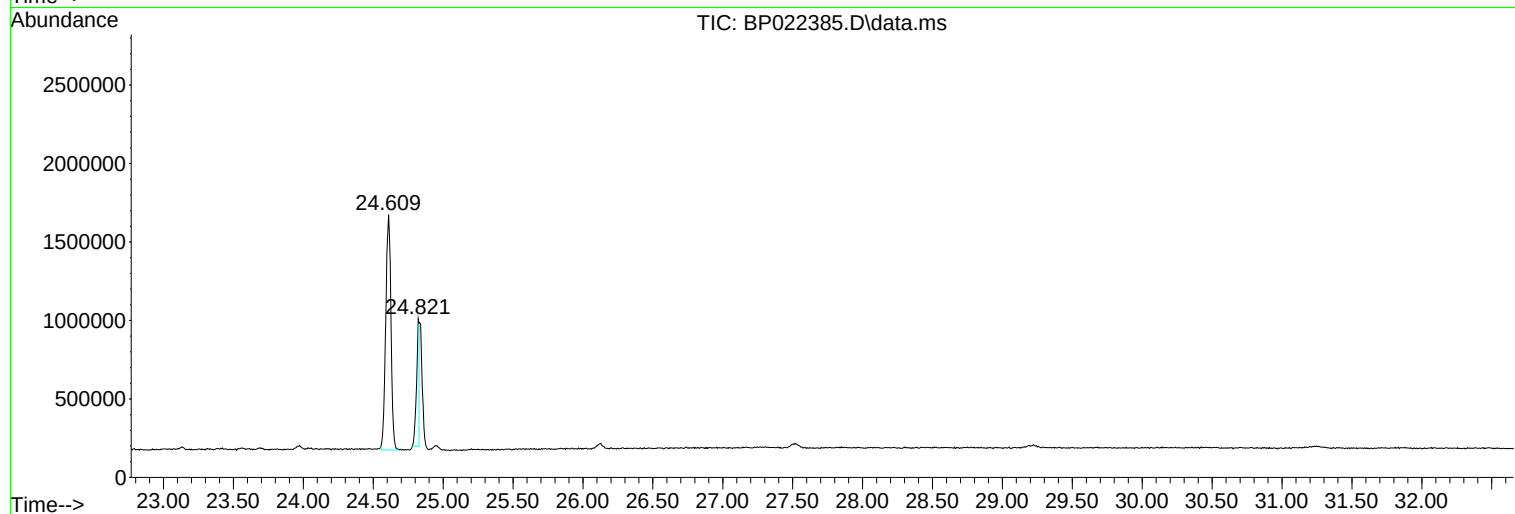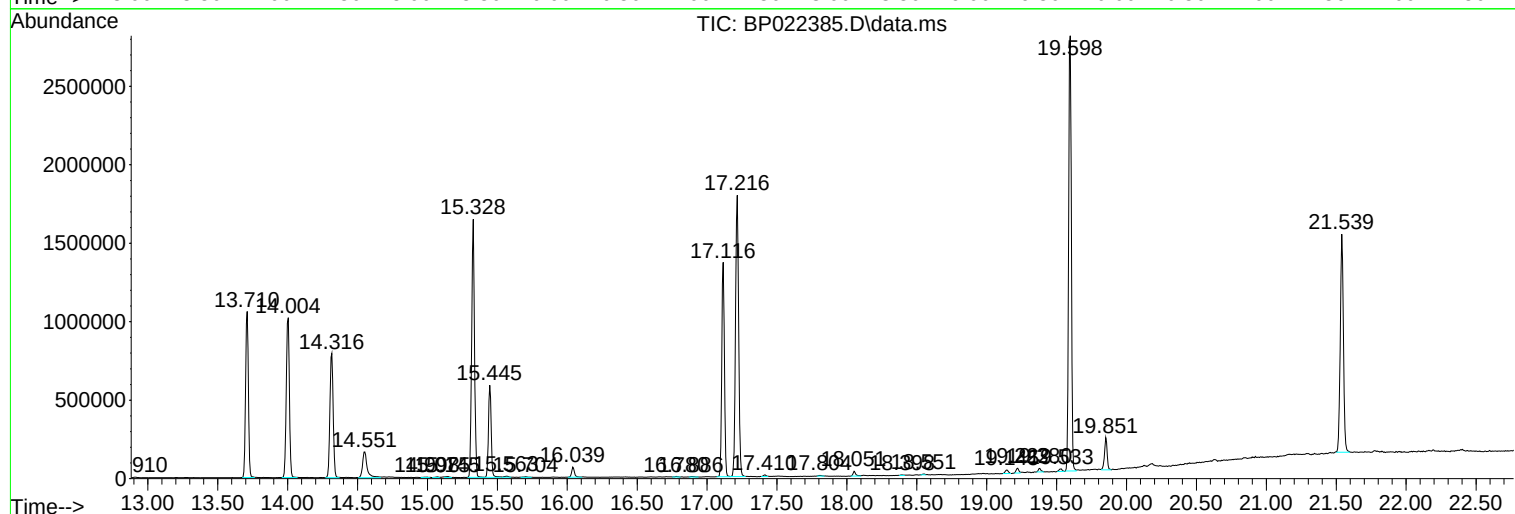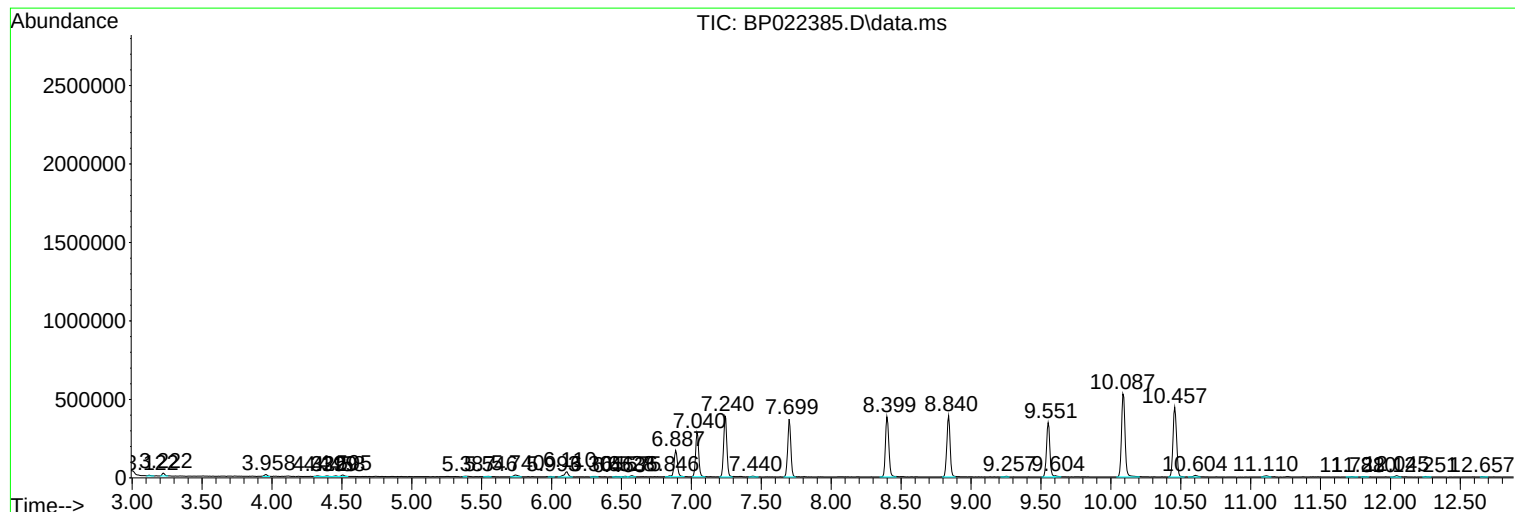

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022385.D
Acq On : 15 Oct 2024 11:44
Operator : RC/JU
Sample : P4349-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentene, 1,2,3,3,4-pen... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.110	2.35 ng/ul	66558	1,4-Dichlorobenzene-d4	7.699

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentene, 1,2,3,3,4-pentamet...	138	C10H18	197390-29-7	90
2			Cyclopentene, 1,2,3,4,5-pentamet...	138	C10H18	1000154-28-6	90
3			Furan, 2-(1,1-dimethylethyl)-4-m...	138	C9H14O	006141-68-0	74
4			Phorone	138	C9H14O	000504-20-1	64
5			1,3-Benzenediol, 4-ethyl-	138	C8H10O2	002896-60-8	64

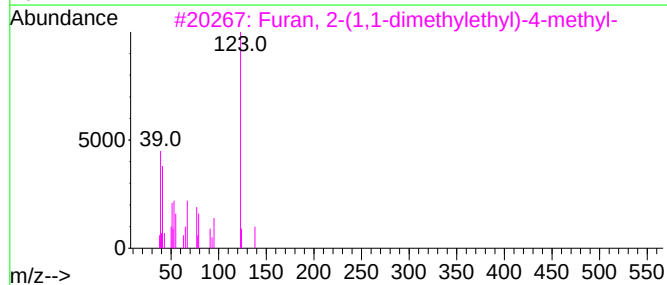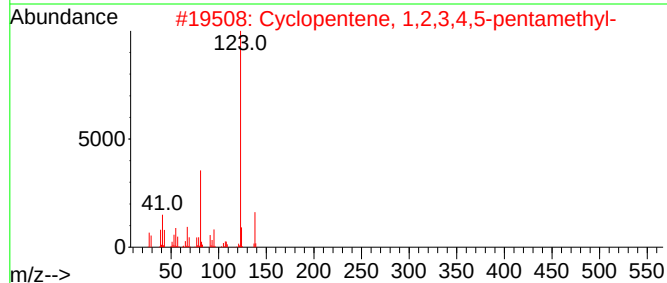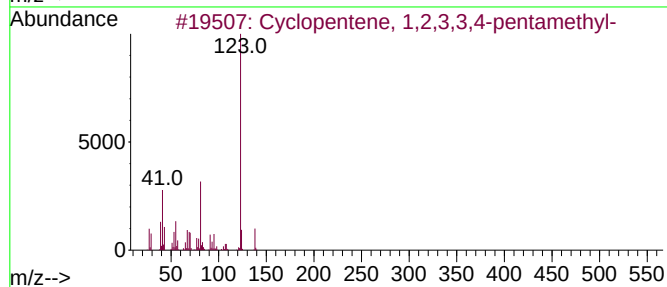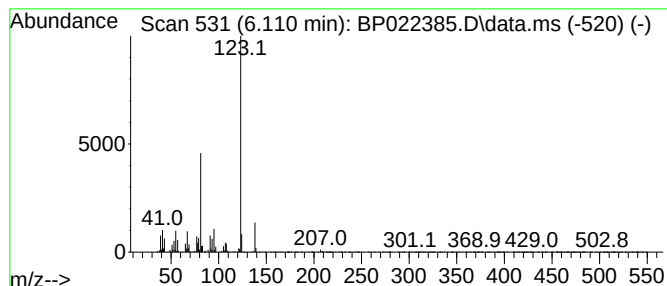

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022385.D
Acq On : 15 Oct 2024 11:44
Operator : RC/JU
Sample : P4349-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butyl citrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.851	2.46 ng/ul	268746	Chrysene-d12	21.539

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butyl citrate	360	C18H32O7	000077-94-1	64
2			Tributyl acetylcitrate	402	C20H34O8	000077-90-7	59
3			Adipic acid, butyl 2,4-dimethylp...	300	C17H32O4	1000349-77-7	40
4			6-Chloro-2,3-dihydro-1,2-benzoth...	185	C7H4ClNOS	000070-10-0	38
5			Butyl citrate	360	C18H32O7	000077-94-1	38

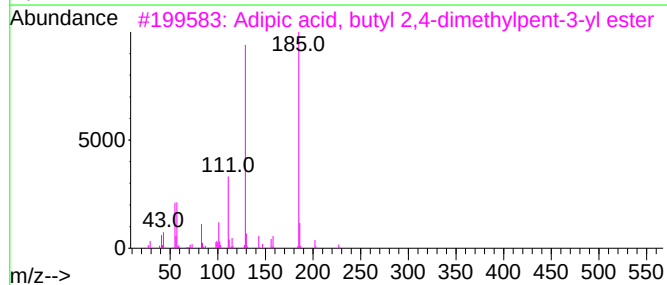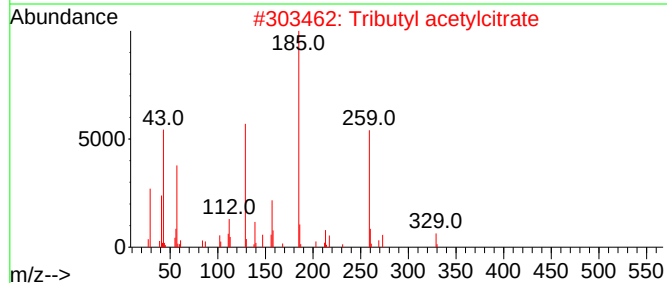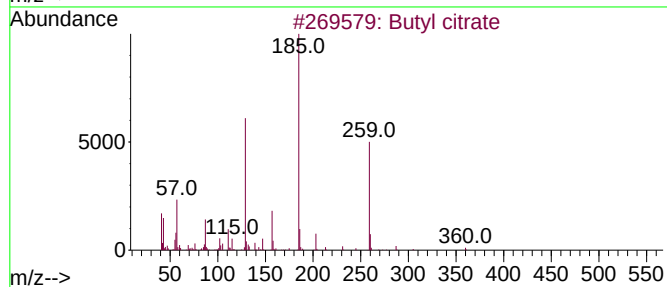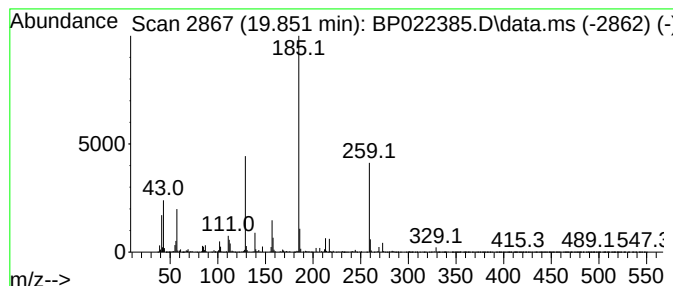

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022385.D
Acq On : 15 Oct 2024 11:44
Operator : RC/JU
Sample : P4349-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentene, 1...	6.110	2.4	ng/ul	66558	1	7.699	567464	20.0
Butyl citrate	19.851	2.5	ng/ul	268746	5	21.539	2187570	20.0