

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022396.D
 Acq On : 15 Oct 2024 19:40
 Operator : RC/JU
 Sample : P4349-14
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	47	rVB	15992	23004	0.71%	0.088%
2	3.640	107	111	121	rBV	93157	141472	4.39%	0.543%
3	3.958	161	165	168	rVB3	5926	7900	0.25%	0.030%
4	4.328	224	228	234	rVB8	4209	6796	0.21%	0.026%
5	4.505	254	258	264	rVB4	7622	13587	0.42%	0.052%
6	4.746	294	299	301	rBV6	2683	4105	0.13%	0.016%
7	4.858	314	318	324	rBV4	3827	7931	0.25%	0.030%
8	5.540	430	434	441	rVB10	2346	4490	0.14%	0.017%
9	5.740	462	468	476	rVB6	6860	14258	0.44%	0.055%
10	5.987	504	510	516	rVB7	4688	8313	0.26%	0.032%
11	6.105	519	530	536	rBV4	20705	41481	1.29%	0.159%
12	6.570	605	609	613	rVB5	4516	7479	0.23%	0.029%
13	6.881	657	662	675	rVB	160659	271067	8.42%	1.040%
14	7.034	682	688	698	rBV	238709	377655	11.72%	1.449%
15	7.240	712	723	731	rBV	324386	543813	16.88%	2.086%
16	7.699	792	801	810	rBV	307952	498078	15.46%	1.910%
17	8.399	912	920	936	rBV	349262	593095	18.41%	2.275%
18	8.834	986	994	1003	rBV	346374	554260	17.21%	2.126%
19	9.246	1060	1064	1070	rVB7	4597	6777	0.21%	0.026%
20	9.552	1107	1116	1122	rBV	284486	494593	15.35%	1.897%
21	9.605	1122	1125	1132	rVB4	7652	14386	0.45%	0.055%
22	10.087	1198	1207	1225	rBV	446016	794511	24.67%	3.048%
23	10.452	1261	1269	1277	rBV	379453	687443	21.34%	2.637%
24	10.593	1286	1293	1313	rVB	302990	532983	16.55%	2.044%
25	11.269	1399	1408	1410	rBV10	2230	5026	0.16%	0.019%
26	11.716	1479	1484	1490	rBV9	2624	4488	0.14%	0.017%
27	12.040	1532	1539	1545	rBV3	7055	12069	0.37%	0.046%
28	13.710	1816	1823	1835	rBV	822597	1209390	37.55%	4.639%
29	13.993	1864	1871	1885	rBV	970305	1369938	42.53%	5.255%
30	14.304	1917	1924	1932	rBV	686870	1066648	33.11%	4.091%
31	14.540	1954	1964	1981	rVV	156129	307878	9.56%	1.181%
32	14.681	1984	1988	1993	rVV7	6710	13406	0.42%	0.051%
33	14.757	1997	2001	2007	rVB8	3497	6303	0.20%	0.024%
34	15.140	2060	2066	2071	rBV10	4399	10799	0.34%	0.041%
35	15.310	2089	2095	2102	rBV	1299278	1834566	56.95%	7.037%
36	15.363	2102	2104	2109	rVB6	2061	3430	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022396.D
Acq On : 15 Oct 2024 19:40
Operator : RC/JU
Sample : P4349-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	15.451	2112	2119	2129	rBV	385204	637999	19.81%	2.447%
38	15.569	2135	2139	2147	rVB6	6004	10692	0.33%	0.041%
39	15.687	2154	2159	2165	rBV	27688	40816	1.27%	0.157%
40	15.898	2191	2195	2200	rBV7	3278	5508	0.17%	0.021%
41	15.981	2205	2209	2212	rBV6	1893	3447	0.11%	0.013%
42	16.028	2212	2217	2225	rBV	33216	54942	1.71%	0.211%
43	16.698	2329	2331	2337	rVB7	3731	4263	0.13%	0.016%
44	16.775	2340	2344	2350	rVB8	3879	7651	0.24%	0.029%
45	17.110	2393	2401	2410	rBV	906271	1461292	45.37%	5.605%
46	17.216	2412	2419	2429	rVV	1330497	2194182	68.12%	8.416%
47	18.034	2553	2558	2565	rBV3	34526	53988	1.68%	0.207%
48	18.545	2641	2645	2650	rBV7	6402	10484	0.33%	0.040%
49	19.128	2741	2744	2750	rVB	24535	31136	0.97%	0.119%
50	19.204	2753	2757	2761	rBV2	19431	29994	0.93%	0.115%
51	19.369	2781	2785	2789	rBV4	24317	35753	1.11%	0.137%
52	19.586	2815	2822	2830	rVB	1896033	2838012	88.11%	10.886%
53	21.551	3149	3156	3165	rBV2	1158060	1891674	58.73%	7.256%
54	24.616	3668	3677	3688	rVB	1369882	3221101	100.00%	12.355%
55	24.833	3705	3714	3728	rVB	699188	2044536	63.47%	7.842%




Sum of corrected areas: 26070888

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022396.D
Acq On : 15 Oct 2024 19:40
Operator : RC/JU
Sample : P4349-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

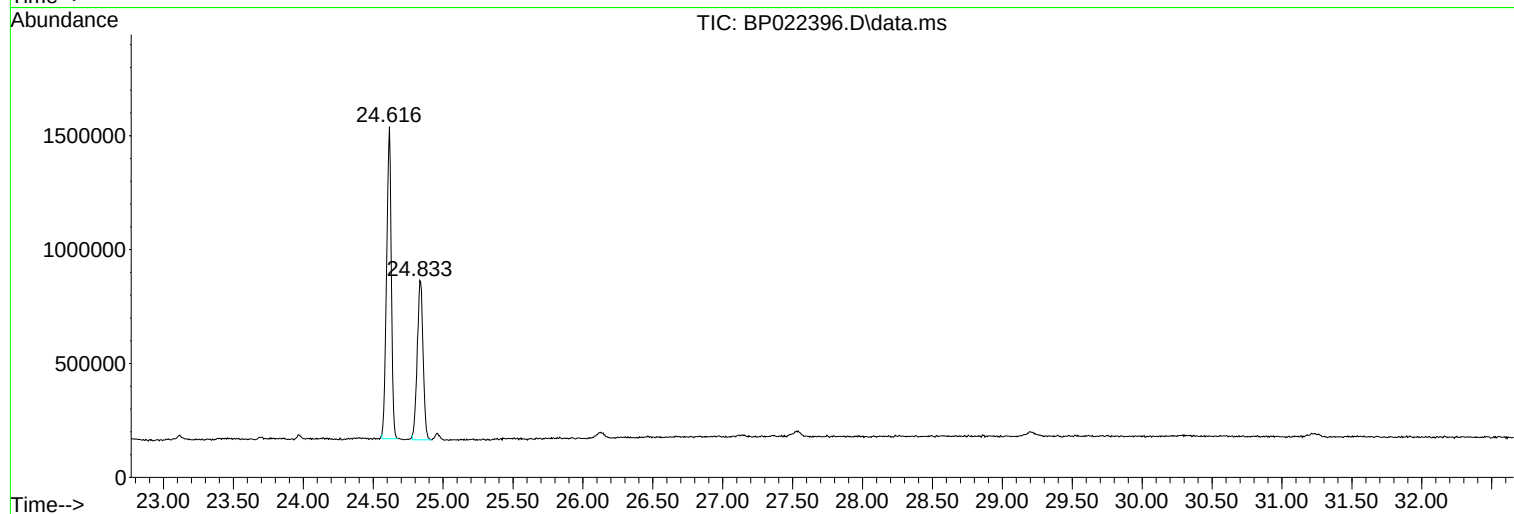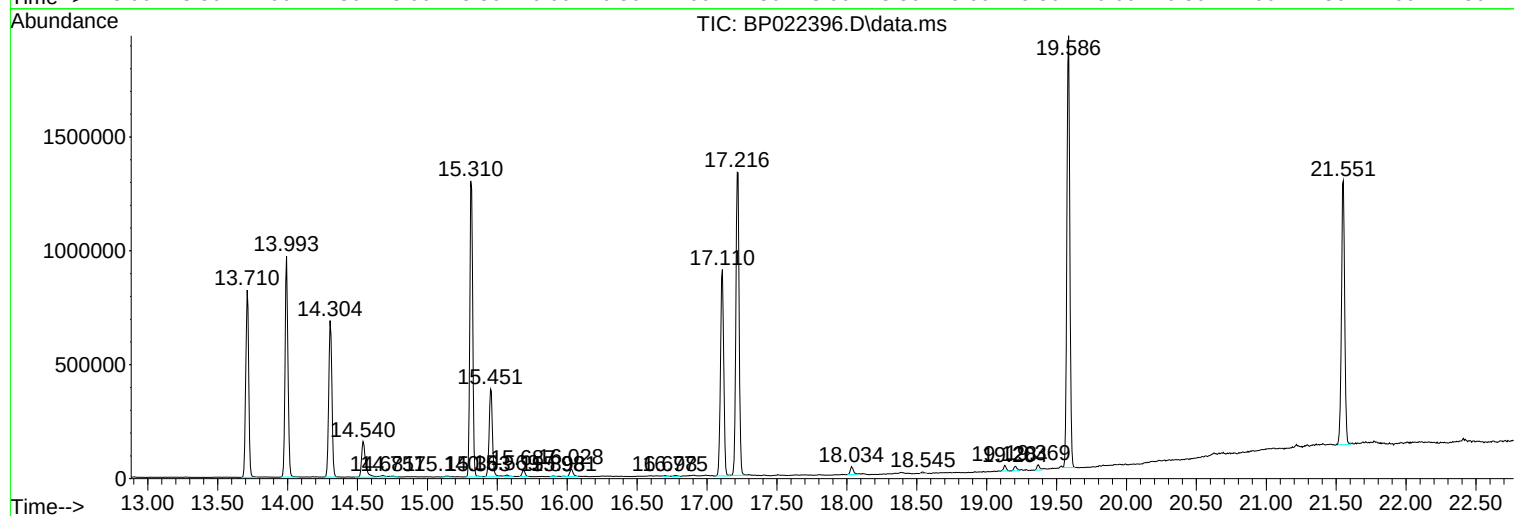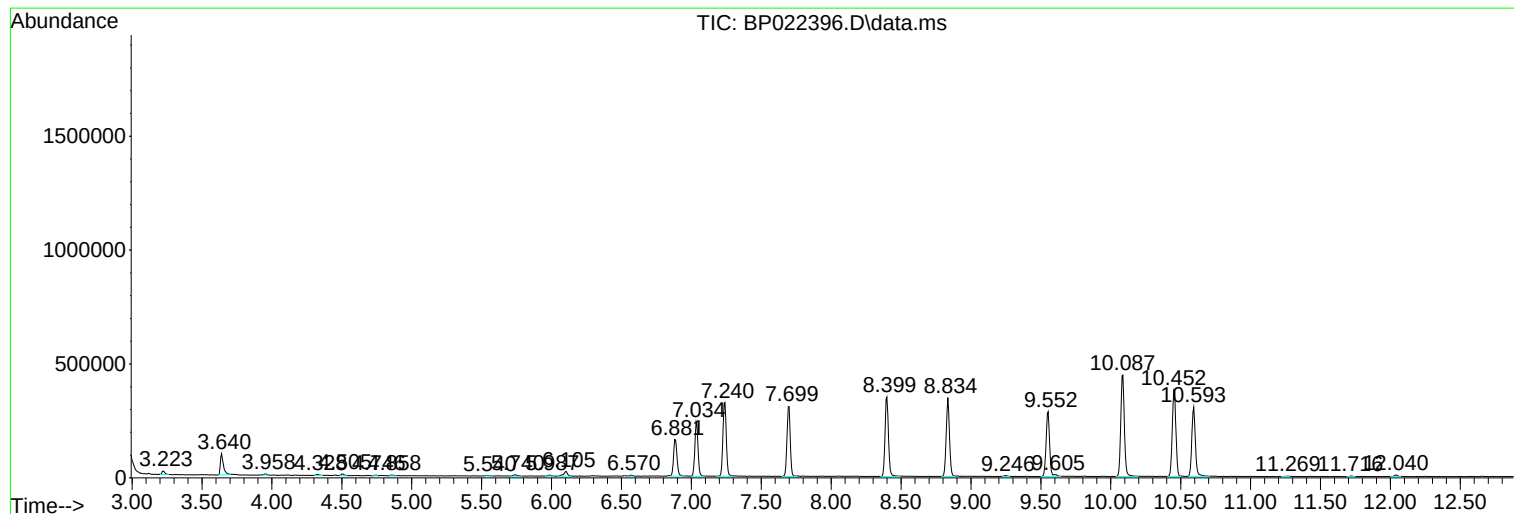

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022396.D
Acq On : 15 Oct 2024 19:40
Operator : RC/JU
Sample : P4349-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022396.D
Acq On : 15 Oct 2024 19:40
Operator : RC/JU
Sample : P4349-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc