

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022399.D
 Acq On : 15 Oct 2024 21:42
 Operator : RC/JU
 Sample : P4349-18
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	48	rVB	18210	25902	0.72%	0.093%
2	3.646	108	112	123	rVB	45942	70805	1.96%	0.255%
3	3.952	161	164	171	rVB2	4797	6861	0.19%	0.025%
4	6.887	657	663	676	rVB	108611	181118	5.02%	0.652%
5	7.040	680	689	698	rBV	264996	410200	11.37%	1.476%
6	7.240	715	723	734	rBV	334010	529881	14.69%	1.907%
7	7.699	793	801	810	rBV	310681	511235	14.17%	1.840%
8	8.399	912	920	931	rBV	291327	488544	13.54%	1.758%
9	8.840	986	995	1008	rBV	342307	599488	16.62%	2.158%
10	9.251	1059	1065	1071	rVB2	7941	13887	0.38%	0.050%
11	9.393	1084	1089	1095	rBV4	9039	15319	0.42%	0.055%
12	9.551	1108	1116	1126	rBV	303084	543560	15.07%	1.957%
13	10.087	1199	1207	1226	rBV	481842	868346	24.07%	3.126%
14	10.457	1261	1270	1279	rBV	419698	720516	19.97%	2.593%
15	10.598	1286	1294	1306	rBV	96345	175256	4.86%	0.631%
16	11.363	1420	1424	1431	rBV9	2306	5229	0.14%	0.019%
17	11.722	1481	1485	1492	rVB5	4480	7968	0.22%	0.029%
18	12.045	1534	1540	1548	rBV3	7594	14712	0.41%	0.053%
19	13.710	1816	1823	1837	rBV	1050887	1375222	38.12%	4.950%
20	13.992	1862	1871	1882	rBV	940075	1509521	41.85%	5.433%
21	14.304	1917	1924	1935	rBV	781113	1127279	31.25%	4.058%
22	14.534	1957	1963	1980	rBV	95171	206934	5.74%	0.745%
23	14.739	1994	1998	2003	rVB8	4335	7682	0.21%	0.028%
24	15.310	2088	2095	2107	rBV	1431564	2095216	58.08%	7.542%
25	15.439	2110	2117	2127	rBV	521485	752136	20.85%	2.707%
26	15.551	2132	2136	2142	rVB6	6010	12039	0.33%	0.043%
27	15.681	2153	2158	2166	rBV	135449	177487	4.92%	0.639%
28	15.886	2186	2193	2194	rBV5	2447	4249	0.12%	0.015%
29	16.028	2211	2217	2224	rBV	31591	49273	1.37%	0.177%
30	16.586	2308	2312	2316	rBV7	2289	3998	0.11%	0.014%
31	17.104	2392	2400	2406	rBV	1057218	1567527	43.45%	5.642%
32	17.198	2410	2416	2427	rBV2	1573040	2604169	72.19%	9.374%
33	17.392	2447	2449	2455	rVB7	4070	4992	0.14%	0.018%
34	18.027	2552	2557	2566	rBV2	46719	69830	1.94%	0.251%
35	18.345	2608	2611	2614	rVV5	4532	7043	0.20%	0.025%
36	19.122	2739	2743	2748	rBV3	25726	36760	1.02%	0.132%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022399.D
Acq On : 15 Oct 2024 21:42
Operator : RC/JU
Sample : P4349-18
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	19.198	2751	2756	2761	rBV2	25359	46450	1.29%	0.167%
38	19.369	2782	2785	2789	rVB5	15023	18800	0.52%	0.068%
39	19.522	2809	2811	2814	rVB4	8952	7666	0.21%	0.028%
40	19.574	2814	2820	2831	rVB2	2166197	3228231	89.49%	11.620%
41	21.210	3095	3098	3106	rVB5	47498	72792	2.02%	0.262%
42	21.539	3148	3154	3161	rBV	1350895	1942660	53.85%	6.993%
43	24.598	3664	3674	3687	rVB	1139798	3607276	100.00%	12.984%
44	24.821	3703	3712	3724	rVB	775833	2057944	57.05%	7.407%




Sum of corrected areas: 27782003

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022399.D
Acq On : 15 Oct 2024 21:42
Operator : RC/JU
Sample : P4349-18
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

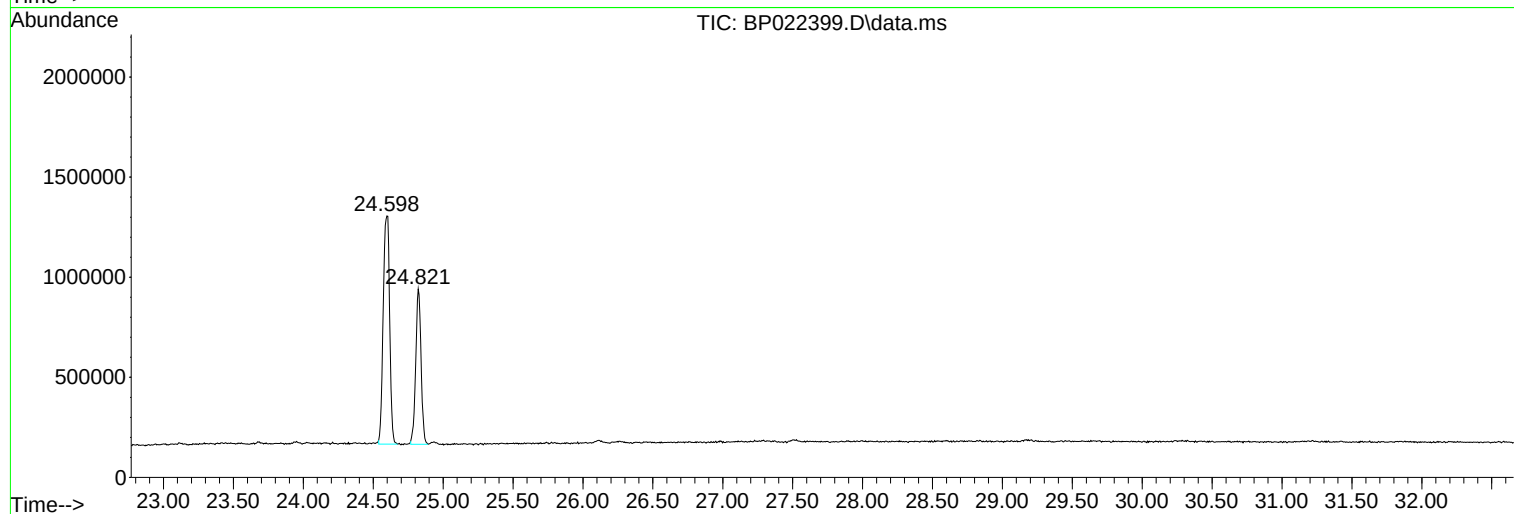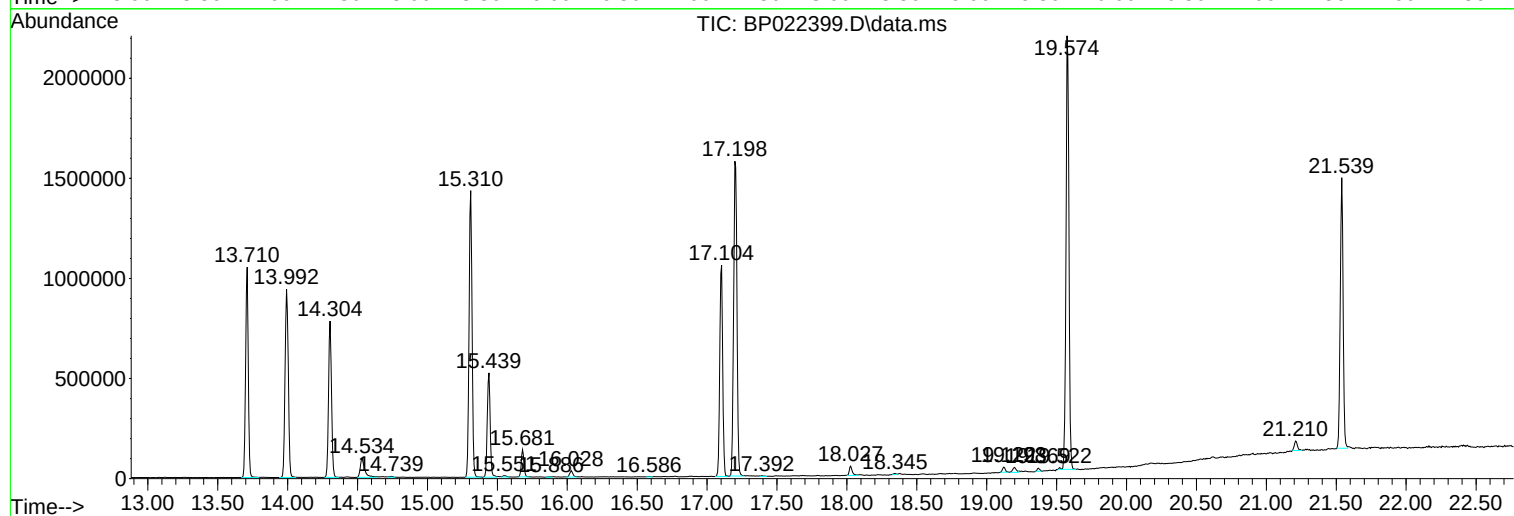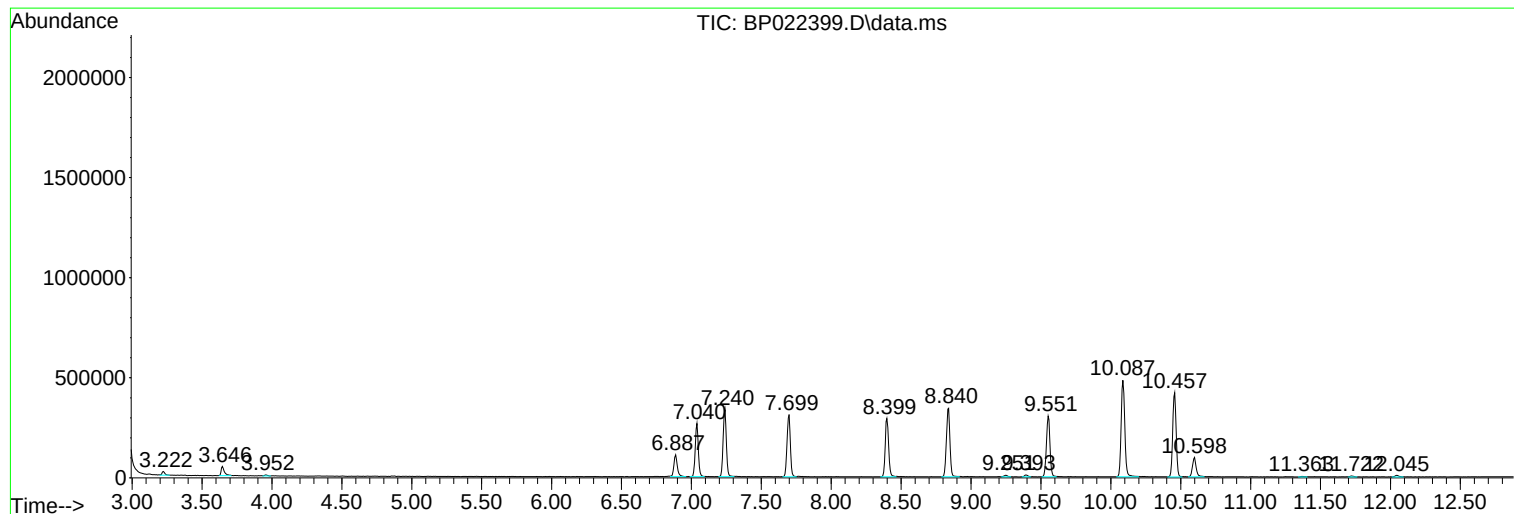

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022399.D
Acq On : 15 Oct 2024 21:42
Operator : RC/JU
Sample : P4349-18
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.681	3.15 ng/ul	177487	Acenaphthene-d10	14.304

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	93
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	81

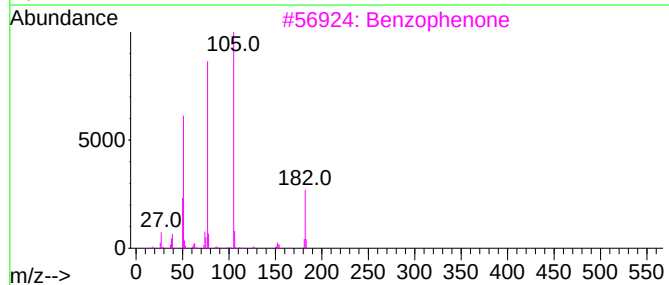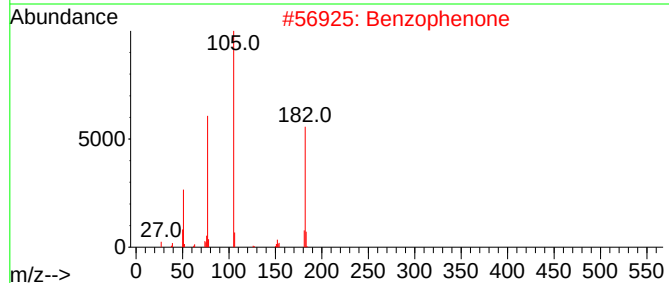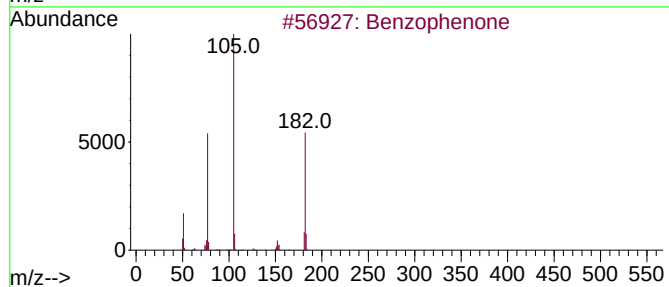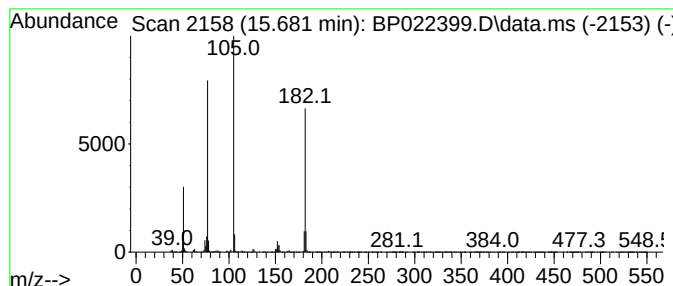

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022399.D
Acq On : 15 Oct 2024 21:42
Operator : RC/JU
Sample : P4349-18
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.681	3.1	ng/ul	177487	3	14.304	1127280	20.0