

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022400.D
 Acq On : 15 Oct 2024 22:23
 Operator : RC/JU
 Sample : P4349-19
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	37	40	48	rVB3	15437	25977	0.93%	0.108%
2	3.640	107	111	120	rBV	62414	98249	3.52%	0.409%
3	3.952	160	164	171	rVB	10802	15475	0.55%	0.064%
4	5.387	403	408	411	rBV5	2253	3866	0.14%	0.016%
5	5.746	465	469	472	rVB5	2324	3382	0.12%	0.014%
6	6.881	656	662	672	rVB	77791	137905	4.94%	0.574%
7	7.034	682	688	701	rVB	216404	354734	12.70%	1.477%
8	7.240	713	723	736	rBV	270550	467379	16.73%	1.946%
9	7.693	792	800	809	rBV	274672	480993	17.21%	2.003%
10	8.399	912	920	930	rBV2	234616	407018	14.57%	1.695%
11	8.834	987	994	1005	rBV	305624	522664	18.71%	2.176%
12	9.246	1059	1064	1070	rBV2	5128	8950	0.32%	0.037%
13	9.546	1108	1115	1130	rBV	289724	476125	17.04%	1.982%
14	10.087	1199	1207	1220	rBV	430232	737759	26.40%	3.072%
15	10.452	1262	1269	1282	rVB	423148	674037	24.12%	2.806%
16	10.587	1285	1292	1305	rBV	336125	643977	23.05%	2.681%
17	11.110	1375	1381	1393	rBV8	2817	6766	0.24%	0.028%
18	11.722	1479	1485	1490	rVV4	4229	6742	0.24%	0.028%
19	12.040	1535	1539	1547	rBV	6631	10417	0.37%	0.043%
20	12.651	1639	1643	1648	rBV7	2436	4059	0.15%	0.017%
21	13.710	1816	1823	1838	rBV	706619	1125894	40.30%	4.688%
22	13.822	1838	1842	1846	rVB6	1706	3015	0.11%	0.013%
23	13.998	1864	1872	1884	rBV	834674	1298973	46.49%	5.408%
24	14.310	1916	1925	1932	rBV	689357	1060130	37.94%	4.414%
25	14.534	1956	1963	1981	rBV	73242	147390	5.28%	0.614%
26	14.740	1994	1998	2008	rVB8	8212	15943	0.57%	0.066%
27	14.969	2032	2037	2042	rBV8	1751	3251	0.12%	0.014%
28	15.140	2060	2066	2070	rVB3	3174	5318	0.19%	0.022%
29	15.322	2088	2097	2105	rBV	1072517	1744734	62.44%	7.264%
30	15.445	2111	2118	2131	rBV	395392	562441	20.13%	2.342%
31	15.563	2134	2138	2144	rVB3	6229	10445	0.37%	0.043%
32	16.040	2209	2219	2227	rBV	24341	41224	1.48%	0.172%
33	16.881	2358	2362	2371	rVB9	2750	6621	0.24%	0.028%
34	17.110	2394	2401	2411	rBV	942877	1474554	52.77%	6.140%
35	17.210	2411	2418	2430	rVB	1469397	2122453	75.96%	8.837%
36	17.410	2449	2452	2459	rBV2	7237	9968	0.36%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022400.D
Acq On : 15 Oct 2024 22:23
Operator : RC/JU
Sample : P4349-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	17.798	2515	2518	2521	rBV5	5202	6070	0.22%	0.025%
38	18.039	2556	2559	2567	rBV9	7916	14351	0.51%	0.060%
39	19.128	2741	2744	2750	rBV3	17147	27703	0.99%	0.115%
40	19.210	2754	2758	2763	rVV	18754	28554	1.02%	0.119%
41	19.592	2816	2823	2831	rBV	1913043	2660763	95.23%	11.078%
42	21.539	3148	3154	3168	rVB	1196275	1867547	66.84%	7.776%
43	24.610	3666	3676	3687	rVB	1149069	2794092	100.00%	11.634%
44	24.827	3704	3713	3726	rVB	678070	1899459	67.98%	7.909%




Sum of corrected areas: 24017367

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022400.D
Acq On : 15 Oct 2024 22:23
Operator : RC/JU
Sample : P4349-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

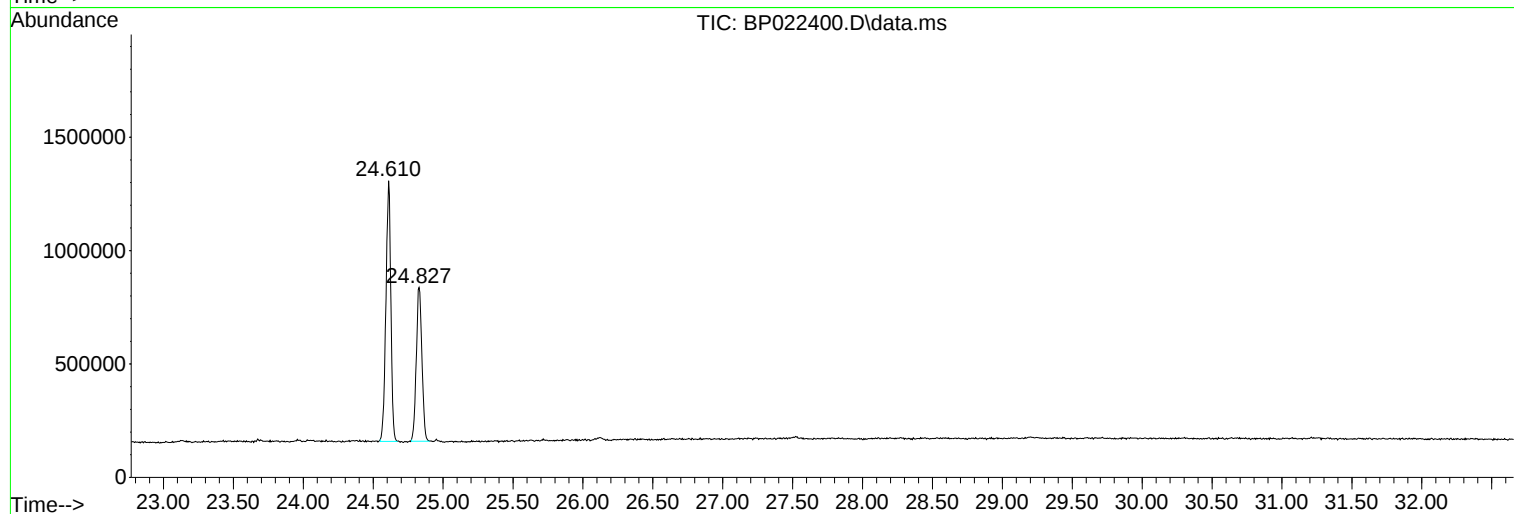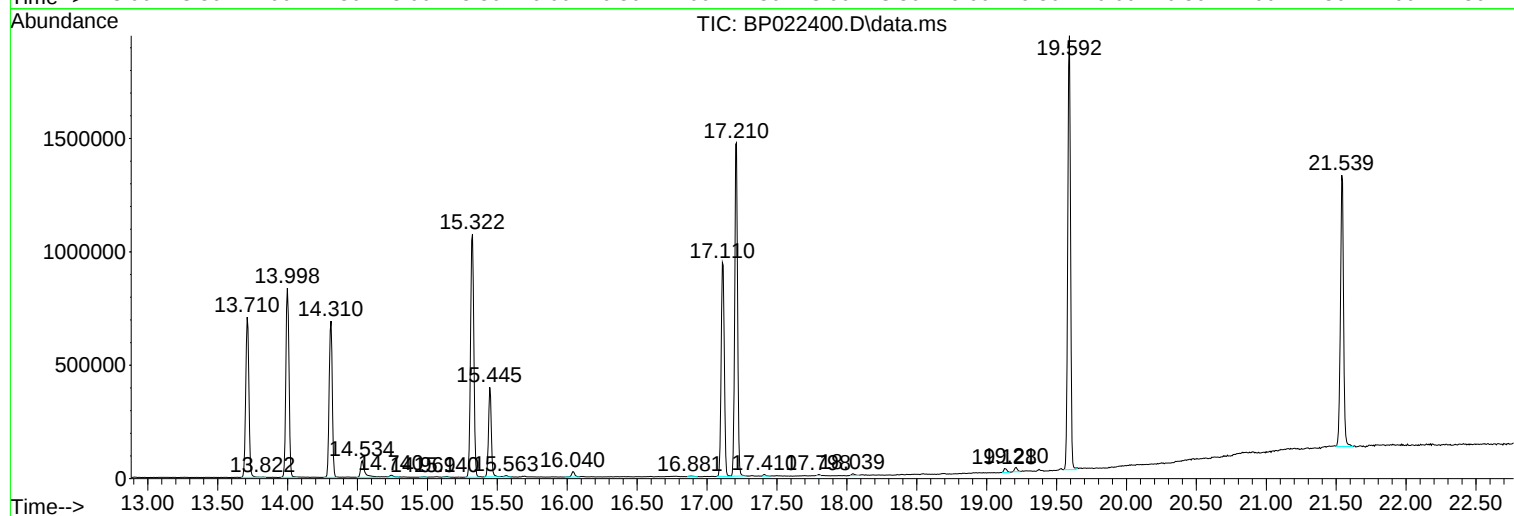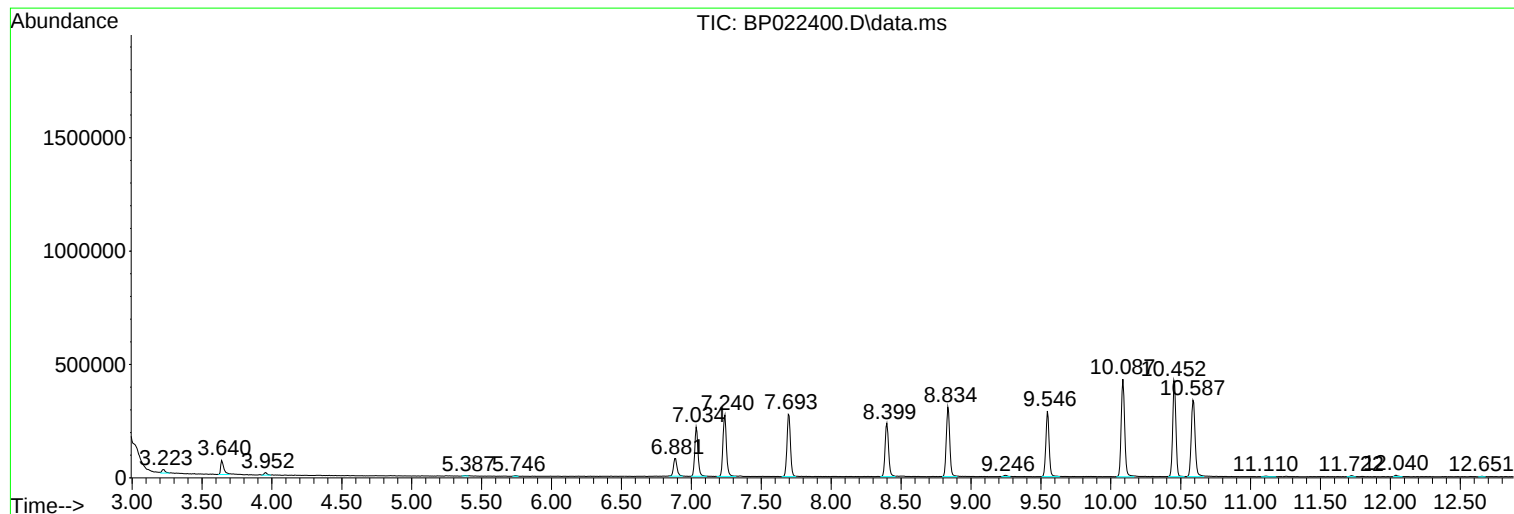

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022400.D
Acq On : 15 Oct 2024 22:23
Operator : RC/JU
Sample : P4349-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022400.D
Acq On : 15 Oct 2024 22:23
Operator : RC/JU
Sample : P4349-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------