

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
 Data File : BP022404.D
 Acq On : 16 Oct 2024 01:46
 Operator : RC/JU
 Sample : P4349-20
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	46	rVB	22344	28909	0.75%	0.096%
2	3.640	108	111	123	rBV	56635	95076	2.46%	0.316%
3	3.952	161	164	170	rVB3	5056	7620	0.20%	0.025%
4	4.505	255	258	263	rVB5	3657	4781	0.12%	0.016%
5	6.881	657	662	675	rVB	108403	190798	4.93%	0.634%
6	7.034	681	688	698	rBV	305705	495064	12.79%	1.645%
7	7.240	715	723	733	rBV	380682	625064	16.15%	2.078%
8	7.322	733	737	742	rVB8	2245	4323	0.11%	0.014%
9	7.693	791	800	809	rBV	359203	579645	14.98%	1.927%
10	8.393	912	919	936	rBV	321726	538411	13.91%	1.790%
11	8.834	986	994	1007	rBV	432330	711987	18.40%	2.366%
12	9.251	1060	1065	1069	rBV2	7149	11105	0.29%	0.037%
13	9.393	1084	1089	1093	rBV2	6051	10269	0.27%	0.034%
14	9.546	1108	1115	1126	rBV	377317	630023	16.28%	2.094%
15	10.081	1196	1206	1222	rBV	550269	1009671	26.09%	3.356%
16	10.446	1258	1268	1277	rBV	404718	774641	20.02%	2.575%
17	10.593	1284	1293	1302	rBV	112639	211652	5.47%	0.703%
18	11.722	1481	1485	1490	rVB3	4187	6642	0.17%	0.022%
19	12.040	1532	1539	1546	rBV2	10462	17825	0.46%	0.059%
20	13.716	1816	1824	1833	rBV	1137255	1589881	41.09%	5.284%
21	13.992	1863	1871	1885	rBV	965536	1742548	45.03%	5.792%
22	14.304	1916	1924	1935	rBV	677109	1173187	30.32%	3.899%
23	14.528	1956	1962	1976	rBV2	81592	188478	4.87%	0.626%
24	14.751	1997	2000	2005	rVB7	4240	6472	0.17%	0.022%
25	15.122	2058	2063	2069	rBV9	2371	4995	0.13%	0.017%
26	15.310	2088	2095	2103	rBV	1625158	2411013	62.31%	8.014%
27	15.451	2113	2119	2130	rBV	632007	813365	21.02%	2.703%
28	15.557	2134	2137	2142	rVB4	8769	12882	0.33%	0.043%
29	15.686	2151	2159	2168	rBV	60087	106599	2.75%	0.354%
30	16.022	2211	2216	2225	rBV	24535	45617	1.18%	0.152%
31	16.122	2229	2233	2240	rVB10	2502	4434	0.11%	0.015%
32	16.575	2308	2310	2315	rBV6	2641	3895	0.10%	0.013%
33	16.886	2357	2363	2371	rVB8	3398	8378	0.22%	0.028%
34	17.104	2393	2400	2407	rBV	1064195	1560886	40.34%	5.188%
35	17.204	2411	2417	2427	rVV2	2030939	2821614	72.92%	9.378%
36	17.692	2497	2500	2506	rVB8	2549	4084	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022404.D
Acq On : 16 Oct 2024 01:46
Operator : RC/JU
Sample : P4349-20
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	18.033	2552	2558	2567	rBV3	36732	67958	1.76%	0.226%
38	18.539	2640	2644	2649	rBV7	6794	11911	0.31%	0.040%
39	19.122	2739	2743	2748	rVB	26432	38245	0.99%	0.127%
40	19.198	2752	2756	2761	rBV	25253	42150	1.09%	0.140%
41	19.363	2780	2784	2790	rBV4	27160	43334	1.12%	0.144%
42	19.586	2814	2822	2831	rBV	2199229	3504663	90.57%	11.649%
43	21.216	3096	3099	3104	rBV4	31962	48514	1.25%	0.161%
44	21.545	3148	3155	3162	rBV2	1216572	1982309	51.23%	6.589%
45	24.598	3664	3674	3685	rVB	1499194	3869354	100.00%	12.861%
46	24.827	3705	3713	3725	rVB	740327	2026078	52.36%	6.734%




Sum of corrected areas: 30086350

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022404.D
Acq On : 16 Oct 2024 01:46
Operator : RC/JU
Sample : P4349-20
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

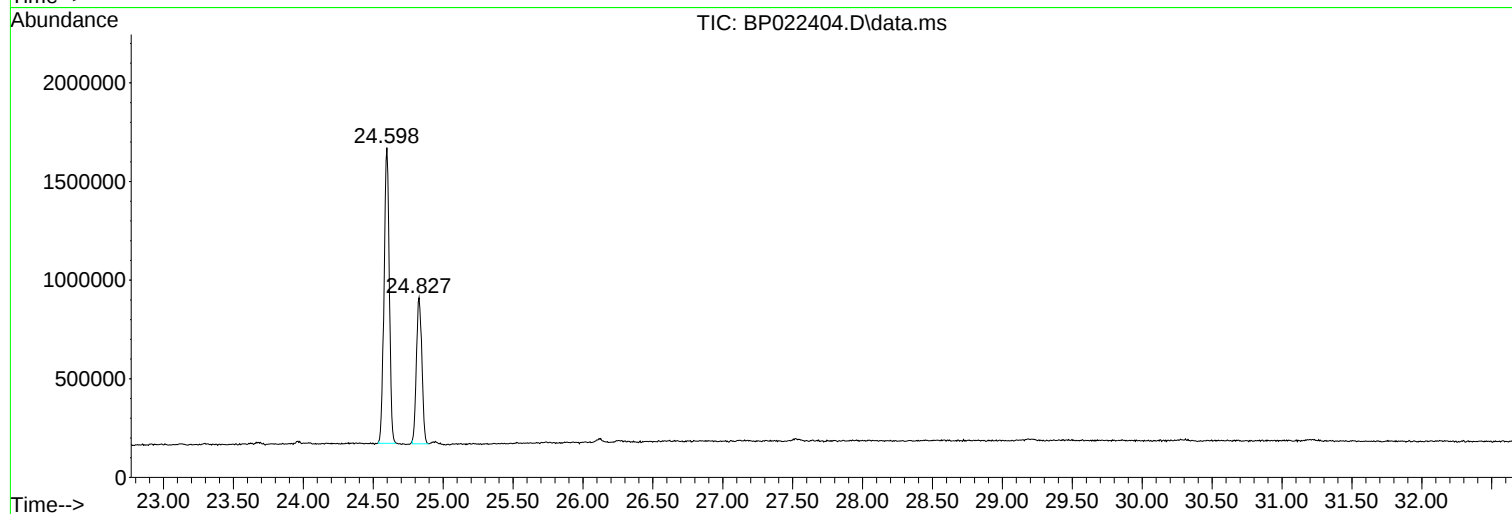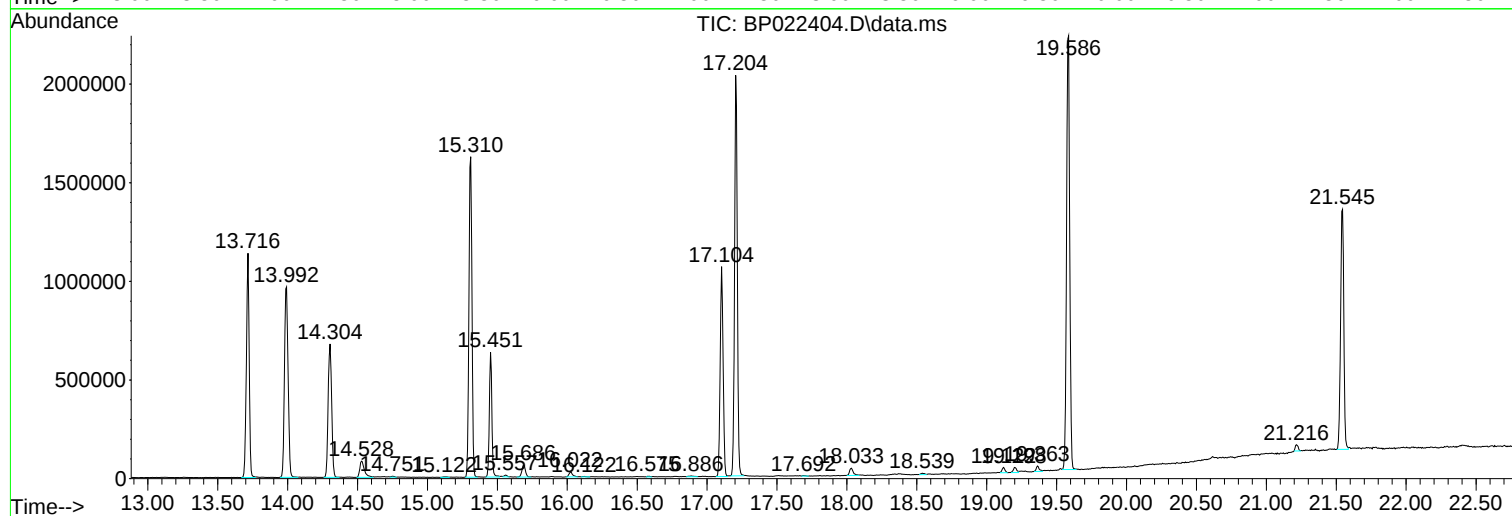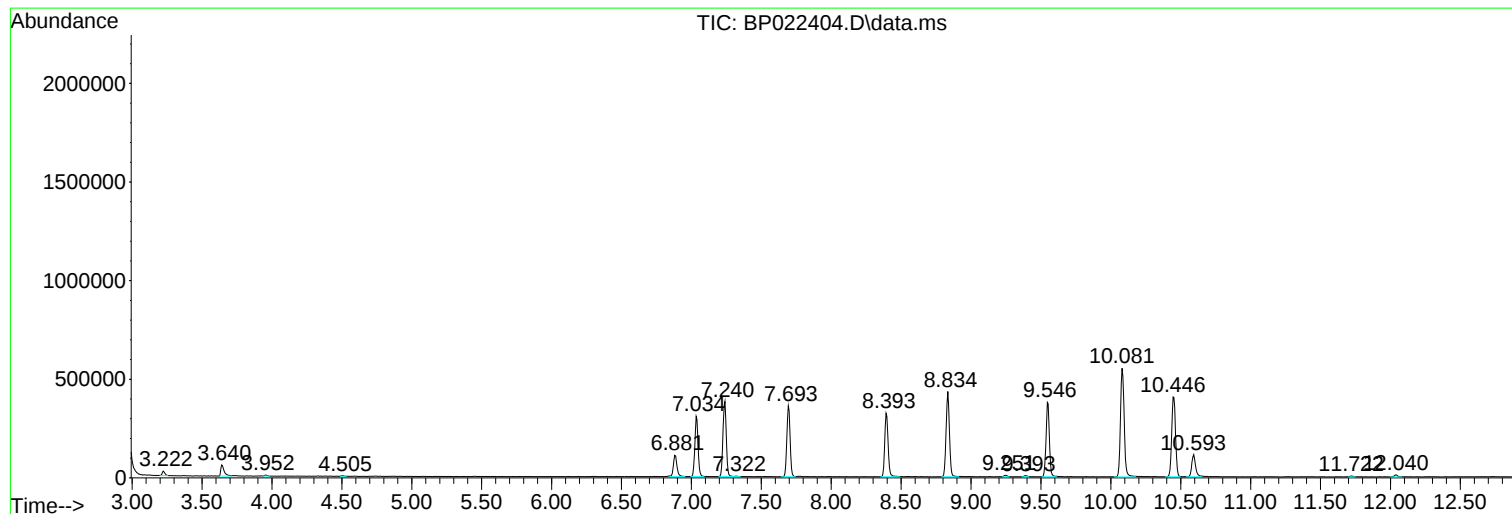

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022404.D
Acq On : 16 Oct 2024 01:46
Operator : RC/JU
Sample : P4349-20
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101424\
Data File : BP022404.D
Acq On : 16 Oct 2024 01:46
Operator : RC/JU
Sample : P4349-20
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc