

Data File : BP000733.D
Acq On : 15 Oct 2019 00:56
Operator : JU
Sample : PB123959BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK59

Quant Time: Oct 15 03:57:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 15 03:51:25 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	180136	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	700347	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	391159	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	724752	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	616645	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	642183	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.36	96	36318	8.36	ng/uL	0.00
5) Phenol-d5	6.39	99	576110	41.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	287407	41.37	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	486295	41.54	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	450303	42.42	ng/ul	0.00
19) Nitrobenzene-d5	7.31	128	228420	42.91	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	247918	43.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	427204	39.37	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	611821	50.70	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	1188990	43.42	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	1406334	41.75	ng/ul	0.00
52) 4-Nitrophenol-d4	9.91	143	170085	40.33	ng/ul	0.00
58) Fluorene-d10	10.32	176	979972	41.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	109971	31.86	ng/ul	0.00
71) Anthracene-d10	11.35	188	1437635	42.82	ng/ul	0.00
79) Pyrene-d10	12.73	212	1482897	42.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1368756	43.17	ng/ul	0.00

Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	7.13	70	9160	1.297	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data File : BP000733.D

```
Acq On       : 15 Oct 2019   00:56
Operator    : JU
Sample      : PB123959BL
Misc       :
ALS Vial    : 16      Sample Multip
```

Instrument :
BNA_P
ClientSampleId :
SBLK59

Quant Time: Oct 15 03:57:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 15 03:51:25 2019
Response via : Initial Calibration

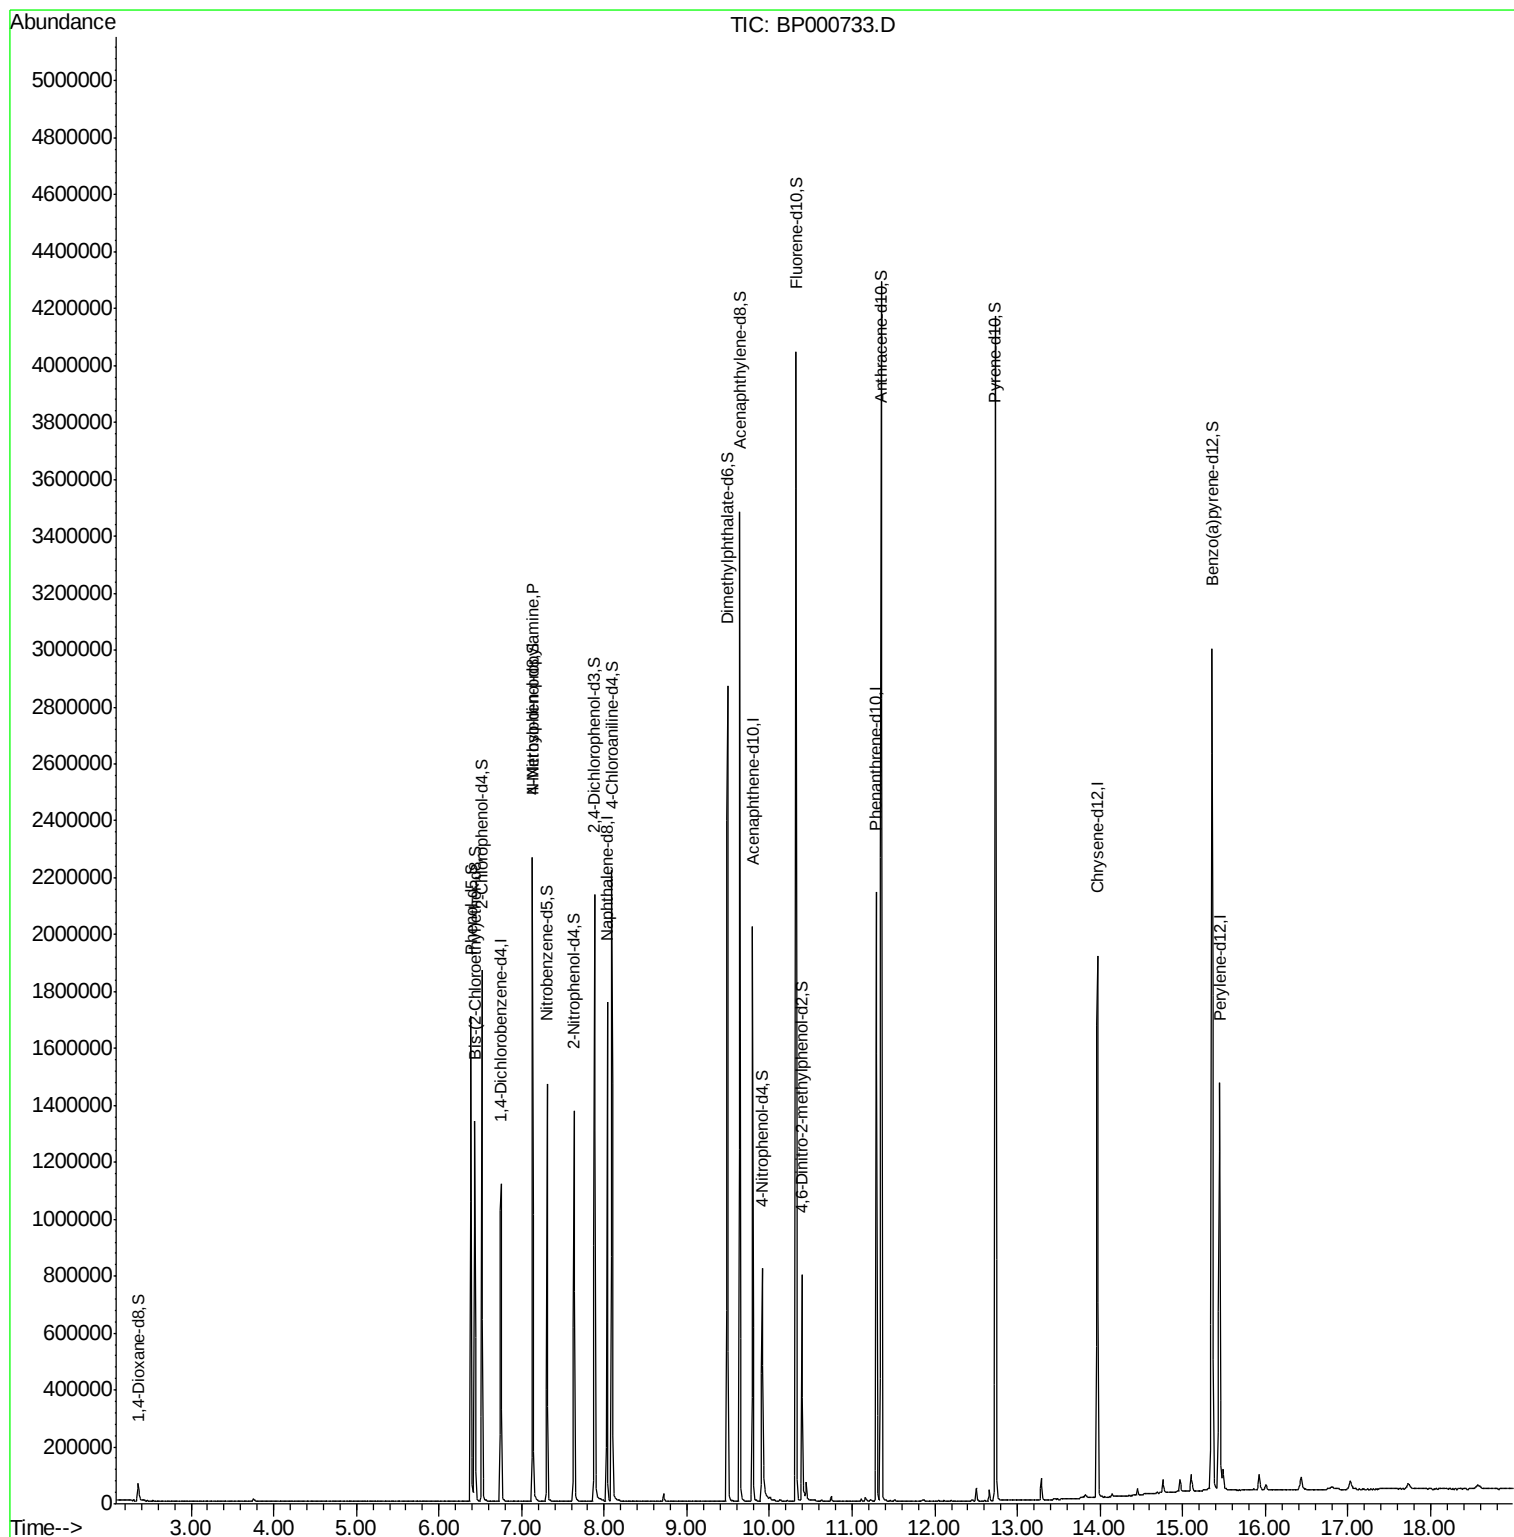

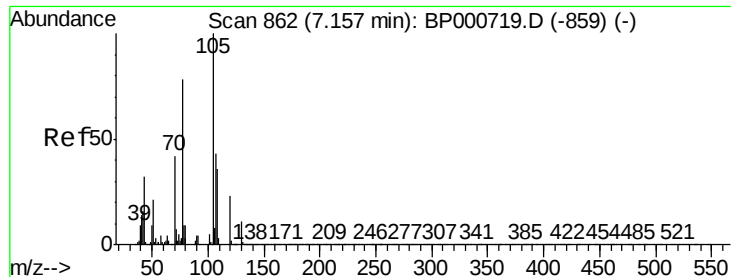

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.297 ng/ul
 RT: 7.13 min Scan# 858
 Delta R.T. -0.02 min
 Lab File: BP000733.D
 Acq: 15 Oct 2019 00:56

Instrument :
 BNA_P
 ClientSampleId :
 SBLK59

Tgt Ion:	70	Resp:	9160
Ion	Ratio	Lower	Upper
70	100		
42	266.8	33.5	50.3#
101	0.1	9.6	14.4#
130	0.2	21.8	32.8#

