

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101519\
 Data File : BP000727.D
 Acq On : 14 Oct 2019 22:31
 Operator : JU
 Sample : K5097-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JLMF5

Quant Time: Oct 15 03:55:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 15 03:51:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	225565	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	849206	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	464428	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	862524	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	785967	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	869216	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.36	96	31751	5.84	ng/uL	0.00
5) Phenol-d5	6.39	99	518353	29.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	270366	31.08	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	446102	30.43	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	416231	31.31	ng/ul	0.00
19) Nitrobenzene-d5	7.31	128	213193	33.03	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	233559	33.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	396834	30.16	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	549659	37.57	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	1069023	32.88	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	1302010	32.56	ng/ul	0.00
52) 4-Nitrophenol-d4	9.91	143	119860	23.94	ng/ul	0.00
58) Fluorene-d10	10.32	176	897549	32.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	82354	20.05	ng/ul	0.00
71) Anthracene-d10	11.35	188	1306601	32.70	ng/ul	0.00
79) Pyrene-d10	12.73	212	1386072	31.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1397197	32.56	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.40	94	62120	3.541	ng/ul 98
45) Dimethylphthalate	9.51	163	277086	8.554	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
Data File : BP000727.D
Acq On : 14 Oct 2019 22:31
Operator : JU
Sample : K5097-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JLMF5

Quant Time: Oct 15 03:55:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 15 03:51:25 2019
Response via : Initial Calibration

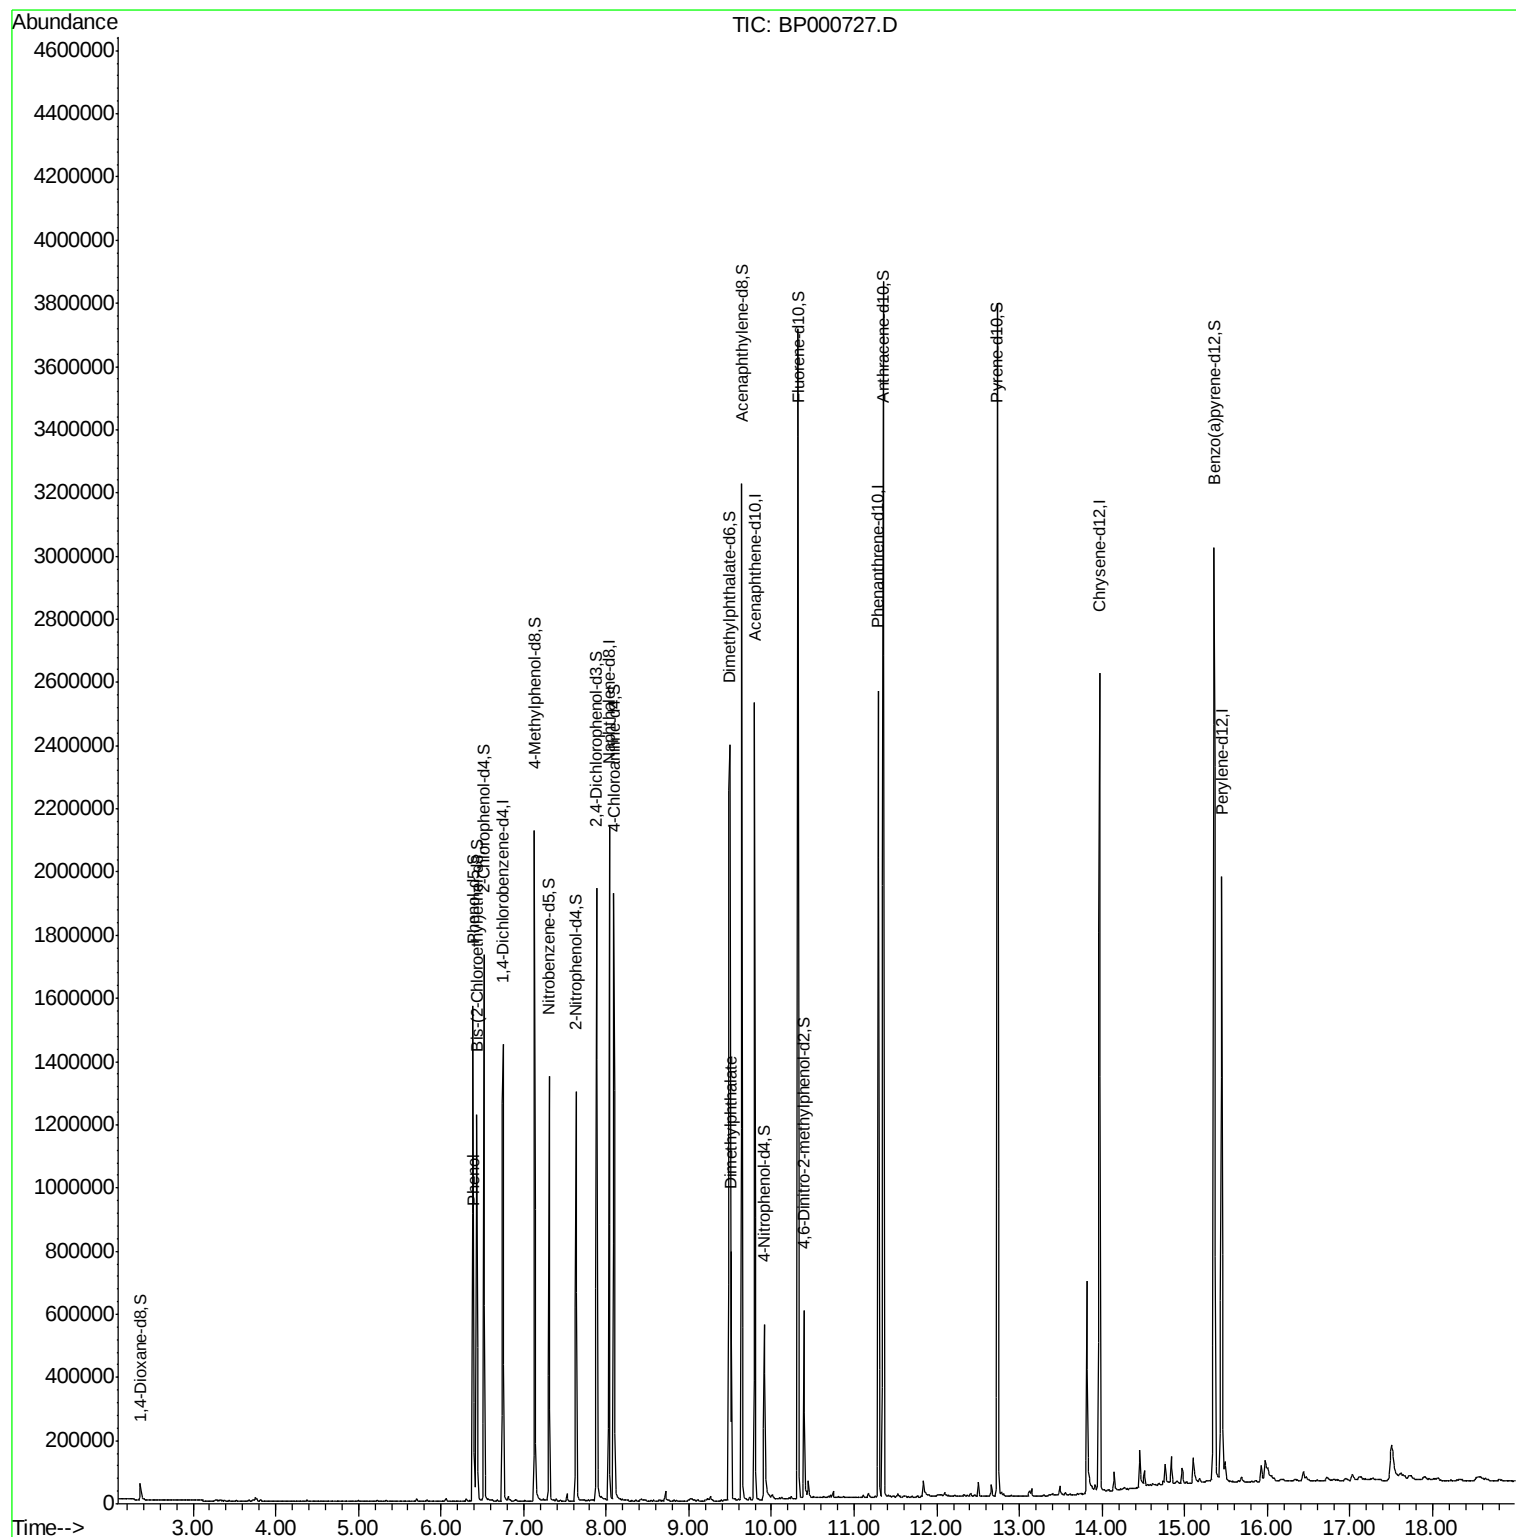

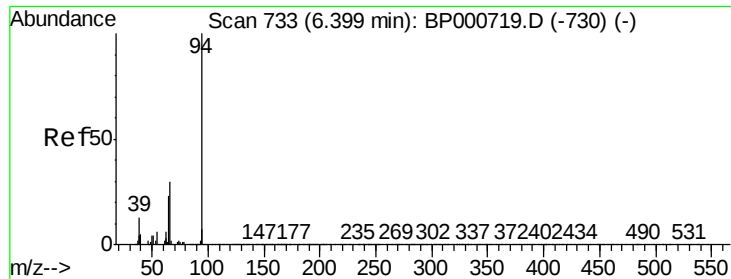

#6

Phenol

Concen: 3.541 ng/ul

RT: 6.40 min Scan# 733

Delta R.T. -0.00 min

Lab File: BP000727.D

Acq: 14 Oct 2019 22:31

Instrument :

BNA_P

ClientSampleId :

JLMF5





Tot Ion: 94 Resp: 62120

Ion Ratio Lower Upper

94 100

65 23.0 19.2 28.8

66 32.7 25.7 38.5

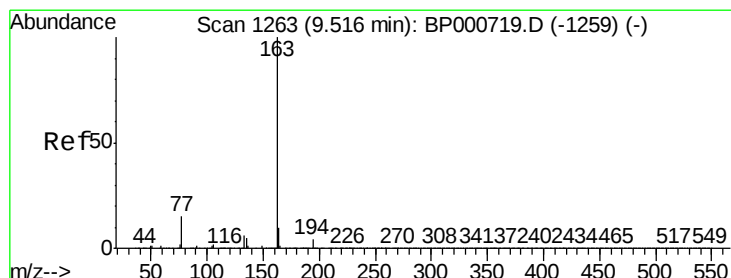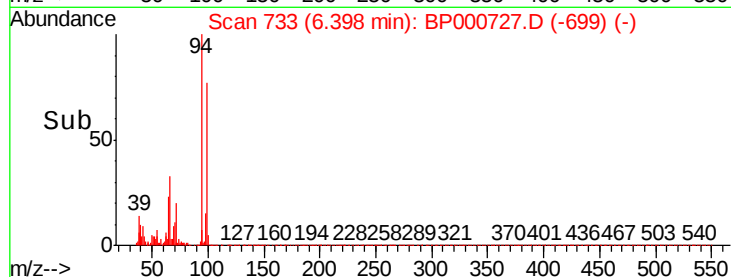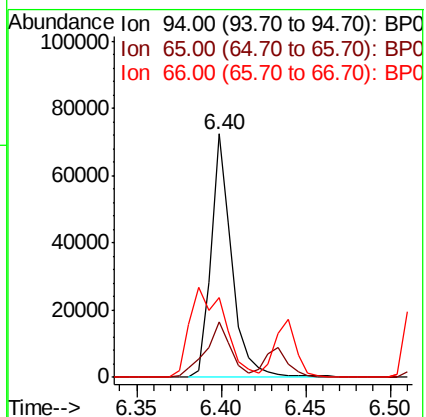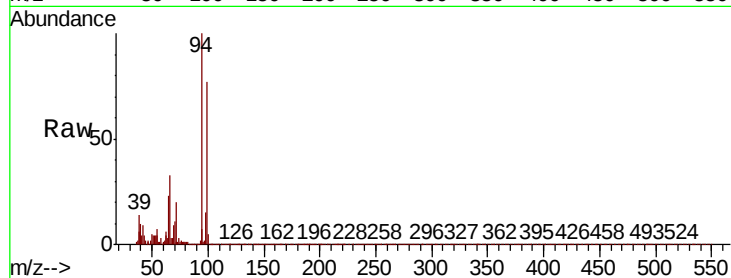

#45

Dimethylphthalate

Concen: 8.554 ng/ul

RT: 9.51 min Scan# 1262

Delta R.T. -0.01 min

Lab File: BP000727.D

Acq: 14 Oct 2019 22:31

Tgt Ion: 163 Resp: 277086

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.6 8.1 12.1

