

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
 Data File : BP000740.D
 Acq On : 15 Oct 2019 04:09
 Operator : JU
 Sample : K5296-02
 Misc : GCMS CONFIRMATION
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX9

Quant Time: Oct 15 05:45:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 15 03:51:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	262302	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	1033293	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	573359	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	1040229	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	806302	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	899961	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	0.00	99	0d	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0d	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0d	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0d	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul	
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul	
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul	
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
69) Pentachlorophenol	11.11	266	5267	1.049	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
Data File : BP000740.D
Acq On : 15 Oct 2019 04:09
Operator : JU
Sample : K5296-02
Misc : GCMS CONFIRMATION
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX9

Quant Time: Oct 15 05:45:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 15 03:51:25 2019
Response via : Initial Calibration

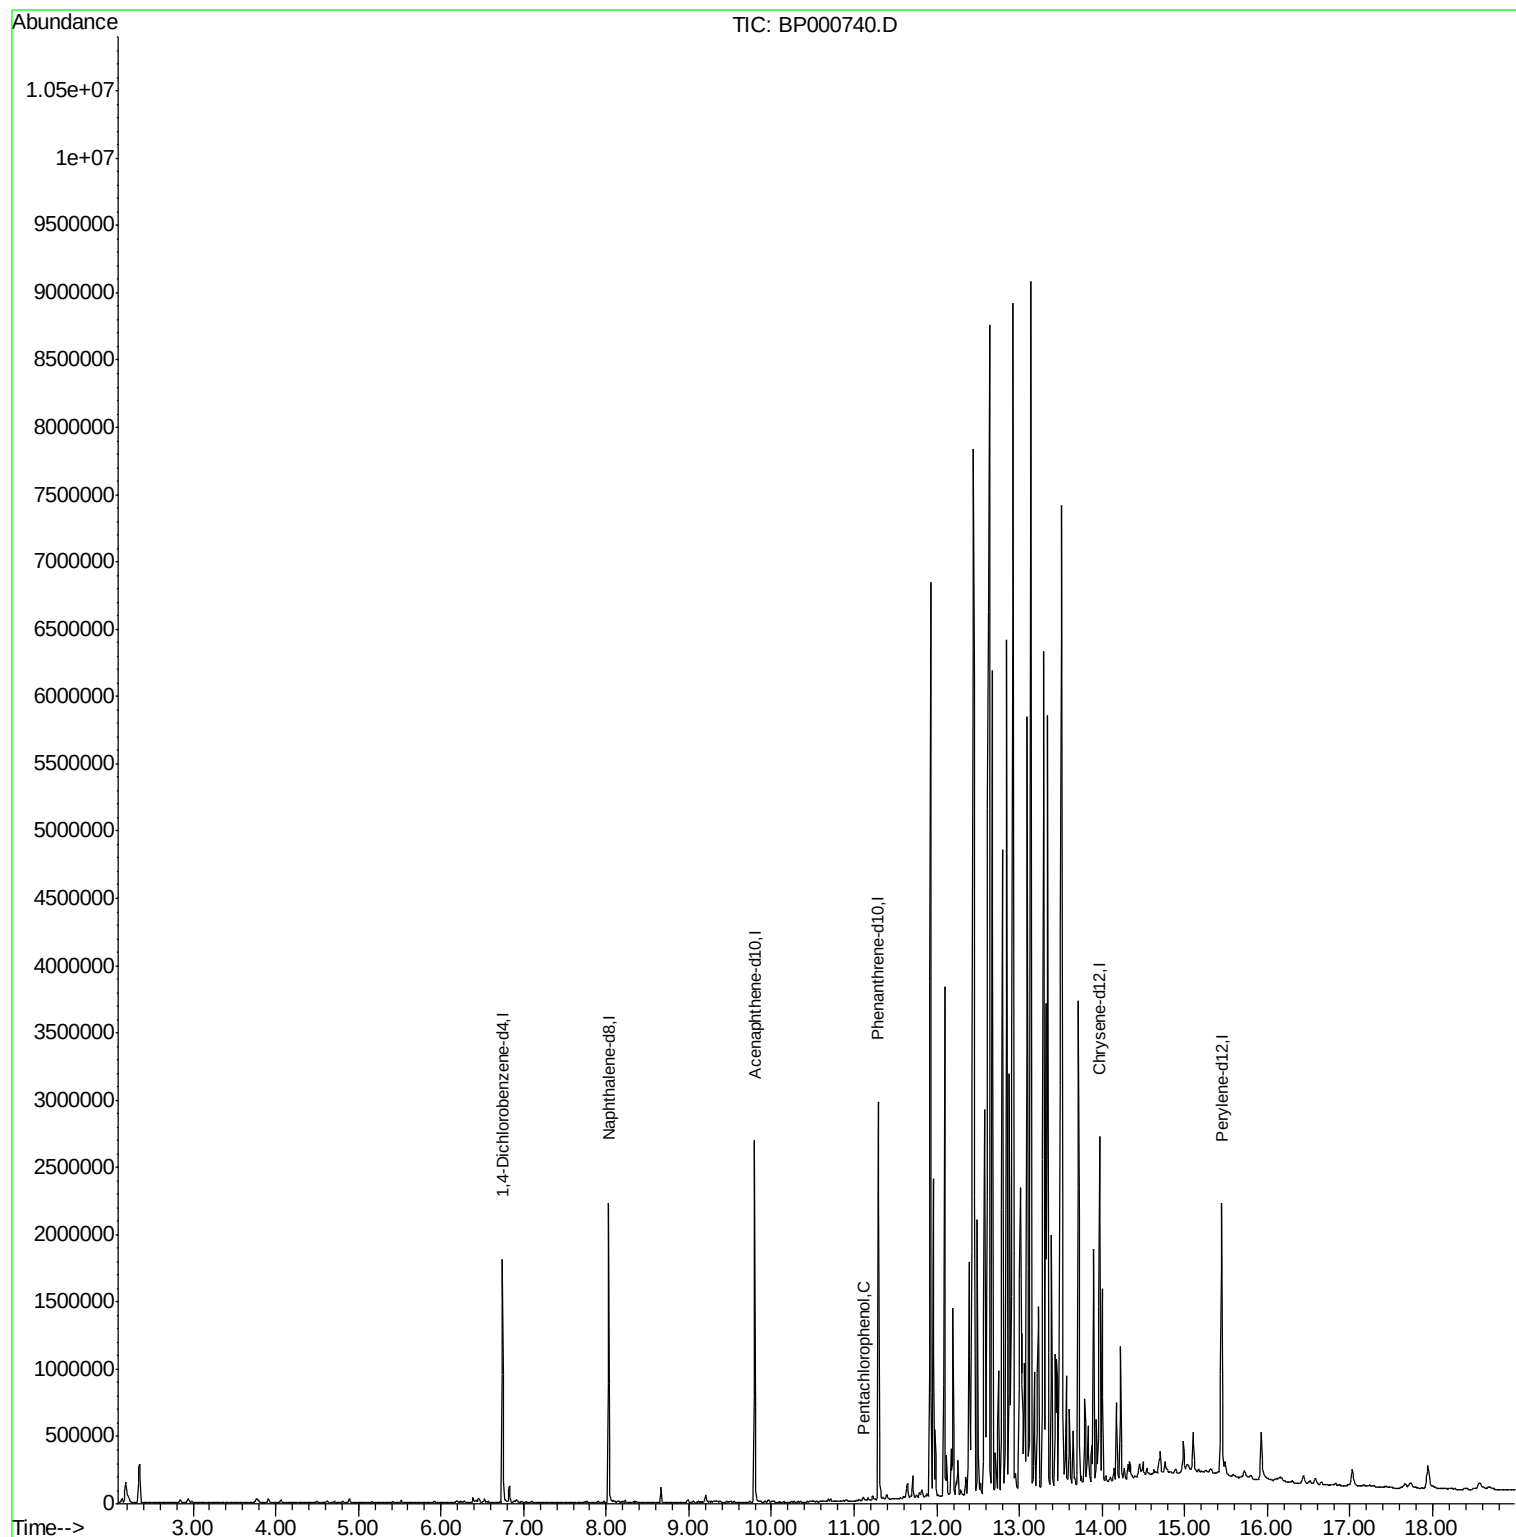

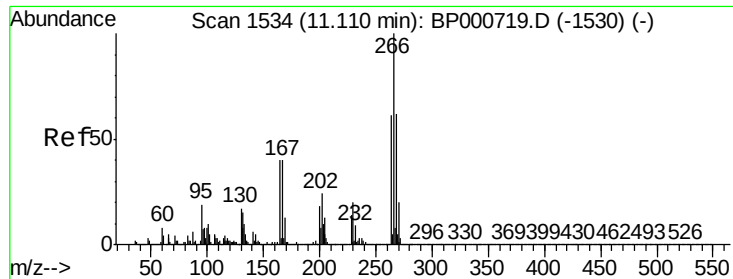

#69

Pentachlorophenol

Concen: 1.049 ng/ul

RT: 11.11 min Scan# 1534

Delta R.T. 0.00 min

Lab File: BP000740.D

Acq: 15 Oct 2019 04:09

Instrument :

BNA_P

ClientSampleId :

C0AX9


Tot Ion:266 Resp: 5267

Ion Ratio Lower Upper

266 100

264 61.8 49.6 74.4

268 62.5 49.6 74.4

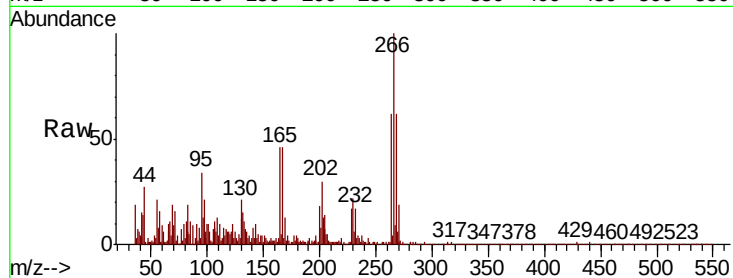

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

