

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
 Data File : BP000743.D
 Acq On : 15 Oct 2019 05:21
 Operator : JU
 Sample : K5296-05
 Misc : GCMS CONFIRMATION
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY2

Quant Time: Oct 15 06:27:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 15 03:51:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	229848	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	900329	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.79	164	504343	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	936746	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	808313	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	891918	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0d	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0d	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0d	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0d	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds				Ovalue
77) Fluoranthene	12.52	202	54740	1.046 ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
Data File : BP000743.D
Acq On : 15 Oct 2019 05:21
Operator : JU
Sample : K5296-05
Misc : GCMS CONFIRMATION
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY2

Quant Time: Oct 15 06:27:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 15 03:51:25 2019
Response via : Initial Calibration

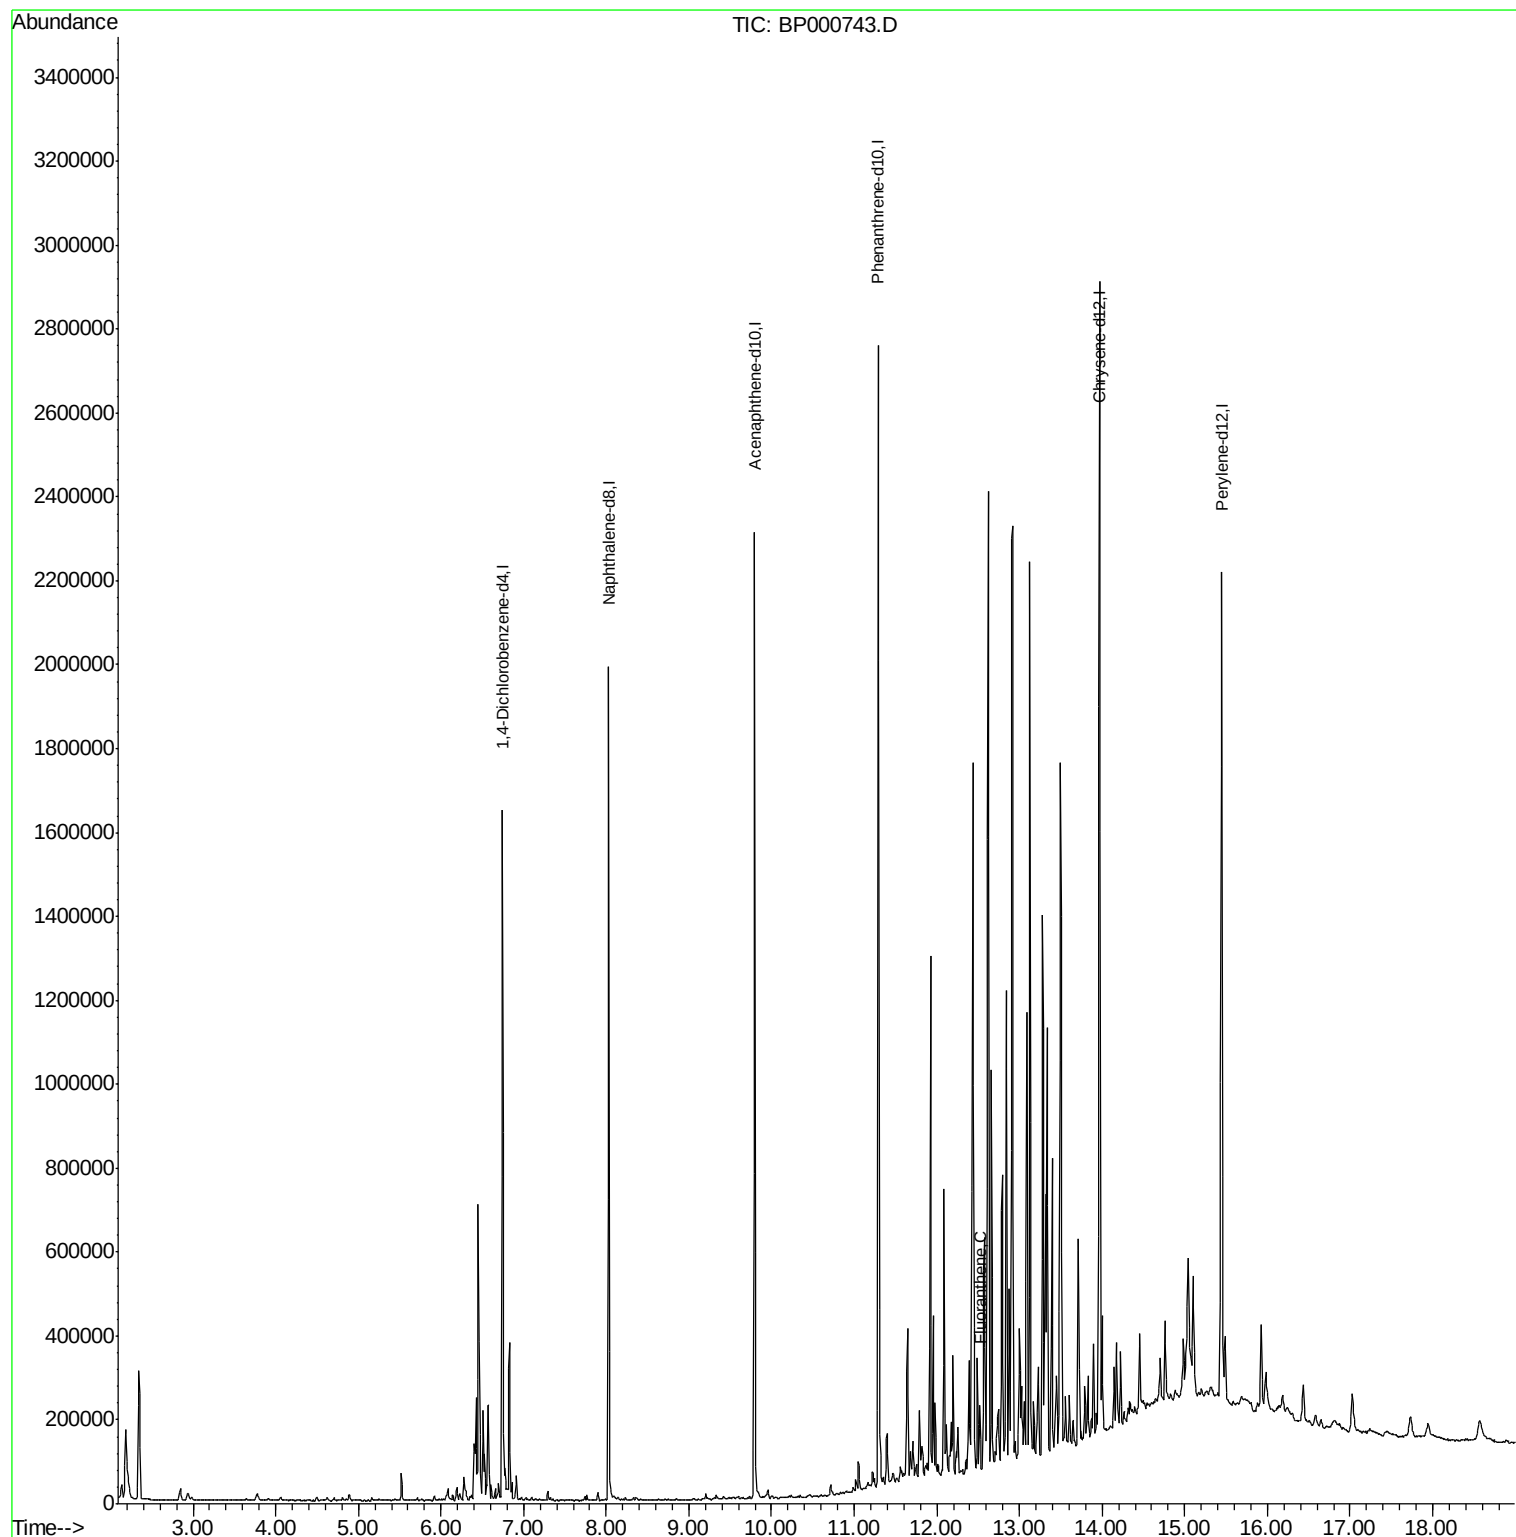


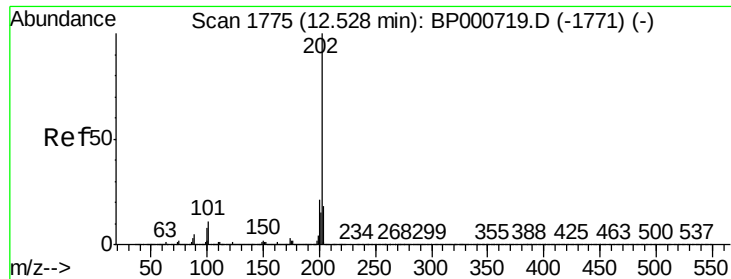

#77
 Fluoranthene
 Concen: 1.046 ng/ul
 RT: 12.52 min Scan# 1774
 Delta R.T. -0.01 min
 Lab File: BP000743.D
 Acq: 15 Oct 2019 05:21

Instrument :
 BNA_P
 ClientSampleId :
 C0AY2

Tot Ion:	202	Resp:	54740
Ion	Ratio	Lower	Upper
202	100		
101	12.1	9.8	14.6
100	8.9	7.2	10.8

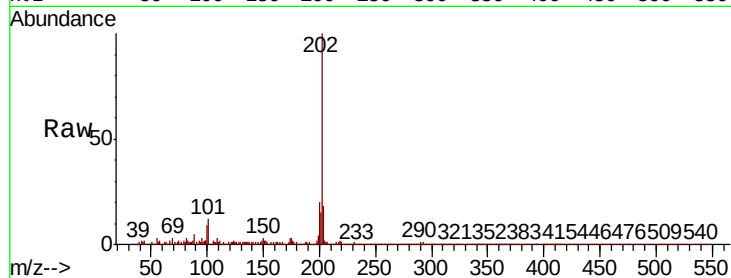

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): BF

