

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
 Data File : BP000733.D
 Acq On : 15 Oct 2019 00:56
 Operator : JU
 Sample : PB123959BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.358	43	46	56	rBV	61940	84749	2.11%	0.195%
2	3.752	278	283	289	rBV	8458	13020	0.32%	0.030%
3	6.387	727	731	735	rBV	1705994	1363210	33.95%	3.134%
4	6.434	735	739	750	rVB	1335827	1157414	28.82%	2.661%
5	6.522	750	754	757	rBV	1865202	1519751	37.84%	3.494%
6	6.752	789	793	808	rBV	1115483	991833	24.70%	2.280%
7	7.134	855	858	870	rVB	2262707	1757746	43.77%	4.041%
8	7.310	884	888	891	rBV	1468048	1277805	31.82%	2.938%
9	7.634	940	943	954	rBV	1369894	1048132	26.10%	2.410%
10	7.881	982	985	1007	rBV	2132505	1775287	44.21%	4.082%
11	8.034	1007	1011	1014	rVV	1752777	1339390	33.35%	3.079%
12	8.093	1018	1021	1045	rVB	2216668	1781579	44.36%	4.096%
13	8.716	1124	1127	1140	rVB	28889	31886	0.79%	0.073%
14	9.493	1255	1259	1262	rBV	2864232	2317221	57.70%	5.327%
15	9.552	1267	1269	1275	rVB4	4120	4377	0.11%	0.010%
16	9.640	1281	1284	1288	rBV	3476448	3041966	75.75%	6.994%
17	9.799	1307	1311	1314	rBV	2020428	1668505	41.55%	3.836%
18	9.910	1327	1330	1344	rBV	818586	868464	21.63%	1.997%
19	10.004	1344	1346	1353	rVB3	11382	14721	0.37%	0.034%
20	10.322	1396	1400	1403	rBV	4039394	3526089	87.81%	8.107%
21	10.393	1408	1412	1419	rBV	791522	664555	16.55%	1.528%
22	10.446	1419	1421	1430	rVB	61332	59619	1.48%	0.137%
23	10.746	1469	1472	1477	rVB	17959	15000	0.37%	0.034%
24	11.110	1531	1534	1539	rVB2	7794	7360	0.18%	0.017%
25	11.157	1539	1542	1549	rVV3	11336	16432	0.41%	0.038%
26	11.222	1550	1553	1556	rVB2	5821	4543	0.11%	0.010%
27	11.293	1562	1565	1569	rBV	2134482	1778795	44.30%	4.090%
28	11.351	1571	1575	1579	rBV	4283643	3607427	89.83%	8.294%
29	11.516	1600	1603	1610	rVB	4151	5042	0.13%	0.012%
30	12.504	1767	1771	1777	rVB	41824	41813	1.04%	0.096%
31	12.657	1794	1797	1801	rBV	39845	33302	0.83%	0.077%
32	12.734	1806	1810	1814	rBV	4162161	4015783	100.00%	9.233%
33	13.287	1901	1904	1908	rBV	76416	64252	1.60%	0.148%
34	13.457	1928	1933	1936	rBV5	4707	6907	0.17%	0.016%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
Data File : BP000733.D
Acq On : 15 Oct 2019 00:56
Operator : JU
Sample : PB123959BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK59

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

35	13.822	1992	1995	1999	rVB5	9630	9566	0.24%	0.022%
36	13.969	2016	2020	2034	rVB	1902608	1761605	43.87%	4.050%
37	14.145	2047	2050	2055	rBV	10154	9818	0.24%	0.023%
38	14.451	2100	2102	2106	rBV	20114	18231	0.45%	0.042%
39	14.763	2152	2155	2160	rVB	44574	42788	1.07%	0.098%
40	14.969	2186	2190	2196	rVB	43107	47367	1.18%	0.109%
41	15.104	2209	2213	2219	rBV2	60004	76493	1.90%	0.176%
42	15.357	2250	2256	2265	rBV	2952805	3574043	89.00%	8.217%
43	15.445	2266	2271	2275	rVV	1427032	1695306	42.22%	3.898%
44	15.487	2275	2278	2292	rVB	75262	113927	2.84%	0.262%
45	15.922	2348	2352	2359	rBV	55932	87516	2.18%	0.201%
46	16.004	2363	2366	2372	rVB3	15430	24378	0.61%	0.056%
47	16.434	2434	2439	2447	rVB2	42615	78234	1.95%	0.180%
48	17.028	2535	2540	2546	rBV3	26650	52583	1.31%	0.121%


Sum of corrected areas: 43495830

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101519\
Data File : BP000733.D
Acq On : 15 Oct 2019 00:56
Operator : JU
Sample : PB123959BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK59

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

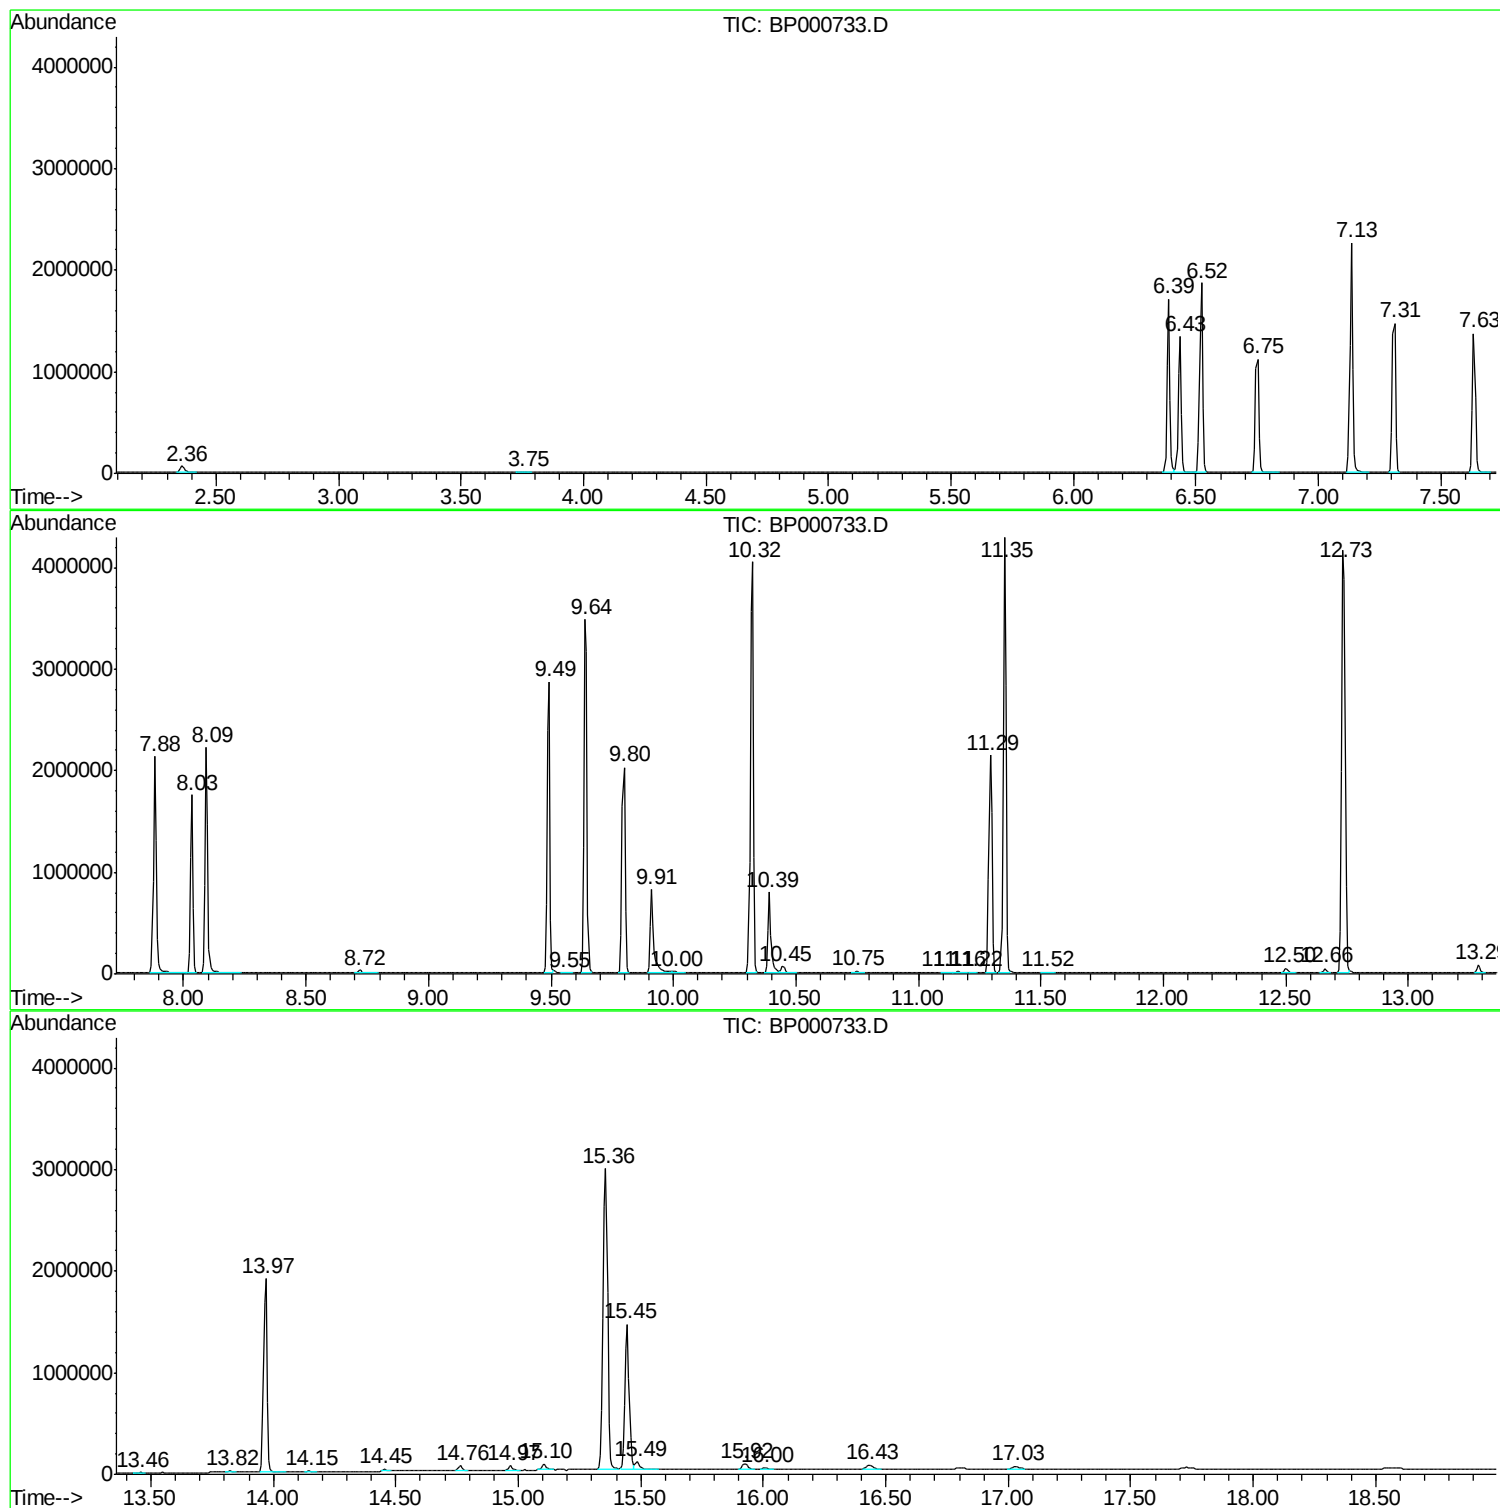

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101519\
Data File : BP000733.D
Acq On : 15 Oct 2019 00:56
Operator : JU
Sample : PB123959BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK59

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101519\
Data File : BP000733.D
Acq On : 15 Oct 2019 00:56
Operator : JU
Sample : PB123959BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK59

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc