
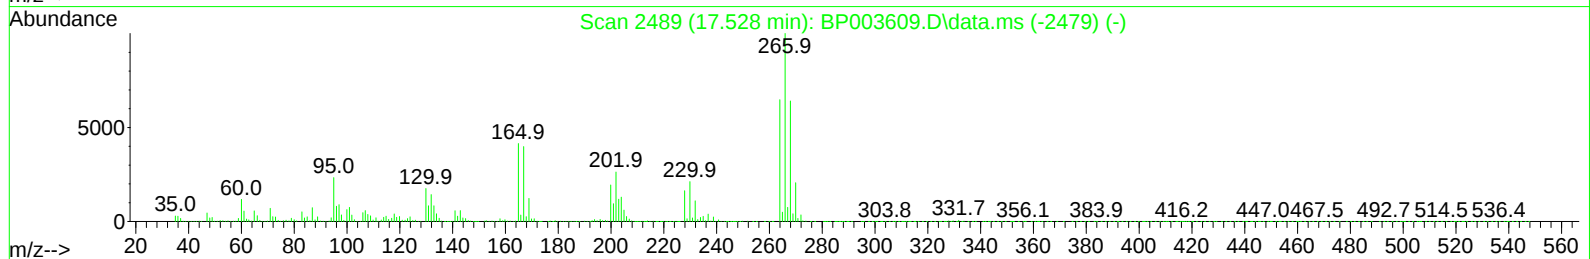
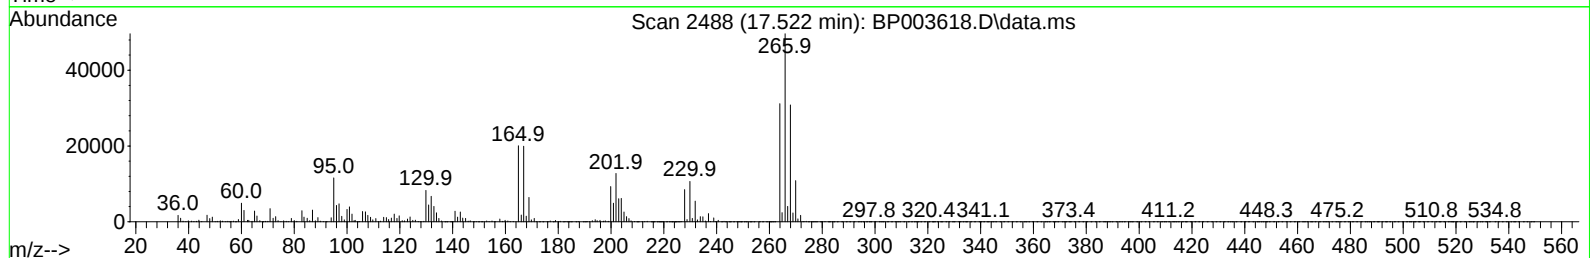


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101520\
Data File : BP003618.D
Acq On : 15 Oct 2020 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 02:43:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 14 17:03:23 2020
Response via : Initial Calibration

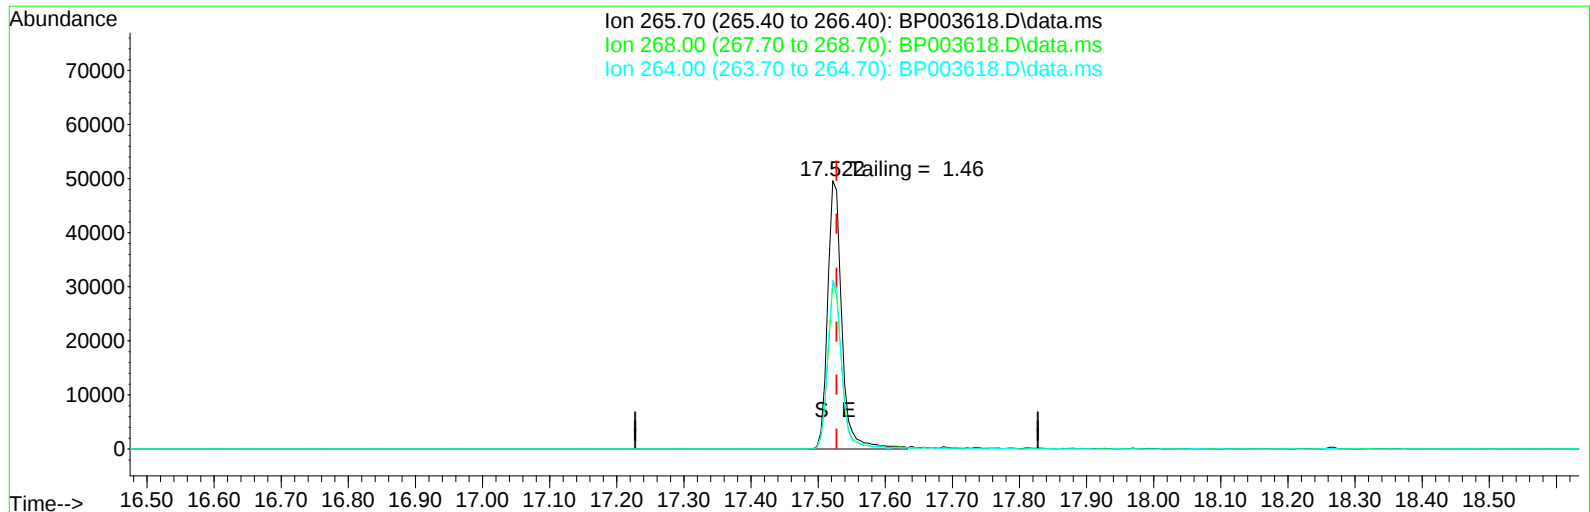

TIC: BP003618.D\data.ms

(70) Pentachlorophenol (C)




17.522min (-0.006) 974948.56 ng

response 73141

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.11
264.00	63.30	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101520\
Data File : BP003618.D
Acq On : 15 Oct 2020 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 02:43:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 14 17:03:23 2020
Response via : Initial Calibration

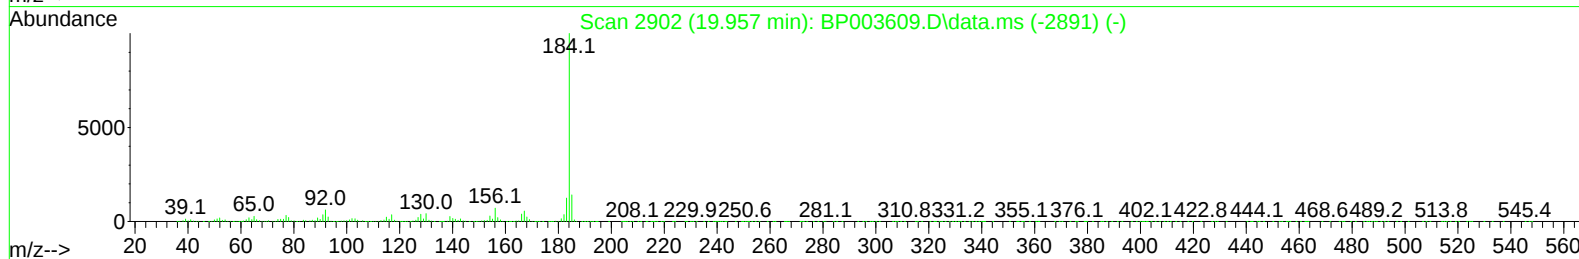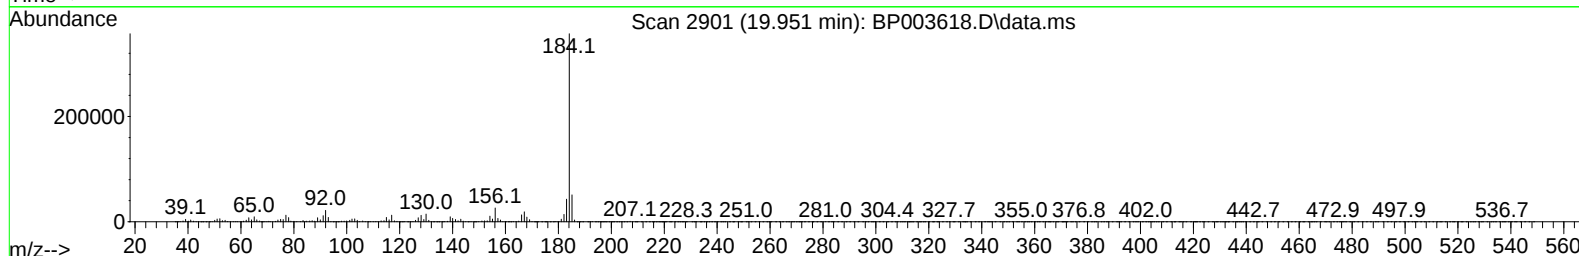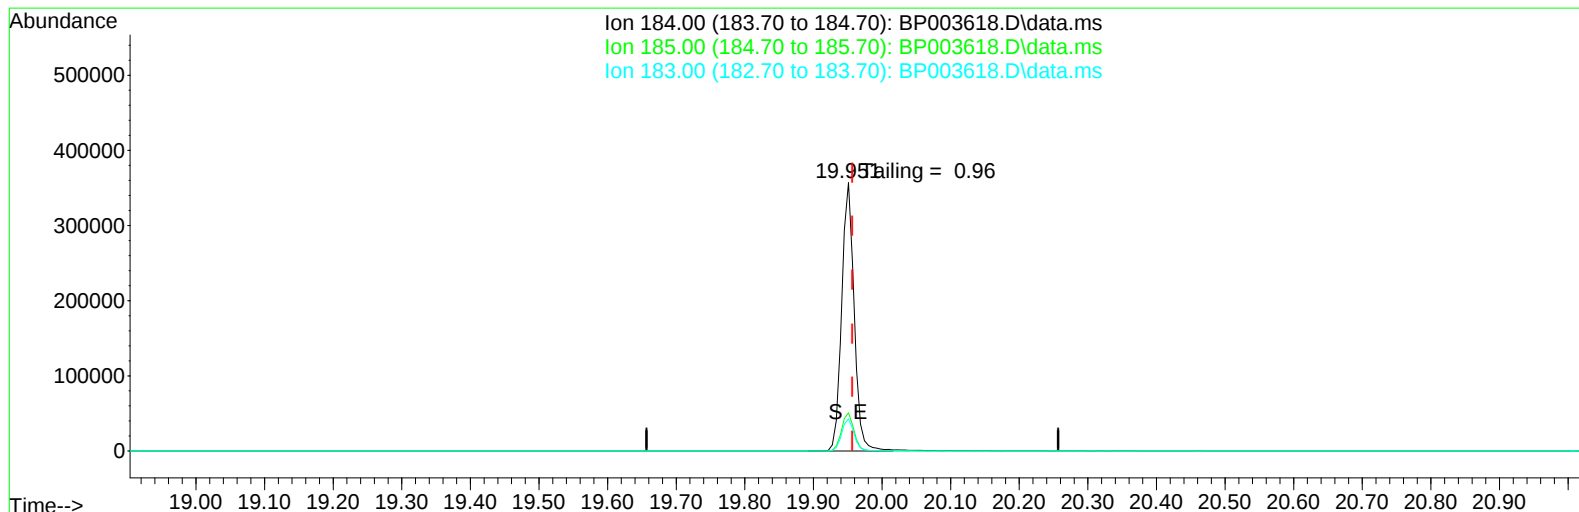

TIC: BP003618.D\data.ms

(77) Benzidine**19.951min (-0.006) 377027.43 ng****response 450770**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.30
183.00	12.00	11.97
0.00	0.00	0.00