

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101520\
 Data File : BP003626.D
 Acq On : 15 Oct 2020 16:11
 Operator : CG/JU
 Sample : L3971-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP

Quant Time: Oct 15 16:40:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 14 17:03:23 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.540	152	69787	20.00	ng	# 0.00
21) Naphthalene-d8	11.387	136	254995	20.00	ng	# 0.00
39) Acenaphthene-d10	15.139	164	170562	20.00	ng	-0.01
64) Phenanthrene-d10	17.857	188	382670	20.00	ng	0.00
76) Chrysene-d12	21.869	240	380883	20.00	ng	#-0.01
86) Perylene-d12	24.445	264	388427	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.034	112	613867	151.22	ng	0.00
7) Phenol-d6	7.687	99	818959	138.50	ng	0.00
23) Nitrobenzene-d5	9.710	82	594022	108.01	ng	0.00
42) 2,4,6-Tribromophenol	16.616	330	380561	167.35	ng	0.00
45) 2-Fluorobiphenyl	13.775	172	1283250	98.71	ng	0.00
79) Terphenyl-d14	20.322	244	2120518	100.73	ng	-0.01
Target Compounds						
						Qvalue
8) 2-Chlorophenol	8.105	128	465024	112.68	ng	82
10) Phenol	7.716	94	907187	158.87	ng	77
17) 2-Methylphenol	8.987	107	233198	60.27	ng	# 88
20) 3+4-Methylphenols	9.310	107	496230	96.34	ng	90
26) 2-Nitrophenol	10.481	139	264136	161.31	ng	# 62
27) 2,4-Dimethylphenol	10.534	122	478627	141.52	ng	# 83
29) 2,4-Dichlorophenol	11.034	162	685880	162.47	ng	95
36) 4-Chloro-3-methylphenol	12.616	107	259107	53.77	ng	84
43) 2,4,6-Trichlorophenol	13.598	196	625749	174.50	ng	100
44) 2,4,5-Trichlorophenol	13.669	196	166985	44.34	ng	# 95
54) 2,4-Dinitrophenol	15.210	184	238521	138.90	ng	# 77
65) 4,6-Dinitro-2-methylph...	16.234	198	380465	202.17	ng	90
70) Pentachlorophenol	17.522	266	199329	76.38	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101520\
Data File : BP003626.D
Acq On : 15 Oct 2020 16:11
Operator : CG/JU
Sample : L3971-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Quant Time: Oct 15 16:40:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 14 17:03:23 2020
Response via : Initial Calibration




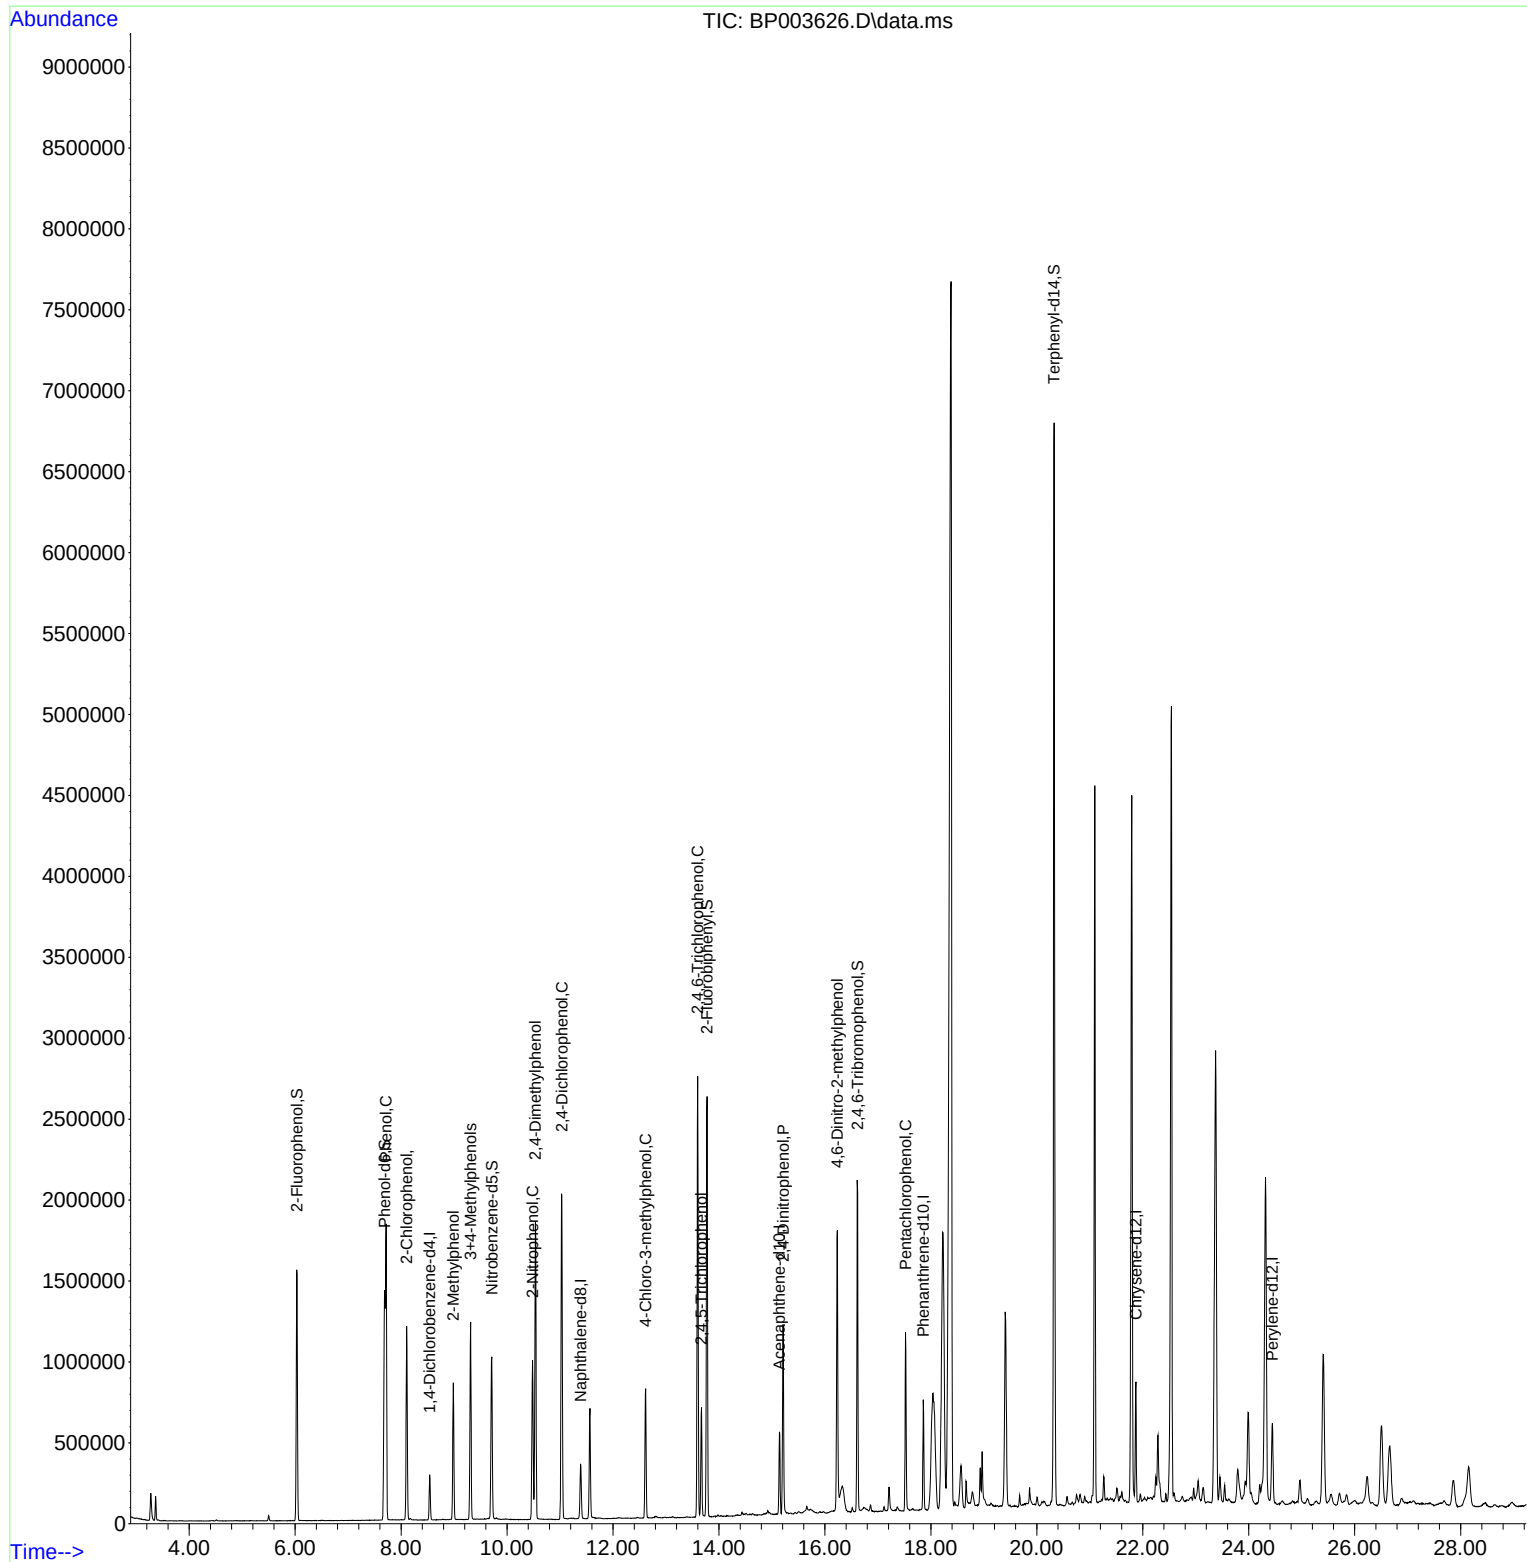




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.540 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:152 Resp: 69787
Ion Ratio Lower Upper
152 100
150 158.0 123.8 185.6
115 66.6 43.8 65.6#

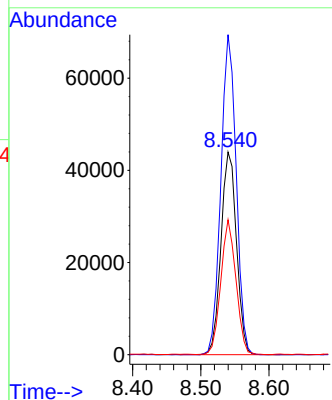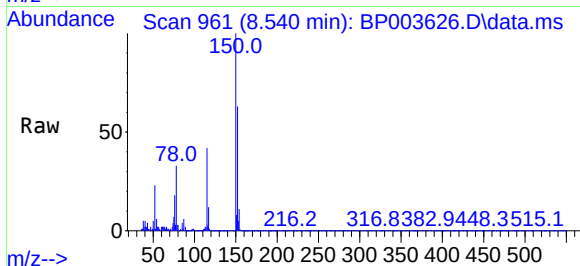

#5
2-Fluorophenol
Concen: 151.22 ng
RT: 6.034 min Scan# 535
Delta R.T. 0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:112 Resp: 613867
Ion Ratio Lower Upper
112 100
64 60.3 32.8 49.2#
63 34.8 17.0 25.4#


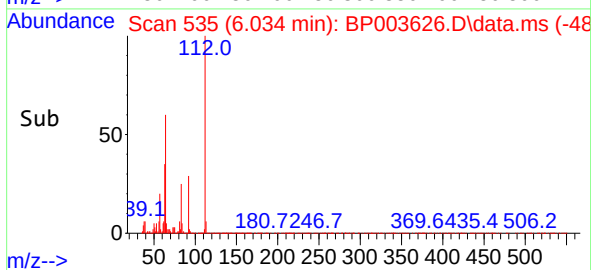
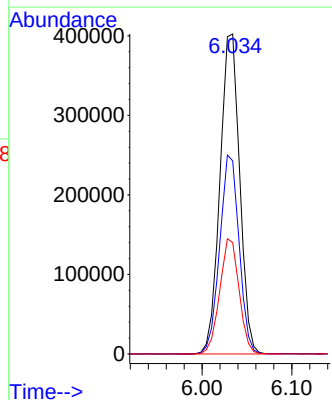
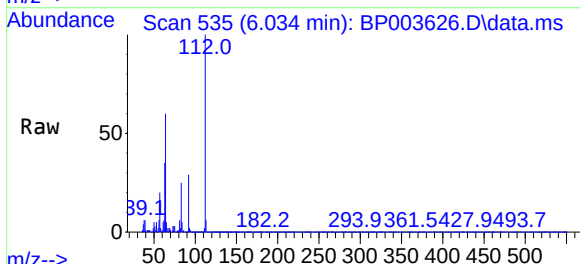




#7
Phenol-d6
Concen: 138.50 ng
RT: 7.687 min Scan# 816
Delta R.T. 0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion: 99 Resp: 818959
Ion Ratio Lower Upper
99 100
42 18.3 8.6 13.0#
71 42.5 23.4 35.2#

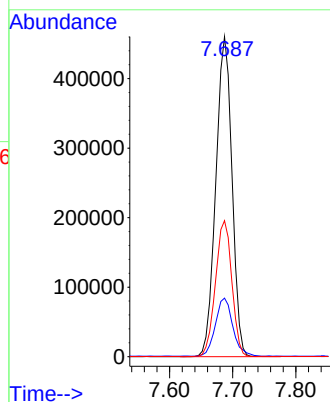

#8
2-Chlorophenol
Concen: 112.68 ng
RT: 8.105 min Scan# 887
Delta R.T. -0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion: 128 Resp: 465024
Ion Ratio Lower Upper
128 100
130 32.2 13.0 53.0
64 50.0 10.4 50.4


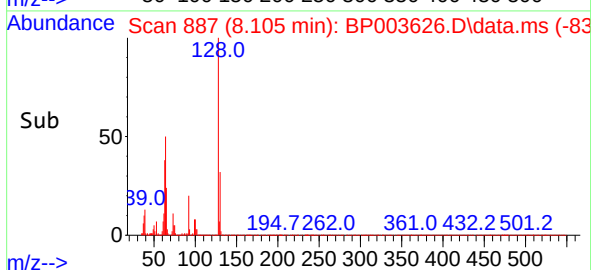






#10
Phenol
Concen: 158.87 ng
RT: 7.716 min Scan# 821
Delta R.T. 0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion: 94 Resp: 907187
Ion Ratio Lower Upper
94 100
65 30.8 2.3 42.3
66 46.0 10.9 50.9



#17
2-Methylphenol
Concen: 60.27 ng
RT: 8.987 min Scan# 1037
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion: 107 Resp: 233198
Ion Ratio Lower Upper
107 100
108 111.5 89.6 134.4
77 56.3 31.8 47.6#
79 56.6 31.1 46.7#


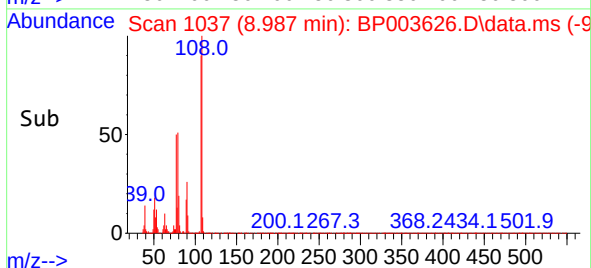
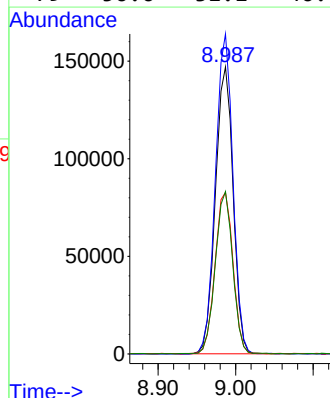





#20
3+4-Methylphenols
Concen: 96.34 ng
RT: 9.310 min Scan# 1092
Delta R.T. -0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:107	Resp:	496230	
Ion	Ratio	Lower	Upper
107	100		
108	79.4	69.0	109.0
77	37.0	8.5	48.5
79	26.6	4.8	44.8

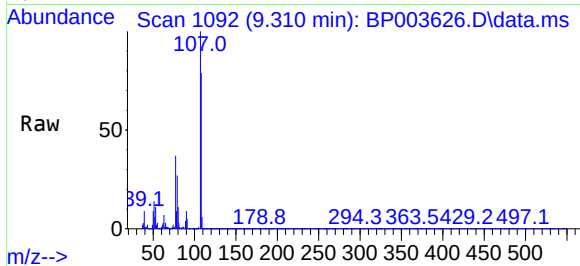

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.387 min Scan# 1445
Delta R.T. -0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt	Ion:136	Resp:	254995
Ion	Ratio	Lower	Upper
136	100		
137	10.4	8.6	13.0
54	7.9	3.6	5.4#
68	6.2	3.3	4.9#


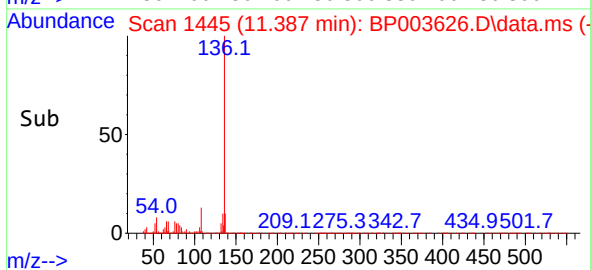

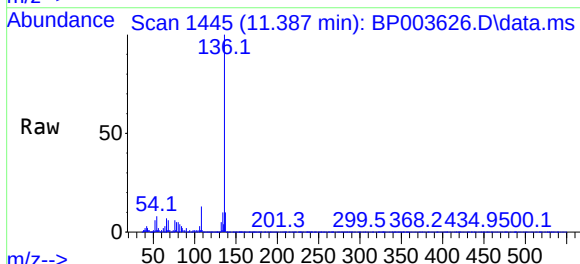




#23
Nitrobenzene-d5
Concen: 108.01 ng
RT: 9.710 min Scan# 1160
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion: 82 Resp: 594022
Ion Ratio Lower Upper
82 100
128 36.9 45.6 68.4#
54 46.4 30.1 45.1#

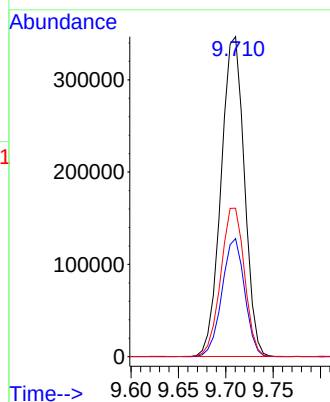

#26
2-Nitrophenol
Concen: 161.31 ng
RT: 10.481 min Scan# 1291
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion: 139 Resp: 264136
Ion Ratio Lower Upper
139 100
109 42.8 22.1 33.1#
65 59.1 26.5 39.7#


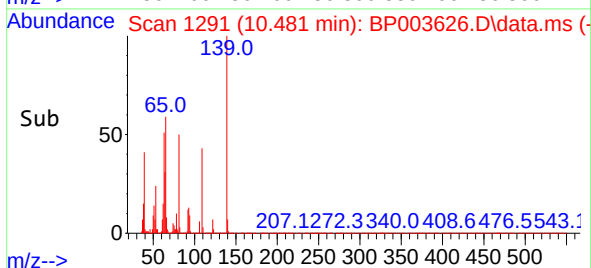






#27
2,4-Dimethylphenol
Concen: 141.52 ng
RT: 10.534 min Scan# 1300
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:122 Resp: 478627
Ion Ratio Lower Upper
122 100
107 136.3 87.3 130.9#
121 60.4 47.3 70.9

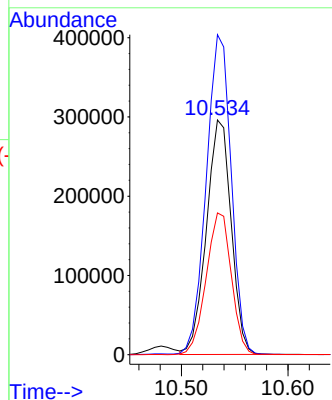

#29
2,4-Dichlorophenol
Concen: 162.47 ng
RT: 11.034 min Scan# 1385
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:162 Resp: 685880
Ion Ratio Lower Upper
162 100
164 65.7 45.8 85.8
98 38.6 10.2 50.2


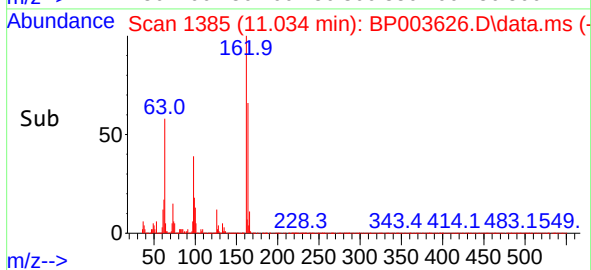
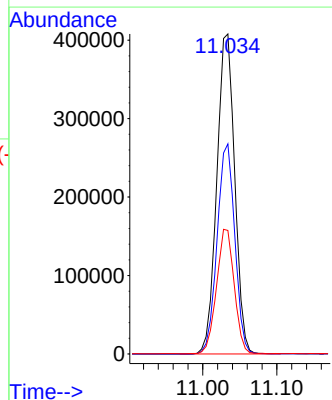





#36
4-Chloro-3-methylphenol
Concen: 53.77 ng
RT: 12.616 min Scan# 1654
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:107 Resp: 259107
Ion Ratio Lower Upper
107 100
144 24.1 22.7 34.1
142 71.3 70.7 106.1

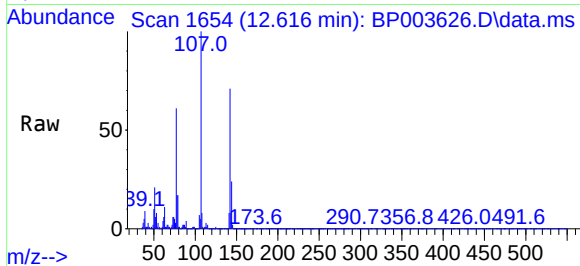

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 15.139 min Scan# 2083
Delta R.T. -0.012 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:164 Resp: 170562
Ion Ratio Lower Upper
164 100
162 101.4 79.4 119.2
160 44.5 36.1 54.1


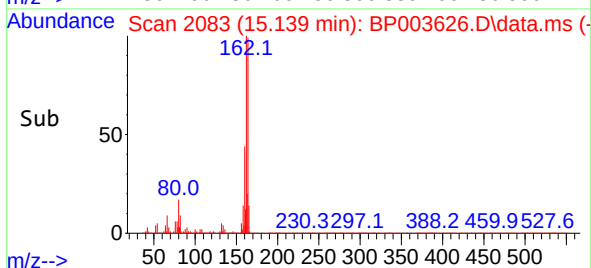
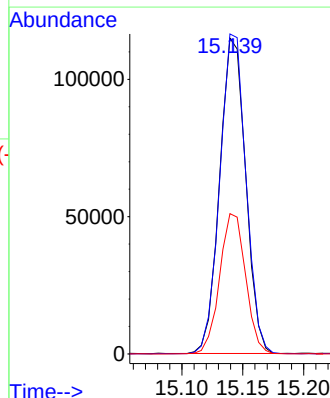
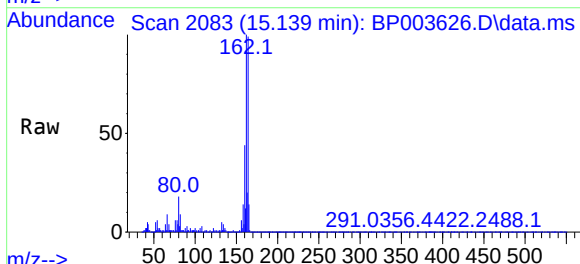




#42
2,4,6-Tribromophenol
Concen: 167.35 ng
RT: 16.616 min Scan# 2334
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:330 Resp: 380561
Ion Ratio Lower Upper
330 100
332 95.8 77.1 115.7
141 32.7 23.4 35.2

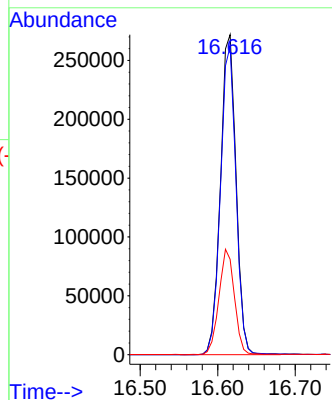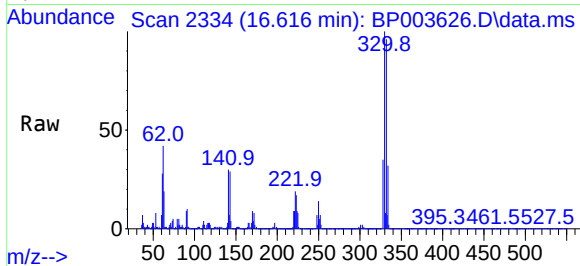

#43
2,4,6-Trichlorophenol
Concen: 174.50 ng
RT: 13.598 min Scan# 1821
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:196 Resp: 625749
Ion Ratio Lower Upper
196 100
198 95.9 77.0 115.6
200 31.1 25.1 37.7

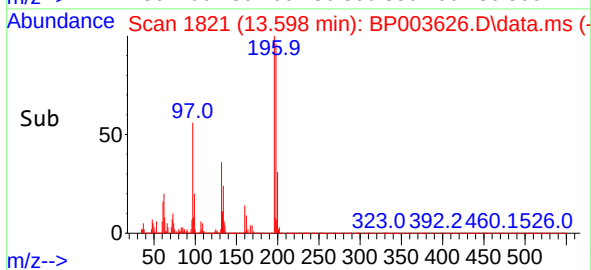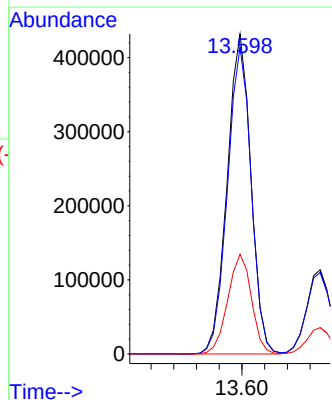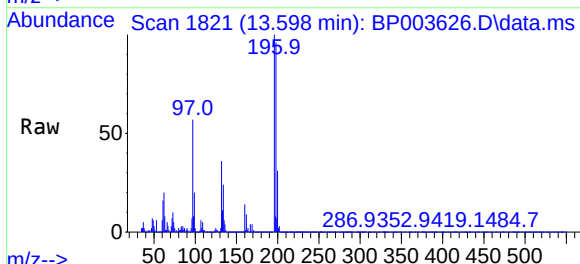







#44
2,4,5-Trichlorophenol
Concen: 44.34 ng
RT: 13.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion:196 Resp: 166985




Ion	Ratio	Lower	Upper
196	100		
198	96.9	77.3	115.9
97	50.6	31.0	46.4#
132	24.1	20.9	31.3




#45
2-Fluorobiphenyl
Concen: 98.71 ng
RT: 13.775 min Scan# 1851
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:172 Resp: 1283250

Ion	Ratio	Lower	Upper
172	100		
171	35.0	28.5	42.7
170	22.1	19.2	28.8


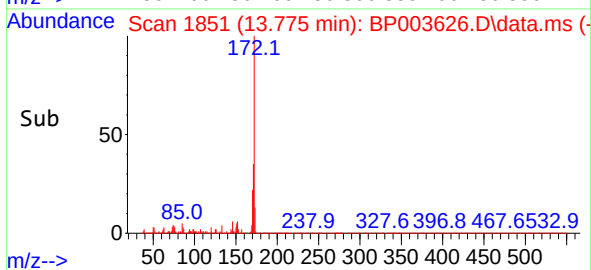






#54
2,4-Dinitrophenol
Concen: 138.90 ng
RT: 15.210 min Scan# 2095
Delta R.T. 0.000 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:184 Resp: 238521
Ion Ratio Lower Upper
184 100
63 67.4 32.3 48.5#
154 68.7 49.1 73.7

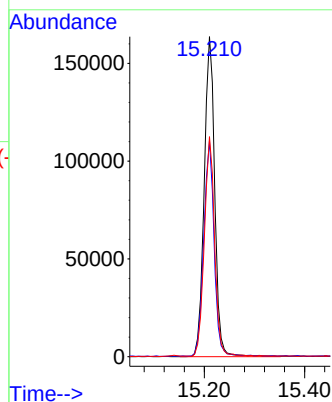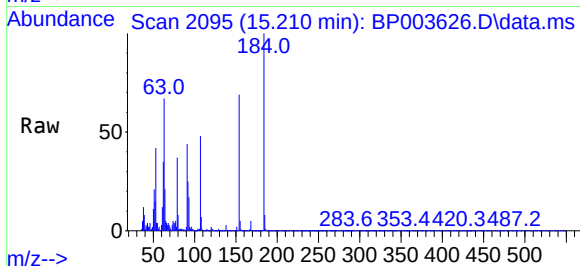

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.857 min Scan# 2545
Delta R.T. -0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:188 Resp: 382670
Ion Ratio Lower Upper
188 100
94 7.6 6.2 9.2
80 8.2 6.2 9.2


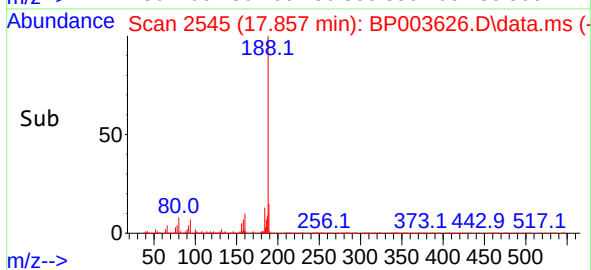
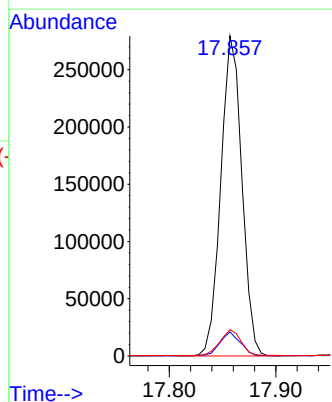
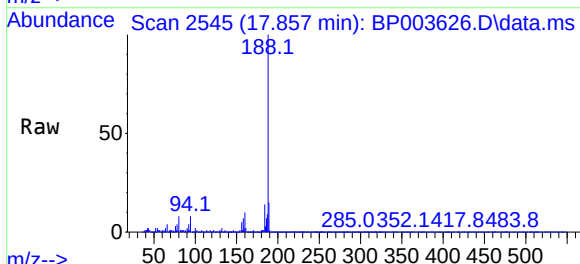




#65
4,6-Dinitro-2-methylphenol
Concen: 202.17 ng
RT: 16.234 min Scan# 2269
Delta R.T. 0.001 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:	198	Resp:	380465
Ion	Ratio	Lower	Upper
198	100		
51	38.6	6.4	46.4
105	38.7	18.9	58.9

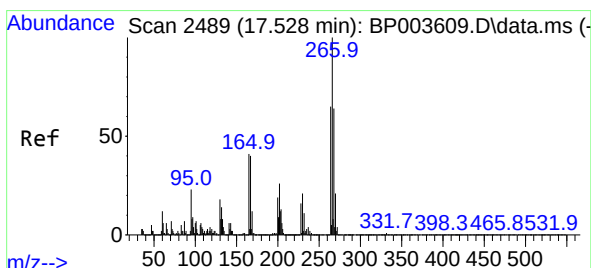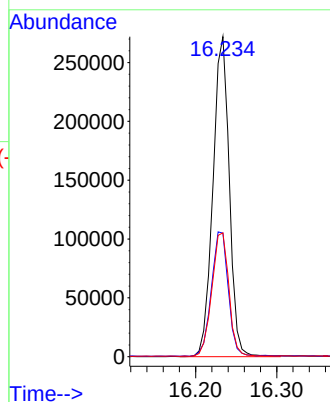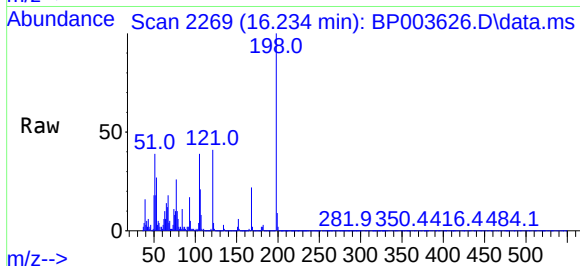

#70
Pentachlorophenol
Concen: 76.38 ng
RT: 17.522 min Scan# 2488
Delta R.T. -0.006 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:	266	Resp:	199329
Ion	Ratio	Lower	Upper
266	100		
268	62.9	51.1	76.7
264	65.6	50.6	76.0


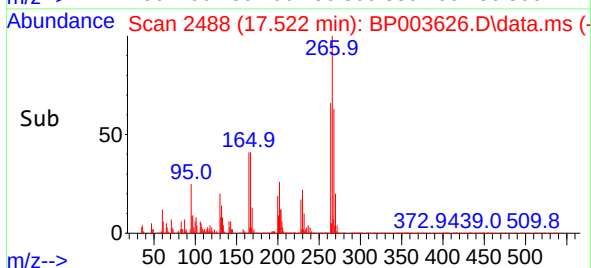

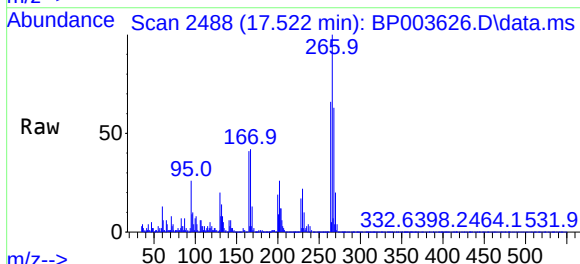




#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.869 min Scan# 3227
Delta R.T. -0.012 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:240 Resp: 380883
Ion Ratio Lower Upper
240 100
120 6.0 7.8 11.6#
236 25.0 20.8 31.2

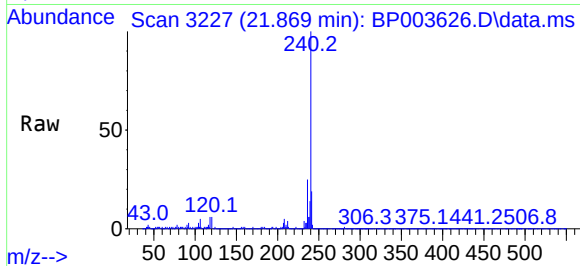

#79
Terphenyl-d14
Concen: 100.73 ng
RT: 20.322 min Scan# 2964
Delta R.T. -0.012 min
Lab File: BP003626.D
Acq: 15 Oct 2020 16:11

Tgt Ion:244 Resp: 2120518
Ion Ratio Lower Upper
244 100
212 7.5 5.8 8.6
122 7.4 7.8 11.8#

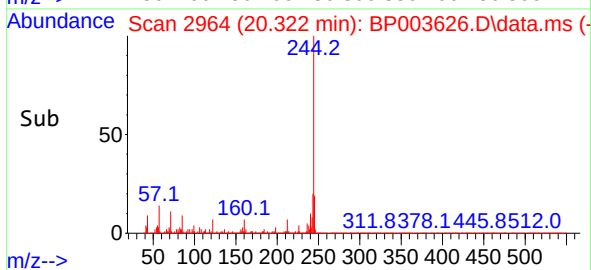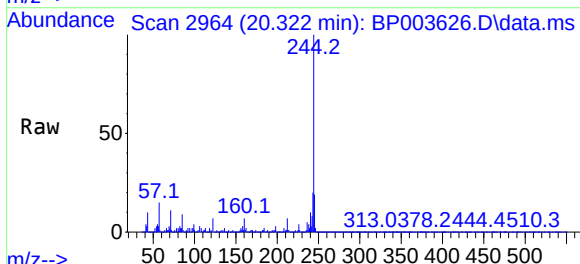

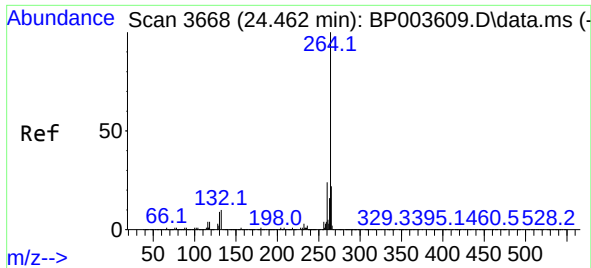

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 24.445 min Scan# 3665
 Delta R.T. -0.018 min
 Lab File: BP003626.D
 Acq: 15 Oct 2020 16:11

Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP

Tgt Ion:264 Resp: 388427

Ion	Ratio	Lower	Upper
264	100		
260	23.0	18.8	28.2
265	22.2	17.4	26.2

