


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101520\
 Data File : BP003618.D
 Acq On : 15 Oct 2020 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 16 12:46:19 2020

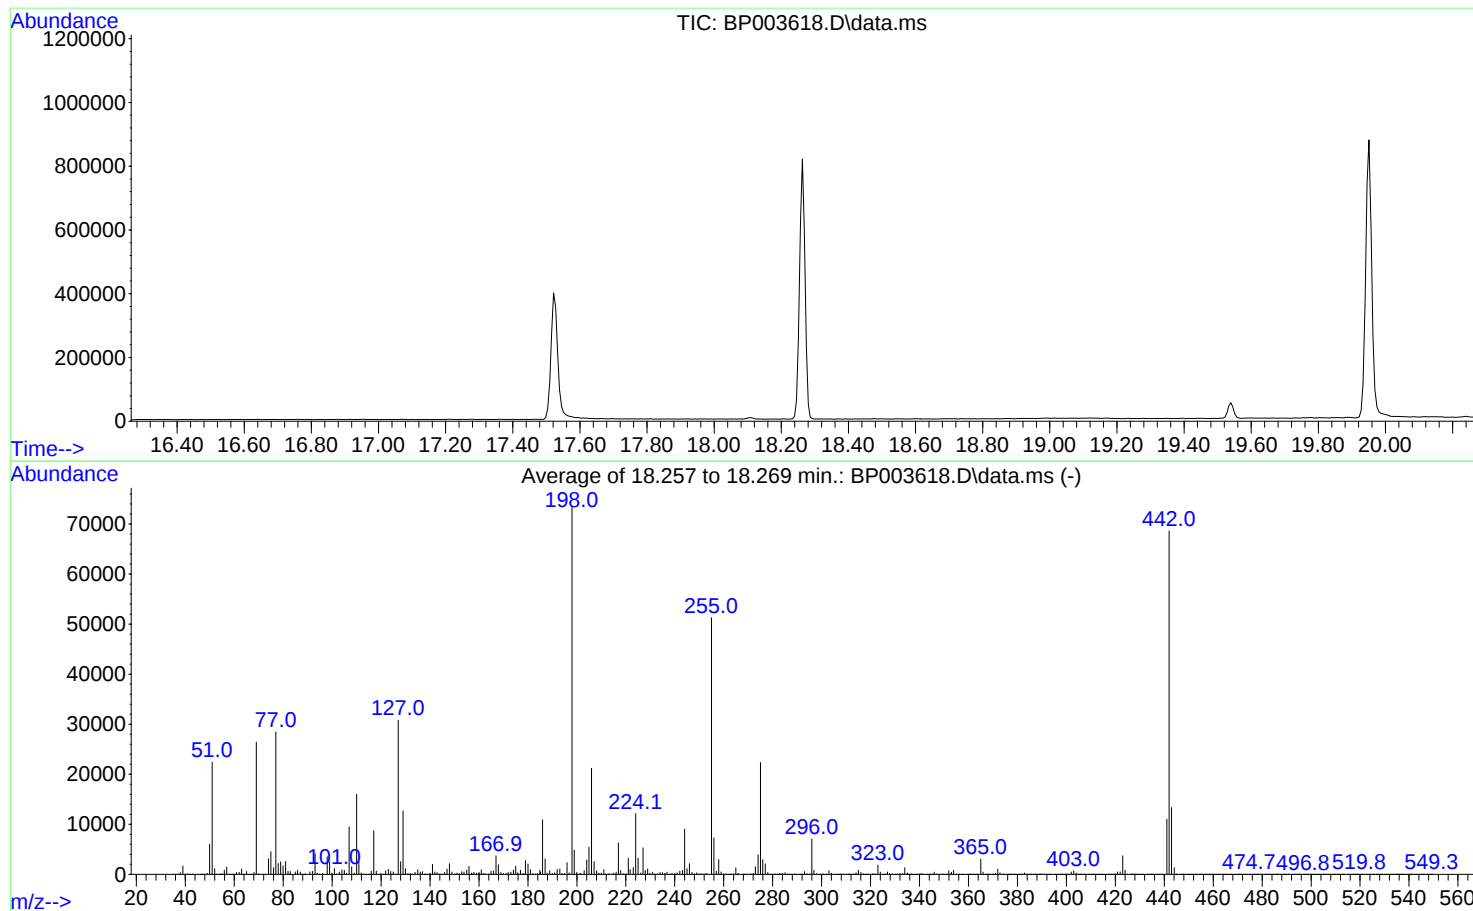

AutoFind: Scans 2613, 2614, 2615; Background Corrected with Scan 2604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	22411	PASS
68	69	0.00	2	1.5	397	PASS
69	198	0.00	100	35.9	26406	PASS
70	69	0.00	2	0.5	123	PASS
127	198	10	80	41.9	30781	PASS
197	198	0.00	2	0.4	278	PASS
198	198	100	100	100.0	73501	PASS
199	198	5	9	6.6	4837	PASS
275	198	10	60	30.4	22360	PASS
365	198	1	100	4.1	3045	PASS
441	198	0.01	100	15.0	11019	PASS
442	198	50	100	93.4	68621	PASS
443	442	15	24	19.5	13359	PASS