
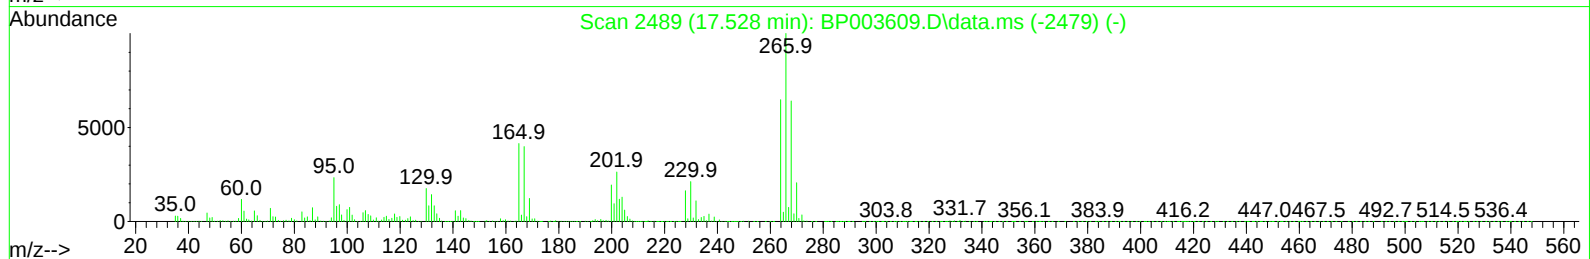
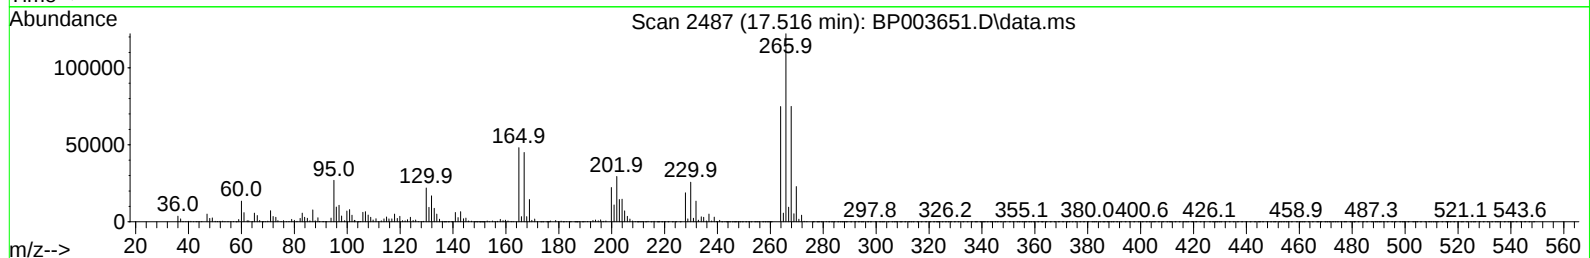


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101620\
Data File : BP003651.D
Acq On : 16 Oct 2020 23:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 02:07:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 12:46:19 2020
Response via : Initial Calibration

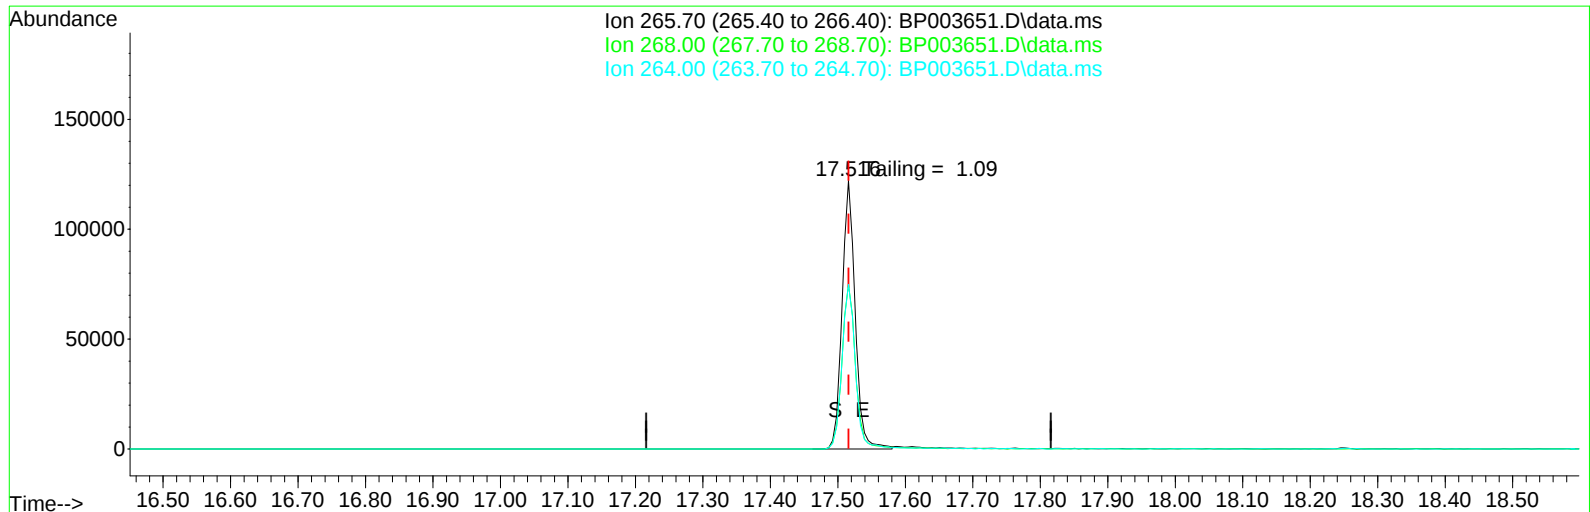

TIC: BP003651.D\data.ms

(70) Pentachlorophenol (C)




17.516min (-0.000) 363665.22 ng

response 166174

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.37
264.00	63.30	61.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101620\
Data File : BP003651.D
Acq On : 16 Oct 2020 23:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 02:07:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 12:46:19 2020
Response via : Initial Calibration

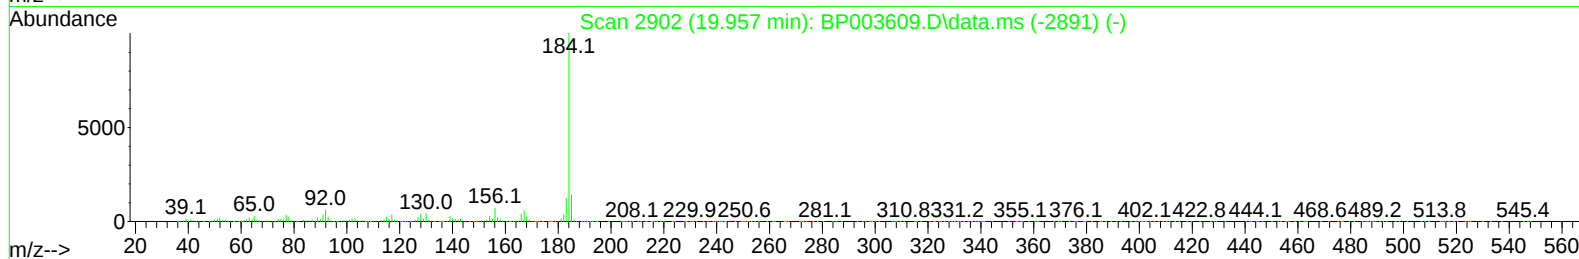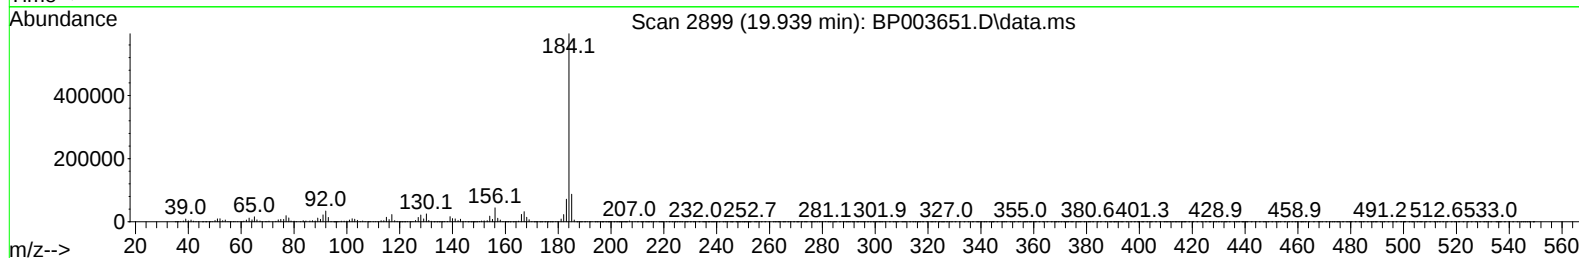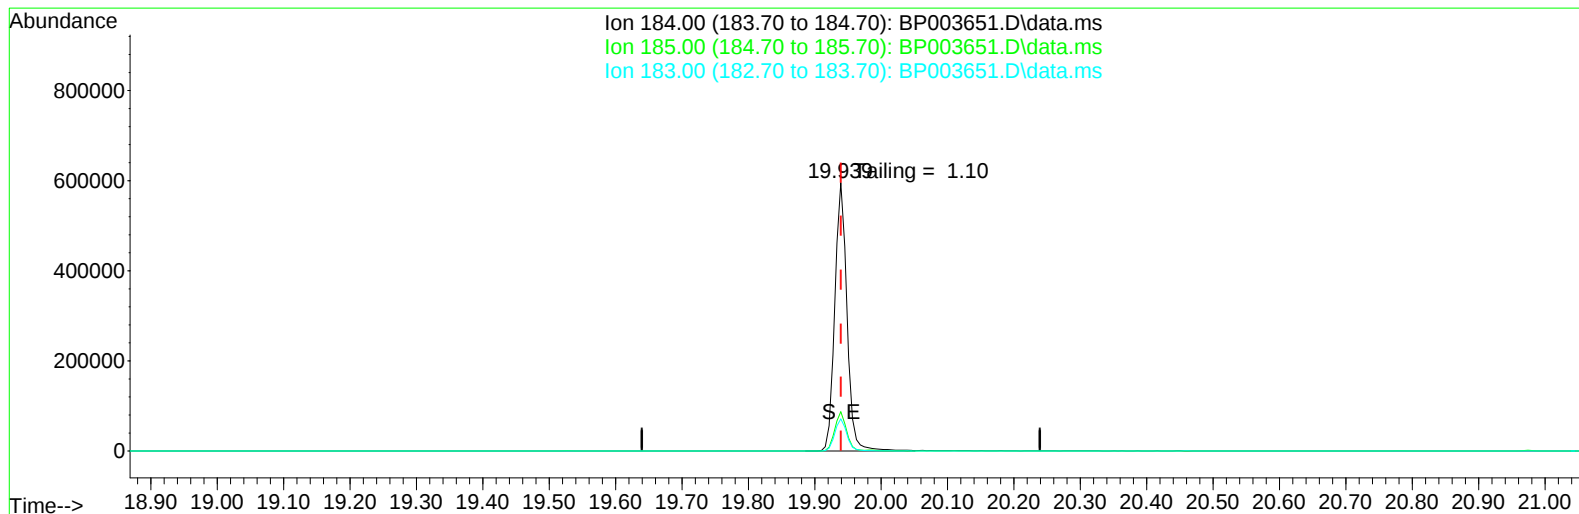

TIC: BP003651.D\data.ms

(77) Benzidine**19.939min (-0.000) 250171.87 ng****response 762419**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.67
183.00	12.00	12.00
0.00	0.00	0.00