
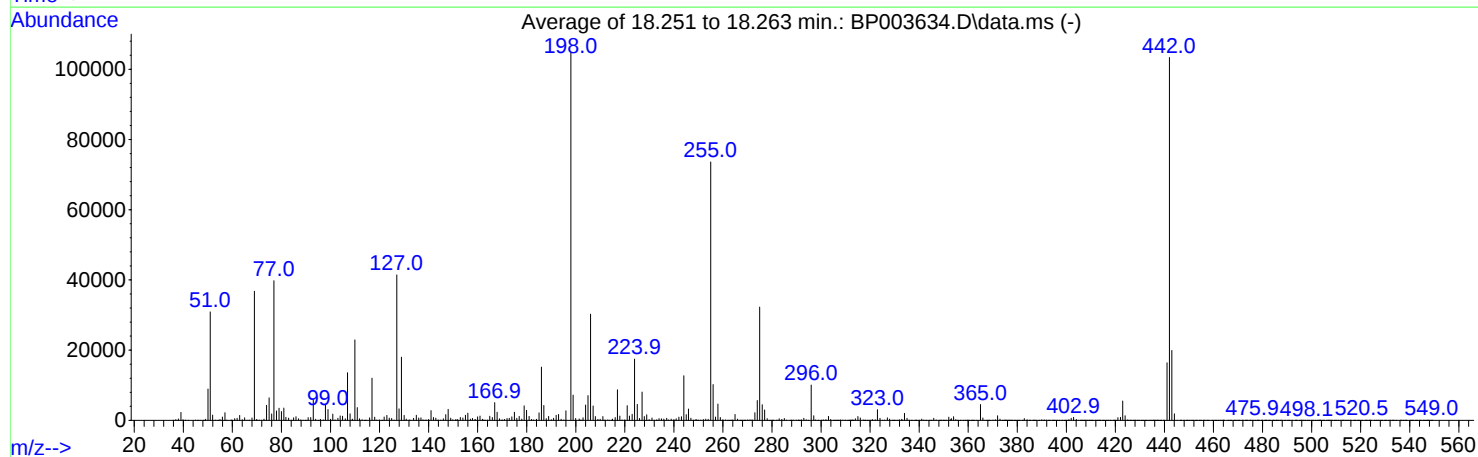


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101620\
 Data File : BP003634.D
 Acq On : 16 Oct 2020 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 16 12:46:19 2020

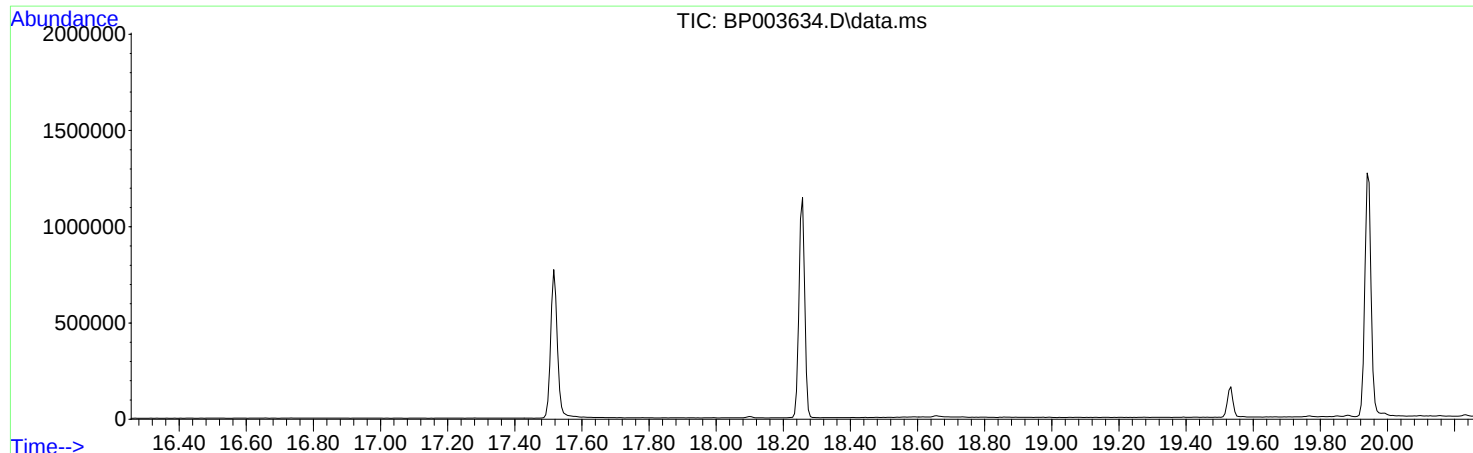

AutoFind: Scans 2612, 2613, 2614; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	30888	PASS
68	69	0.00	2	1.9	699	PASS
69	198	0.00	100	35.1	36806	PASS
70	69	0.00	2	0.6	219	PASS
127	198	10	80	39.5	41413	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	104787	PASS
199	198	5	9	6.9	7200	PASS
275	198	10	60	30.8	32267	PASS
365	198	1	100	4.3	4511	PASS
441	198	0.01	100	15.7	16416	PASS
442	198	50	100	98.7	103395	PASS
443	442	15	24	19.3	19906	PASS