
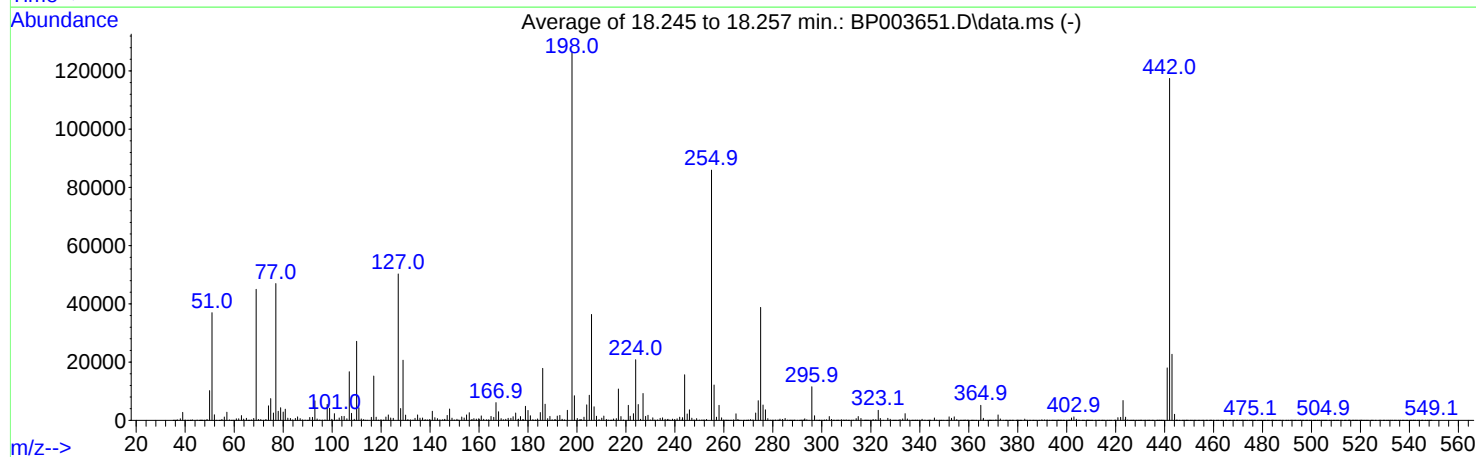


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP101620\  
 Data File : BP003651.D  
 Acq On : 16 Oct 2020 23:11  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP101420.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Oct 16 12:46:19 2020

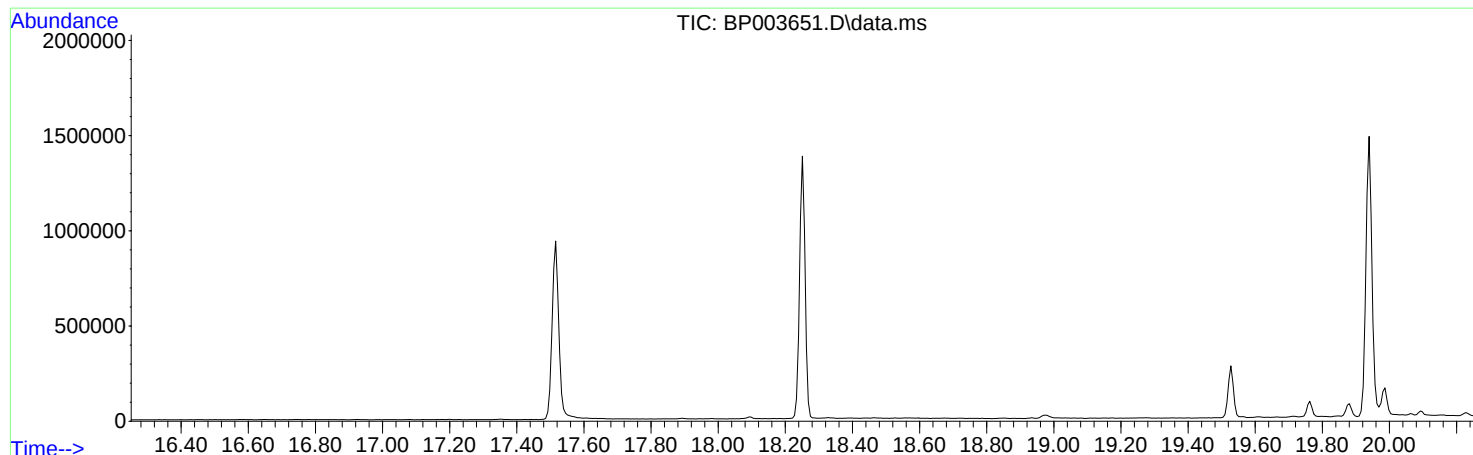

AutoFind: Scans 2611, 2612, 2613; Background Corrected with Scan 2602

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.3         | 37003      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 684        | PASS                |
| 69             | 198             | 0.00            | 100             | 35.6         | 44991      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 313        | PASS                |
| 127            | 198             | 10              | 80              | 39.8         | 50288      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 126333     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 8447       | PASS                |
| 275            | 198             | 10              | 60              | 30.7         | 38820      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 5187       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.3         | 18011      | PASS                |
| 442            | 198             | 50              | 100             | 93.0         | 117428     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 22683      | PASS                |