




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022430.D
Acq On : 17 Oct 2024 01:56
Operator : RC/JU
Sample : P4329-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EG5

Manual IntegrationsAPPROVED

Quant Time: Oct 17 02:22:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 11:47:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/17/2024
Supervised By :mohammad ahmed 10/18/2024

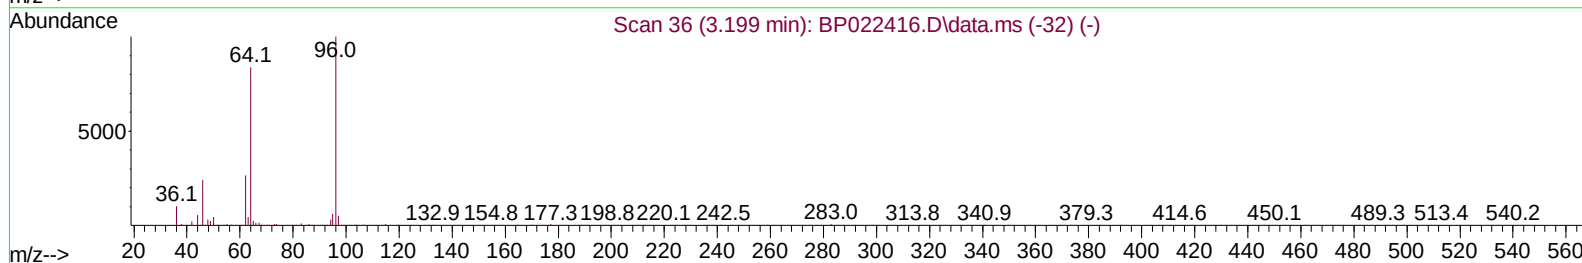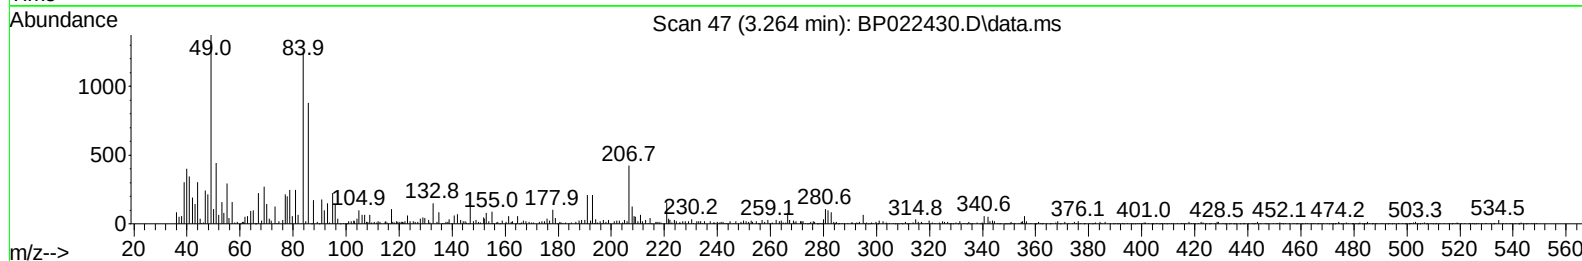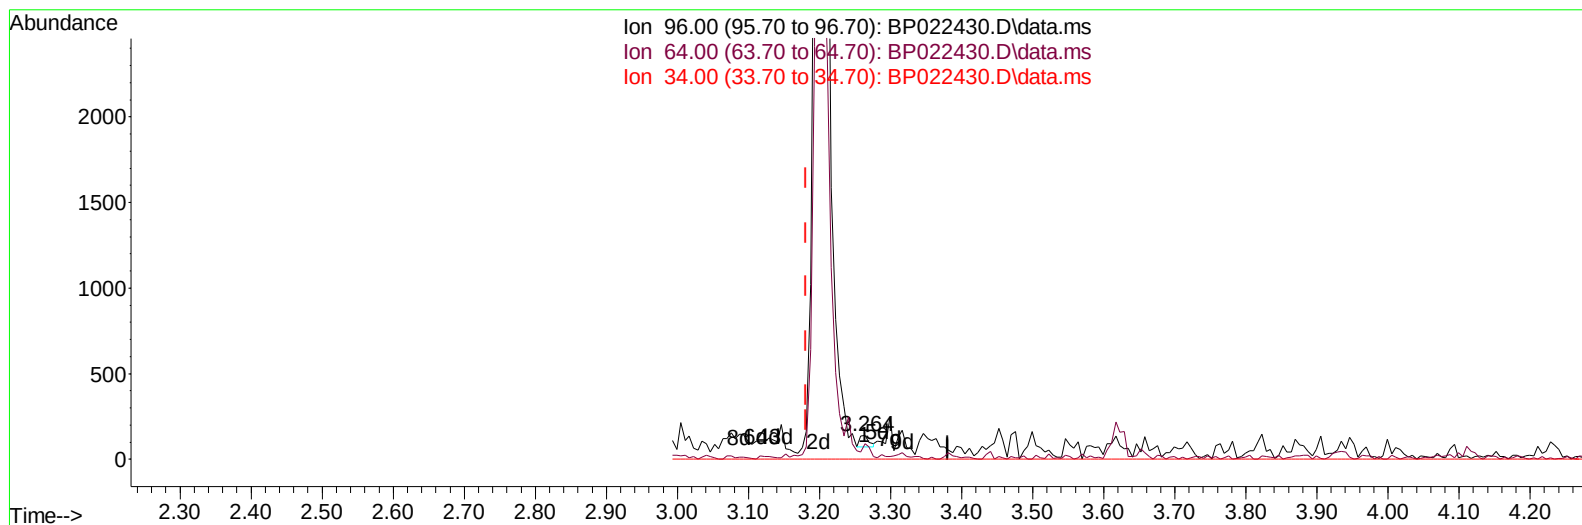

TIC: BP022430.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.264min (+ 0.083) 0.02 ng/uL

response 65

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	65.47
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022430.D
Acq On : 17 Oct 2024 01:56
Operator : RC/JU
Sample : P4329-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EG5

Manual IntegrationsAPPROVED

Quant Time: Oct 17 02:22:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 11:47:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/17/2024
Supervised By :mohammad ahmed 10/18/2024

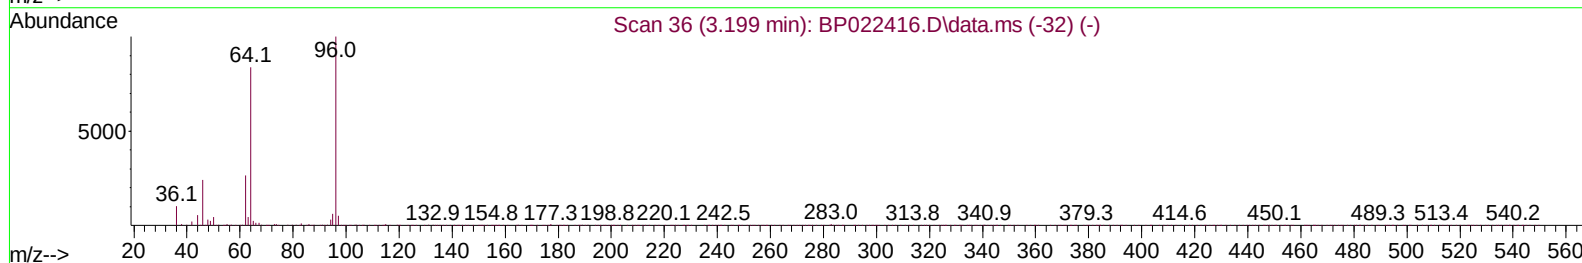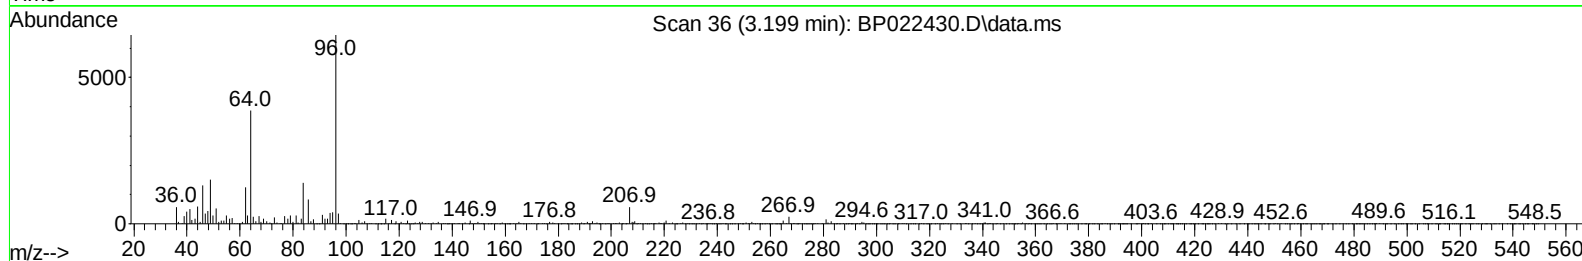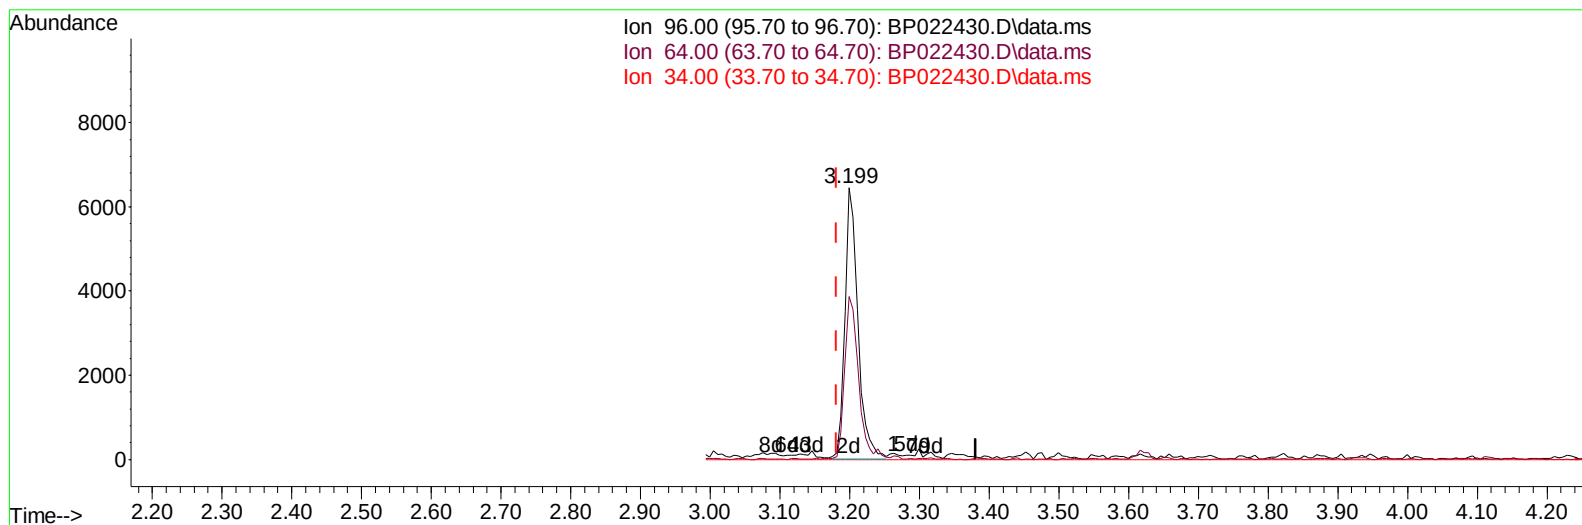

TIC: BP022430.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.199min (+ 0.018) 2.25 ng/uL m

response 8356

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	59.90#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
 Data File : BP022430.D
 Acq On : 17 Oct 2024 01:56
 Operator : RC/JU
 Sample : P4329-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EG5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/17/2024
 Supervised By :mohammad ahmed 10/18/2024

Quant Time: Oct 17 02:23:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 16 11:47:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.669	152	144035	20.000	ng/ul	0.04
20) Naphthalene-d8	10.422	136	538508	20.000	ng/ul	0.03
38) Acenaphthene-d10	14.275	164	440436	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.081	188	1069628	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	1095084	20.000	ng/ul	#-0.02
88) Perylene-d12	24.774	264	1318351	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	8356m	2.254	ng/uL	0.02
4) Pyridine-d5	3.617	84	111511	10.959	ng/ul	0.03
7) Phenol-d5	6.858	99	161537	13.323	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.011	67	93440	13.112	ng/ul	0.04
11) 2-Chlorophenol-d4	7.211	132	125846	14.628	ng/ul	0.04
15) 4-Methylphenol-d8	8.369	113	139496	14.417	ng/ul	0.04
21) Nitrobenzene-d5	8.811	128	64606	15.603	ng/ul	0.04
24) 2-Nitrophenol-d4	9.516	143	75481	15.746	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.058	165	161077	15.810	ng/ul	0.04
31) 4-Chloroaniline-d4	10.558	131	183947	15.279	ng/ul	0.02
46) Dimethylphthalate-d6	13.687	166	599404	17.129	ng/ul	0.02
49) Acenaphthylene-d8	13.969	160	620737	16.701	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	77095	13.132	ng/ul	0.00
60) Fluorene-d10	15.281	176	529313	17.439	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	79310	11.274	ng/ul	0.00
73) Anthracene-d10	17.169	188	886622	17.620	ng/ul	-0.02
81) Pyrene-d10	19.557	212	1074571	18.556	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.545	264	1260937	17.909	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022430.D
Acq On : 17 Oct 2024 01:56
Operator : RC/JU
Sample : P4329-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EG5

Manual IntegrationsAPPROVED

Quant Time: Oct 17 02:23:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 11:47:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/17/2024
Supervised By :mohammad ahmed 10/18/2024

