

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
 Data File : BP022411.D
 Acq On : 16 Oct 2024 11:19
 Operator : RC/JU
 Sample : PB163941BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK941

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	33	36	43	rVB	24649	31858	1.14%	0.120%
2	3.611	102	106	123	rBV	285409	444832	15.86%	1.675%
3	3.928	155	160	165	rBV	7772	11162	0.40%	0.042%
4	6.858	648	658	666	rBV	349099	584554	20.84%	2.200%
5	7.010	678	684	694	rVB	278387	429640	15.32%	1.617%
6	7.210	711	718	727	rBV	371545	591976	21.11%	2.228%
7	7.669	788	796	806	rBV	388106	623333	22.23%	2.346%
8	8.369	907	915	930	rBV	434695	719212	25.64%	2.707%
9	8.805	982	989	1005	rBV	351633	571718	20.38%	2.152%
10	9.222	1057	1060	1064	rVB4	4502	6313	0.23%	0.024%
11	9.516	1102	1110	1124	rBV	286272	504396	17.98%	1.899%
12	10.057	1193	1202	1219	rBV	464804	768237	27.39%	2.892%
13	10.422	1256	1264	1274	rBV	526636	812587	28.97%	3.059%
14	10.563	1280	1288	1303	rBV	387589	717711	25.59%	2.702%
15	11.698	1476	1481	1487	rVB8	3529	6250	0.22%	0.024%
16	12.016	1529	1535	1543	rBV2	7600	13596	0.48%	0.051%
17	13.698	1810	1821	1832	rBV	771386	1192025	42.50%	4.487%
18	13.969	1858	1867	1880	rBV	869506	1301630	46.41%	4.900%
19	14.275	1912	1919	1930	rBV	849771	1187867	42.35%	4.472%
20	14.504	1952	1958	1976	rBV	369256	564014	20.11%	2.123%
21	14.728	1989	1996	2001	rVB	3062	6169	0.22%	0.023%
22	14.857	2014	2018	2023	rVB7	2132	3644	0.13%	0.014%
23	15.292	2086	2092	2102	rBV	1211957	1700834	60.64%	6.403%
24	15.439	2110	2117	2125	rBV	390000	566808	20.21%	2.134%
25	15.545	2132	2135	2142	rVB4	7496	11363	0.41%	0.043%
26	16.504	2292	2298	2301	rBV8	2403	4667	0.17%	0.018%
27	16.875	2355	2361	2365	rBV6	3121	7004	0.25%	0.026%
28	17.098	2389	2399	2409	rBV	942969	1551539	55.32%	5.841%
29	17.192	2409	2415	2428	rBV	1439433	1954766	69.70%	7.358%
30	18.016	2550	2555	2569	rBV2	31569	69514	2.48%	0.262%
31	18.322	2604	2607	2608	rBV3	3379	3883	0.14%	0.015%
32	19.110	2737	2741	2744	rBV2	20057	27339	0.97%	0.103%
33	19.186	2750	2754	2759	rBV3	15094	22662	0.81%	0.085%
34	19.351	2779	2782	2786	rBV5	12272	16374	0.58%	0.062%
35	19.563	2811	2818	2826	rVB	1703267	2543312	90.68%	9.574%
36	21.521	3145	3151	3159	rVB2	1162664	2036357	72.61%	7.666%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022411.D
Acq On : 16 Oct 2024 11:19
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.568	3660	3669	3680	rVB	1052526	2804617	100.00%	10.558%
38	24.798	3699	3708	3722	rVB	737955	2151200	76.70%	8.098%




Sum of corrected areas: 26564963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022411.D
Acq On : 16 Oct 2024 11:19
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

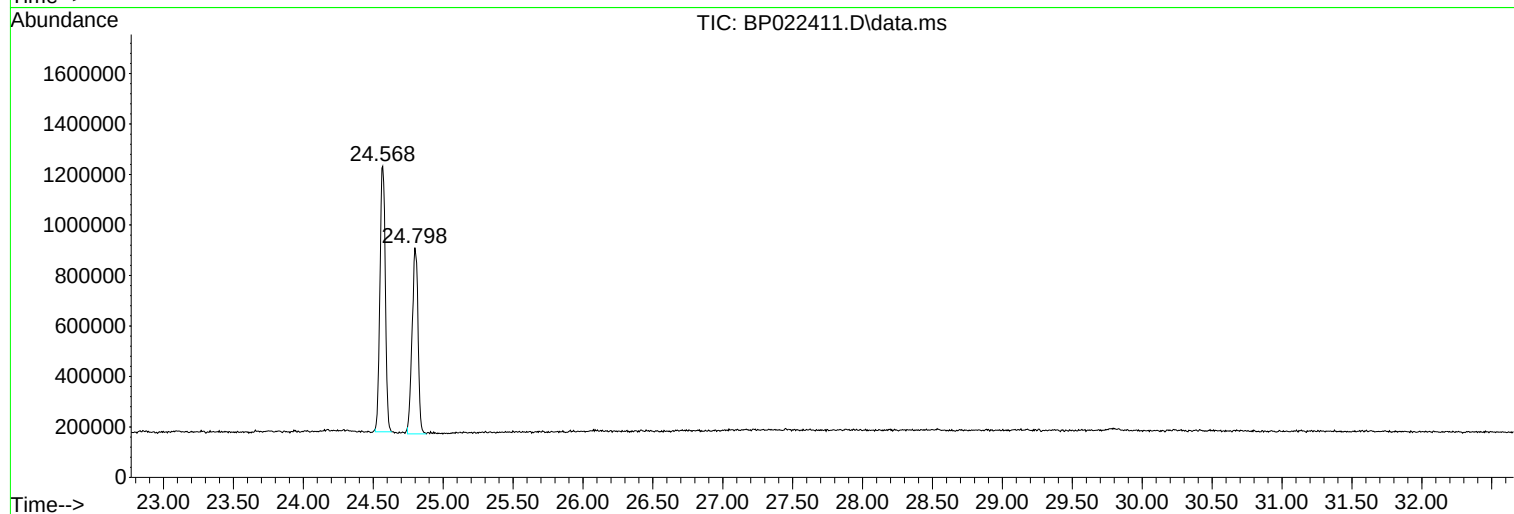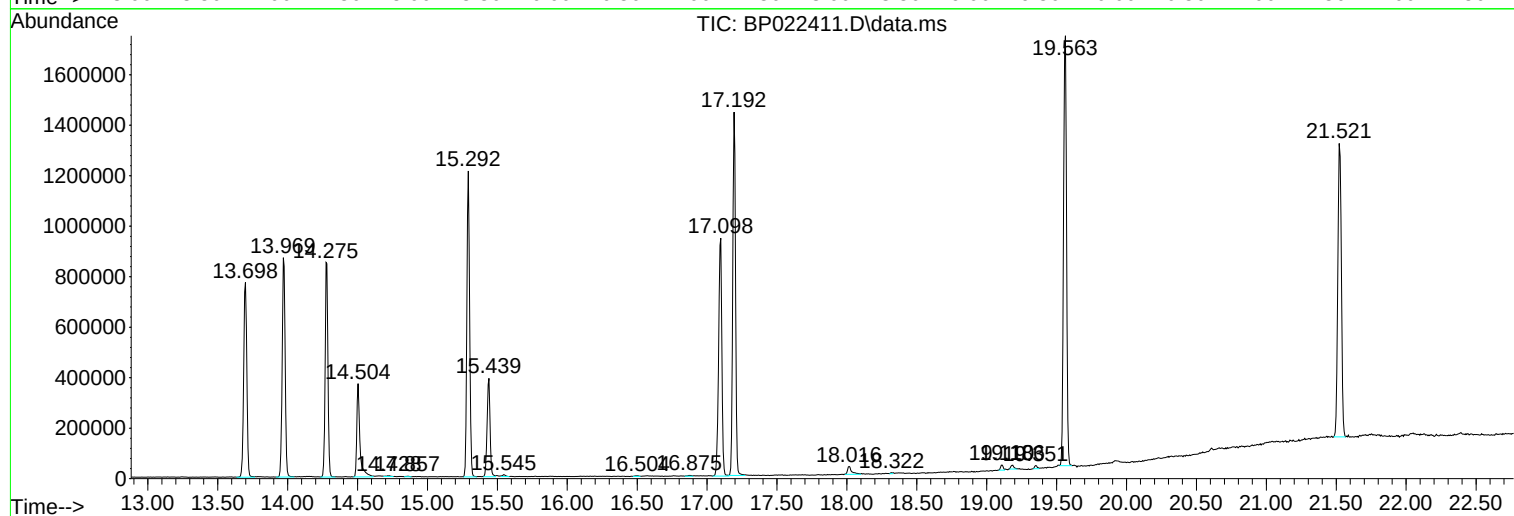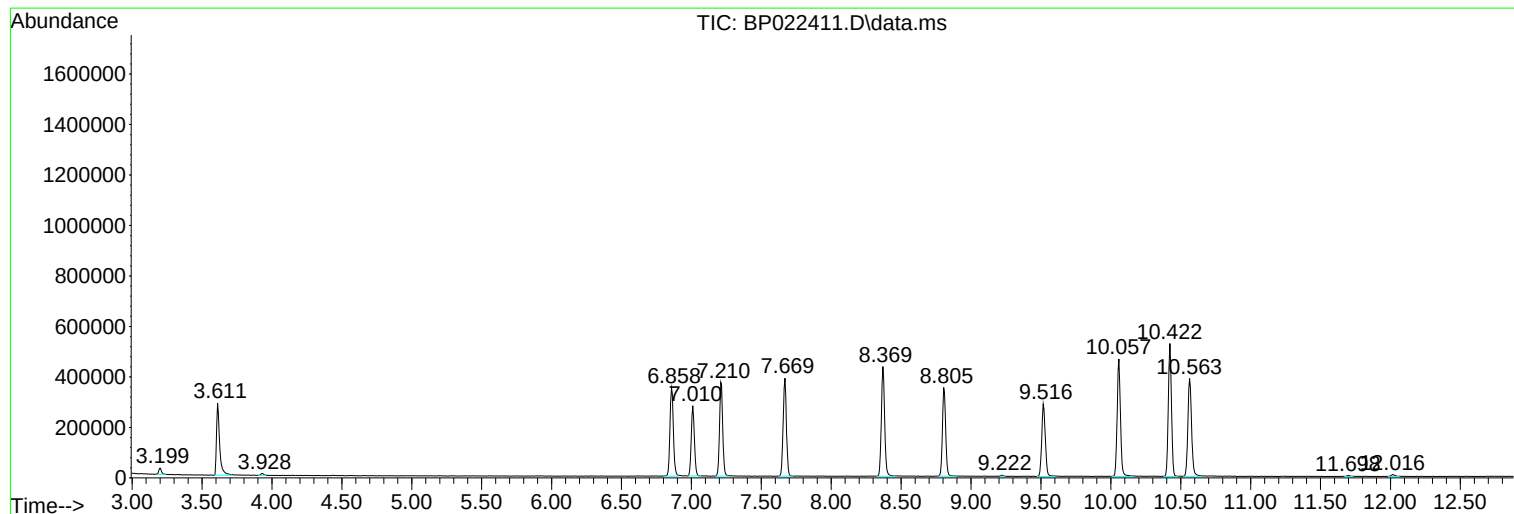

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022411.D
Acq On : 16 Oct 2024 11:19
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022411.D
Acq On : 16 Oct 2024 11:19
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc