

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
 Data File : BP022417.D
 Acq On : 16 Oct 2024 17:09
 Operator : RC/JU
 Sample : PB163941BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK941

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	33	36	47	rVB	24285	33300	1.17%	0.119%
2	3.611	102	106	121	rBV	286469	433149	15.28%	1.542%
3	3.934	154	161	168	rBV2	7740	12850	0.45%	0.046%
4	4.152	194	198	203	rBV7	2684	3828	0.14%	0.014%
5	6.858	647	658	670	rBV	357187	586010	20.68%	2.086%
6	7.011	677	684	694	rBV	275274	422106	14.89%	1.503%
7	7.211	711	718	728	rBV	377195	583219	20.58%	2.076%
8	7.663	786	795	806	rBV	388123	621518	21.93%	2.212%
9	8.363	907	914	930	rBV	428499	737030	26.00%	2.624%
10	8.810	982	990	1001	rBV	346236	584640	20.63%	2.081%
11	9.222	1055	1060	1066	rBV4	6871	10458	0.37%	0.037%
12	9.522	1101	1111	1126	rBV	302308	525878	18.55%	1.872%
13	10.057	1194	1202	1225	rBV	441069	799679	28.21%	2.847%
14	10.428	1257	1265	1273	rBV	497744	838738	29.59%	2.986%
15	10.563	1280	1288	1307	rBV	422885	754121	26.61%	2.685%
16	11.699	1476	1481	1487	rBV5	4221	7957	0.28%	0.028%
17	12.022	1528	1536	1543	rBV5	5549	12778	0.45%	0.045%
18	13.687	1812	1819	1833	rBV	946136	1338241	47.21%	4.764%
19	13.981	1857	1869	1881	rBV	942914	1441179	50.85%	5.130%
20	14.287	1912	1921	1932	rBV	731924	1293052	45.62%	4.603%
21	14.510	1950	1959	1972	rBV	256642	606469	21.40%	2.159%
22	15.287	2084	2091	2100	rBV	1233231	1872828	66.08%	6.667%
23	15.416	2108	2113	2127	rBV	567581	652785	23.03%	2.324%
24	15.528	2129	2132	2139	rVB3	6521	9789	0.35%	0.035%
25	15.869	2184	2190	2196	rBV3	2328	4767	0.17%	0.017%
26	16.569	2305	2309	2313	rVB6	2108	3328	0.12%	0.012%
27	16.757	2333	2341	2342	rBV7	2213	4004	0.14%	0.014%
28	16.857	2355	2358	2364	rVB6	3333	4992	0.18%	0.018%
29	17.087	2390	2397	2406	rBV	1113623	1739491	61.37%	6.192%
30	17.181	2407	2413	2428	rVB	1538991	2167723	76.48%	7.717%
31	18.034	2553	2558	2562	rBV5	10252	18200	0.64%	0.065%
32	19.104	2736	2740	2747	rBV3	19172	29681	1.05%	0.106%
33	19.192	2750	2755	2758	rBV2	18518	30350	1.07%	0.108%
34	19.569	2812	2819	2829	rBV	1884515	2761733	97.44%	9.831%
35	21.510	3144	3149	3159	rVB2	1431467	2112980	74.55%	7.522%
36	24.557	3657	3667	3679	rVB	929476	2834383	100.00%	10.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022417.D
Acq On : 16 Oct 2024 17:09
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.774	3695	3704	3716	rVB	800610	2198106	77.55%	7.825%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 28091340

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022417.D
Acq On : 16 Oct 2024 17:09
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

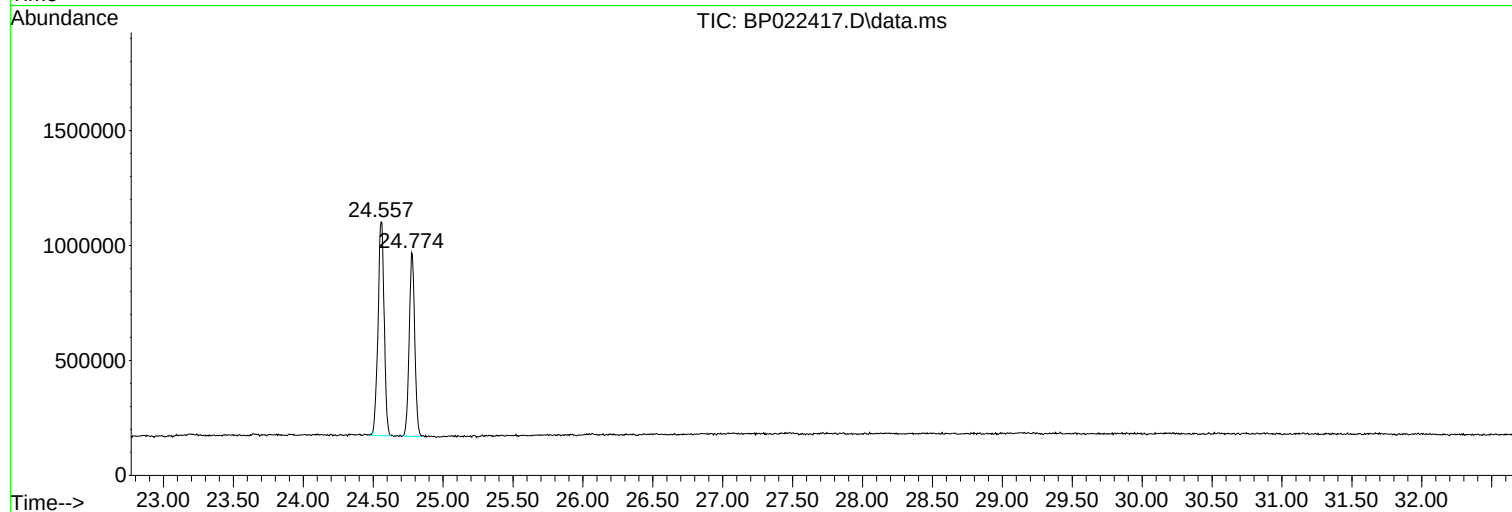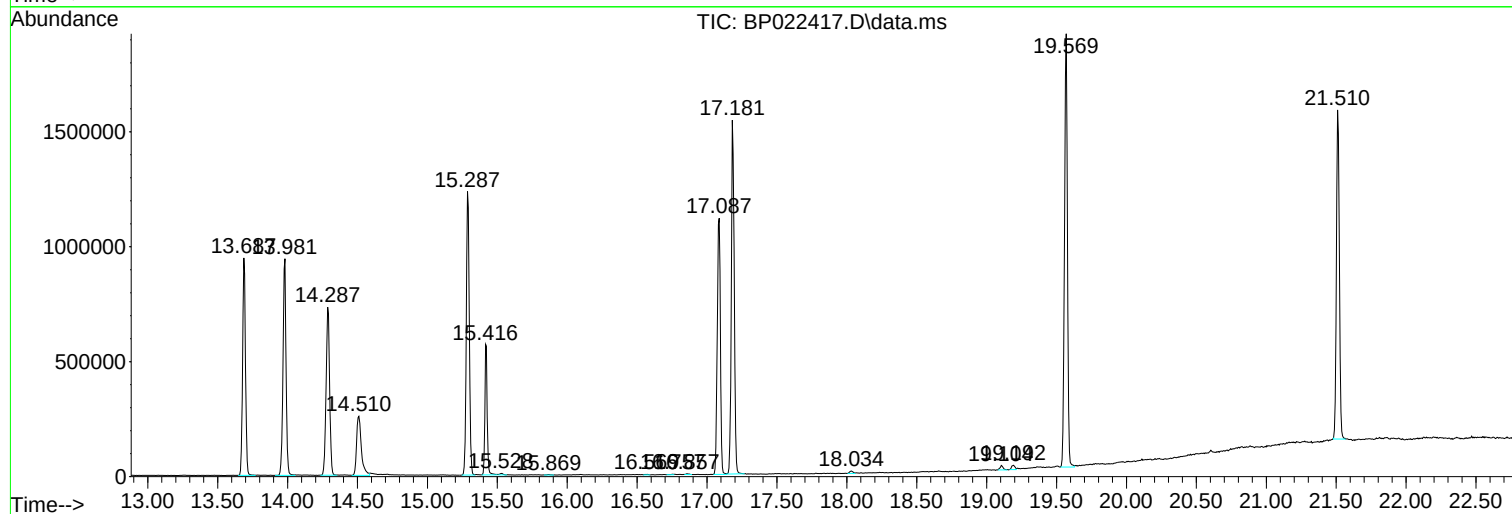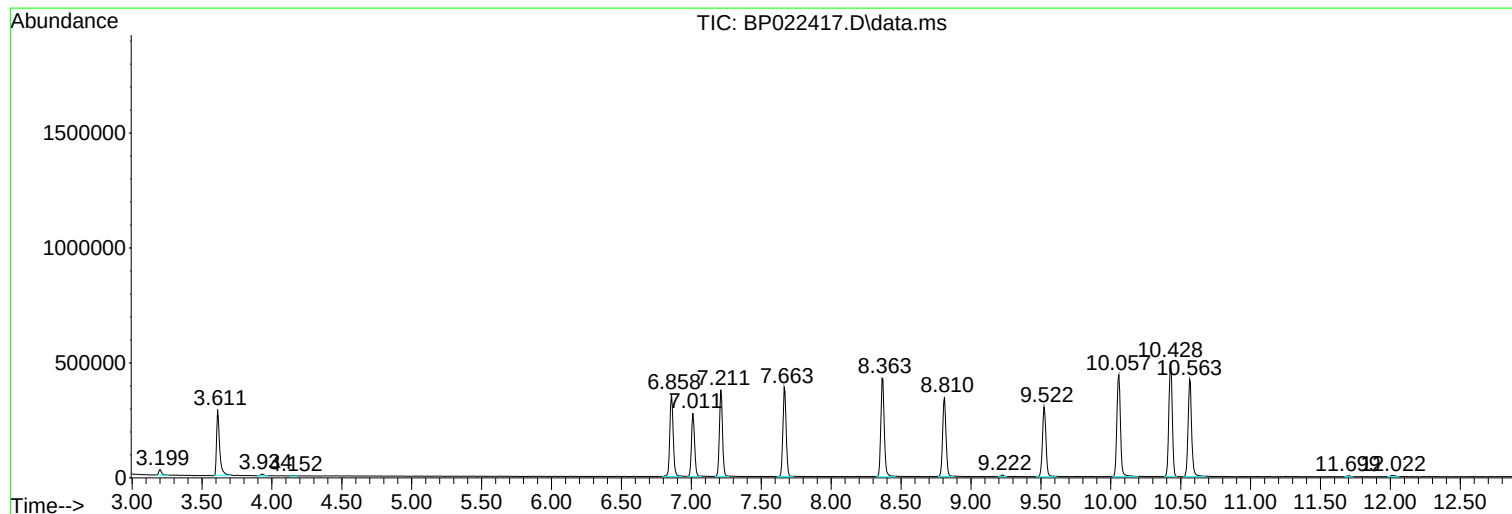

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022417.D
Acq On : 16 Oct 2024 17:09
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022417.D
Acq On : 16 Oct 2024 17:09
Operator : RC/JU
Sample : PB163941BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc