

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
 Data File : BP022443.D
 Acq On : 17 Oct 2024 12:35
 Operator : RC/JU
 Sample : P4329-07DL 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.622	105	108	114	rBV	16756	28599	0.94%	0.196%
2	3.928	155	160	172	rVB2	12709	21694	0.72%	0.149%
3	5.716	459	464	470	rBV5	3858	7045	0.23%	0.048%
4	5.822	475	482	488	rVB	17666	26905	0.89%	0.184%
5	6.728	631	636	640	rBV3	5182	7028	0.23%	0.048%
6	6.811	644	650	654	rVV	38262	57939	1.91%	0.397%
7	6.858	654	658	672	rVB	28020	55754	1.84%	0.382%
8	7.005	679	683	693	rVB	23231	38459	1.27%	0.264%
9	7.210	711	718	729	rBV	32211	59922	1.98%	0.411%
10	7.663	788	795	803	rBV	368594	601169	19.84%	4.120%
11	8.369	910	915	925	rBV	31870	63891	2.11%	0.438%
12	8.810	982	990	996	rBV2	25329	49139	1.62%	0.337%
13	9.210	1049	1058	1067	rBV	64245	101199	3.34%	0.694%
14	9.369	1081	1085	1093	rBV	2122	3350	0.11%	0.023%
15	9.516	1104	1110	1119	rVB	25472	43805	1.45%	0.300%
16	10.063	1195	1203	1213	rBV2	31854	69485	2.29%	0.476%
17	10.416	1256	1263	1271	rBV	442144	807284	26.65%	5.533%
18	10.563	1280	1288	1296	rBV	28860	60936	2.01%	0.418%
19	11.693	1474	1480	1486	rVB2	27183	44925	1.48%	0.308%
20	13.698	1814	1821	1829	rBV	95638	164179	5.42%	1.125%
21	13.969	1861	1867	1878	rBV2	87798	144031	4.75%	0.987%
22	14.275	1911	1919	1927	rBV	823122	1259693	41.58%	8.634%
23	14.416	1939	1943	1946	rBV3	4082	4442	0.15%	0.030%
24	14.528	1956	1962	1966	rBV6	9543	21599	0.71%	0.148%
25	15.281	2084	2090	2097	rBV2	145832	232881	7.69%	1.596%
26	15.345	2097	2101	2107	rVB6	4402	7387	0.24%	0.051%
27	15.434	2111	2116	2125	rBV3	21055	35955	1.19%	0.246%
28	15.545	2130	2135	2140	rVB	27145	36255	1.20%	0.248%
29	15.663	2147	2155	2162	rBV	24073	45652	1.51%	0.313%
30	15.992	2208	2211	2215	rBV6	1645	3216	0.11%	0.022%
31	16.057	2218	2222	2230	rVB10	3937	7303	0.24%	0.050%
32	16.181	2235	2243	2248	rBV10	6965	12310	0.41%	0.084%
33	16.286	2257	2261	2267	rVB2	10833	16575	0.55%	0.114%
34	16.481	2290	2294	2297	rBV5	4801	6519	0.22%	0.045%
35	16.563	2303	2308	2311	rBV3	17220	26738	0.88%	0.183%
36	16.592	2311	2313	2319	rVB6	12150	16866	0.56%	0.116%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
 Data File : BP022443.D
 Acq On : 17 Oct 2024 12:35
 Operator : RC/JU
 Sample : P4329-07DL 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	16.722	2331	2335	2339	rBV7	3060	5000	0.17%	0.034%
38	16.945	2370	2373	2376	rBV5	8699	11036	0.36%	0.076%
39	16.981	2376	2379	2384	rVB3	10516	12324	0.41%	0.084%
40	17.075	2387	2395	2401	rBV	1167788	1724685	56.93%	11.821%
41	17.181	2407	2413	2423	rBV	147532	226380	7.47%	1.552%
42	17.269	2424	2428	2435	rVV4	15866	22437	0.74%	0.154%
43	17.557	2474	2477	2480	rBV5	5368	7367	0.24%	0.050%
44	17.675	2493	2497	2505	rVB3	24013	48482	1.60%	0.332%
45	17.816	2519	2521	2528	rVB8	3761	5089	0.17%	0.035%
46	18.010	2549	2554	2560	rBV3	55991	105541	3.48%	0.723%
47	18.080	2560	2566	2572	rVB	2357158	3029634	100.00%	20.765%
48	18.422	2621	2624	2627	rBV5	8316	10234	0.34%	0.070%
49	18.657	2660	2664	2668	rVB6	16108	23630	0.78%	0.162%
50	19.210	2755	2758	2762	rVB	23302	23481	0.78%	0.161%
51	19.339	2777	2780	2788	rVB6	41317	60594	2.00%	0.415%
52	19.557	2812	2817	2825	rBV	238326	358871	11.85%	2.460%
53	20.586	2989	2992	2997	rVB	86608	96930	3.20%	0.664%
54	21.504	3142	3148	3154	rBV2	1256478	2142677	70.72%	14.686%
55	24.762	3693	3702	3715	rVB	907405	2485746	82.05%	17.037%




Sum of corrected areas: 14590267

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022443.D
Acq On : 17 Oct 2024 12:35
Operator : RC/JU
Sample : P4329-07DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EN4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

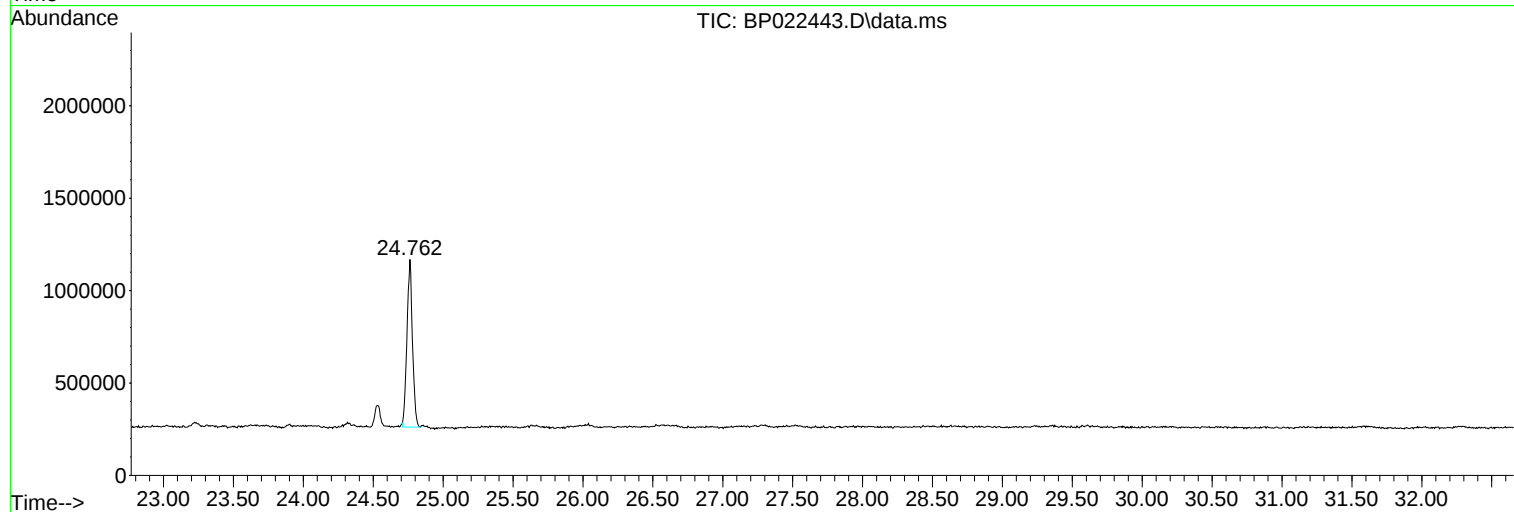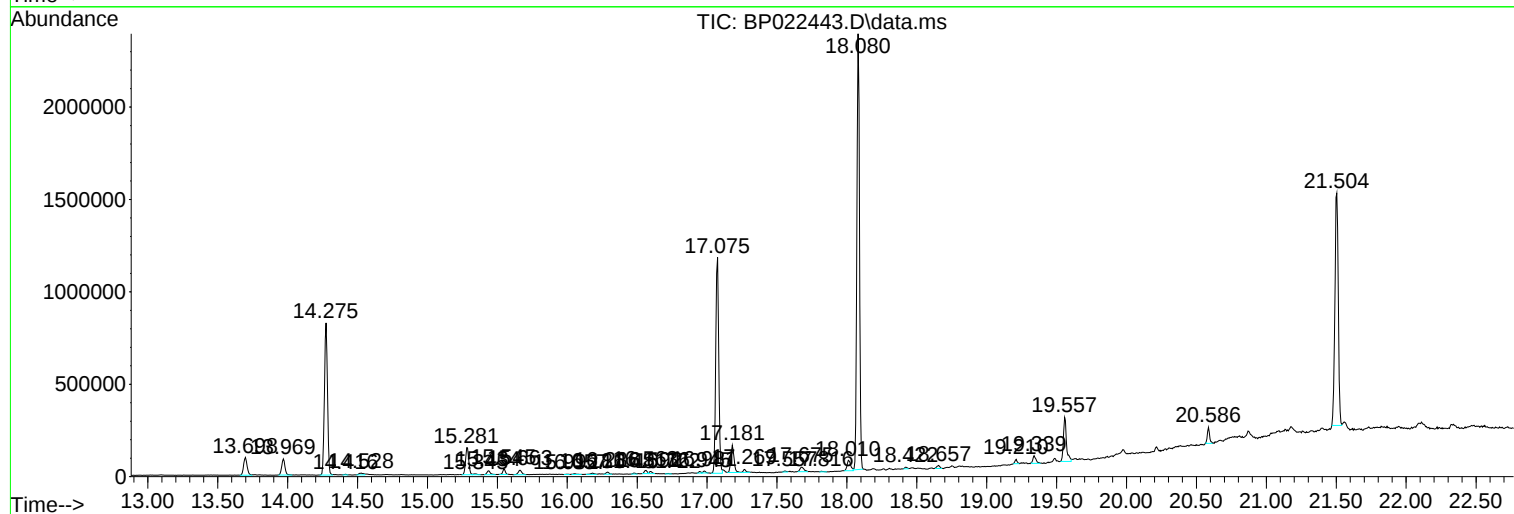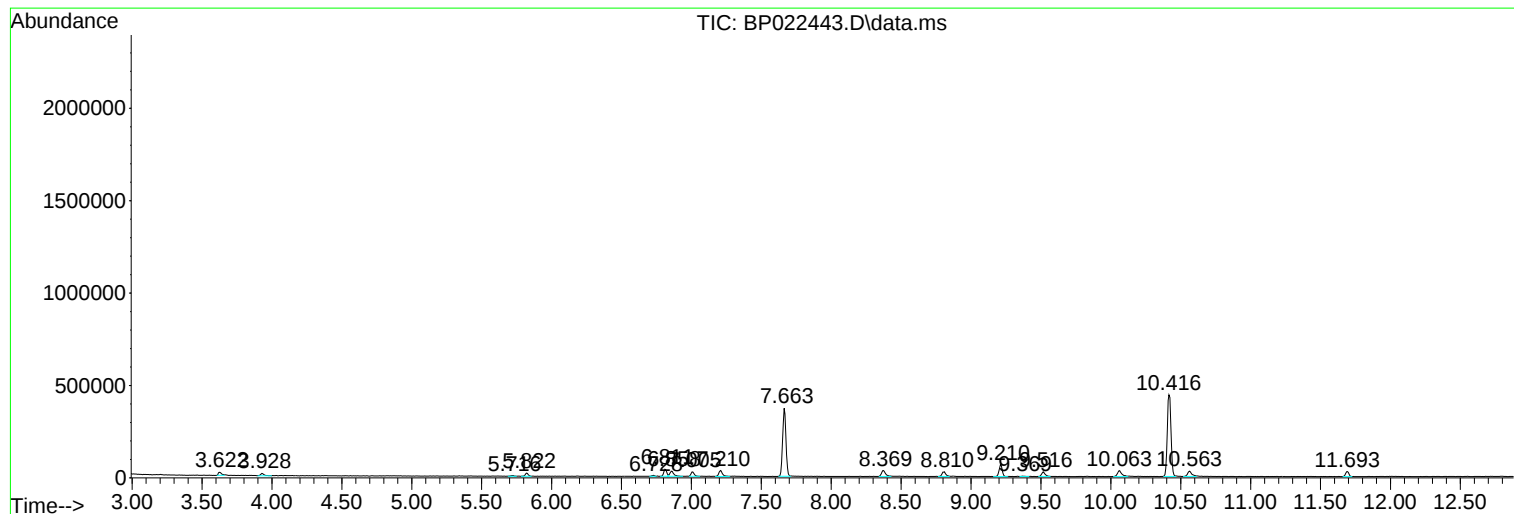

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022443.D
Acq On : 17 Oct 2024 12:35
Operator : RC/JU
Sample : P4329-07DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EN4DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.210	2.51 ng/ul	101199	Naphthalene-d8	10.416

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
2			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
3			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
4			4-(2-amino-1-hydroxypropyl)pheno...	311	C15H29NO2Si2	1000478-98-6	46
5			2,5-Dihydroxybenzaldehyde, 2TMS ...	282	C13H22O3Si2	056114-69-3	43

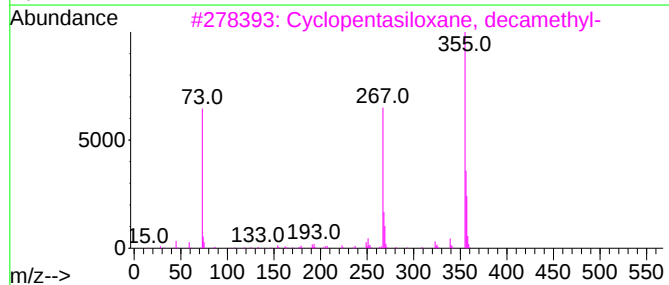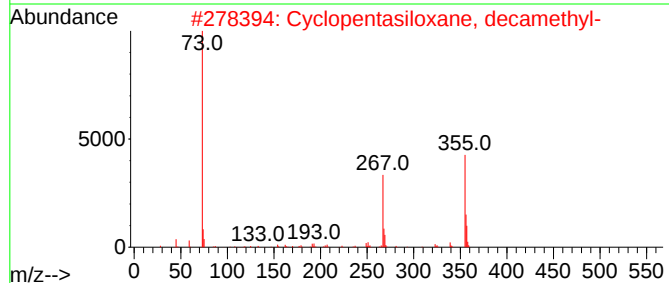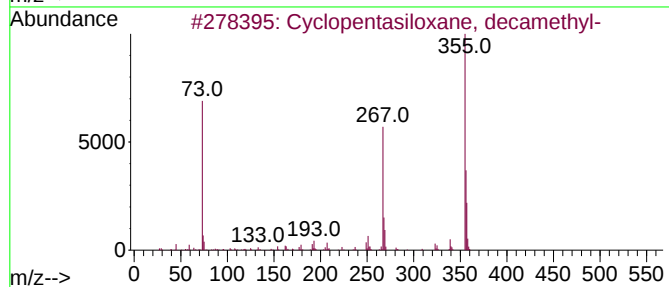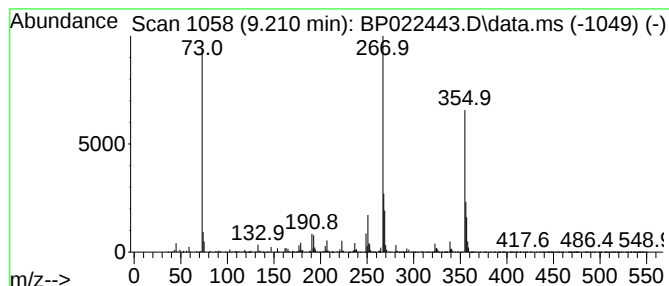

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101624\
Data File : BP022443.D
Acq On : 17 Oct 2024 12:35
Operator : RC/JU
Sample : P4329-07DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EN4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasilox...	9.210	2.5	ng/ul	101199	2	10.416	807284	20.0