

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101722\
 Data File : BP012169.D
 Acq On : 17 Oct 2022 17:12
 Operator : CG/JU
 Sample : SST08078
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080642

Quant Time: Oct 18 01:16:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 18 01:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	428900	20.000	ng/u1	0.00
20) Naphthalene-d8	10.640	136	1813449	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.486	164	989324	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	1798859	20.000	ng/u1	0.00
79) Chrysene-d12	21.339	240	1514502	20.000	ng/u1	0.00
88) Perylene-d12	23.751	264	1679043	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	344435	31.662	ng/uL	0.00
4) Pyridine-d5	3.681	84	2501378	86.462	ng/u1	0.00
7) Phenol-d5	7.010	99	3039486	88.115	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	1768214	90.309	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	2329032	85.060	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	2288229	86.364	ng/u1	0.01
21) Nitrobenzene-d5	9.010	128	1146321	89.504	ng/u1	0.00
24) 2-Nitrophenol-d4	9.728	143	1254649	96.611	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.269	165	2179618	86.601	ng/u1	0.00
31) 4-Chloroaniline-d4	10.787	131	2890009	77.921	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	5075231	81.002	ng/u1	0.00
49) Acenaphthylene-d8	14.181	160	6280965	81.067	ng/u1	0.00
54) 4-Nitrophenol-d4	14.710	143	973076	79.108	ng/u1	0.01
60) Fluorene-d10	15.486	176	4318190	76.175	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	856790	90.202	ng/u1	0.00
73) Anthracene-d10	17.351	188	6103549	78.137	ng/u1	0.00
81) Pyrene-d10	19.586	212	6419383	82.736	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.598	264	6808183	83.411	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.299	88	372912	32.576	ng/uL	97
5) Pyridine	3.705	79	2440068	88.027	ng/u1	97
6) Benzaldehyde	6.981	77	1207672	74.620	ng/u1	98
8) Phenol	7.040	94	3161056	87.290	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.269	93	2478837	86.759	ng/u1	97
12) 2-Chlorophenol	7.399	128	2472299	83.198	ng/u1	98
13) 2-Methylphenol	8.287	108	2361333	87.426	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.375	45	3243975	110.770	ng/u1	99
16) Acetophenone	8.675	105	3415473	83.615	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.669	70	1671681	89.853	ng/u1	99
18) 4-Methylphenol	8.628	108	2499813	85.869	ng/u1	99
19) Hexachloroethane	8.910	117	967290	84.325	ng/u1	94
22) Nitrobenzene	9.051	77	2625719	89.434	ng/u1	97
23) Isophorone	9.587	82	4898268	94.058	ng/u1	100
25) 2-Nitrophenol	9.763	139	1381247	90.529	ng/u1	96
26) 2,4-Dimethylphenol	9.822	107	2536171	85.351	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.063	93	3141900	87.918	ng/u1	99
29) 2,4-Dichlorophenol	10.293	162	2205428	83.383	ng/u1	99
30) Naphthalene	10.693	128	7341966	76.615	ng/u1	99
32) 4-Chloroaniline	10.816	127	2974097	77.777	ng/u1	100
33) Hexachlorobutadiene	10.969	225	1387792	84.614	ng/u1	99
34) Caprolactam	11.634	113	343911	47.318	ng/u1	94
35) 4-Chloro-3-methylphenol	11.945	107	2250838	89.827	ng/u1	98
36) 2-Methylnaphthalene	12.304	142	4845397	78.523	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101722\
 Data File : BP012169.D
 Acq On : 17 Oct 2022 17:12
 Operator : CG/JU
 Sample : SSTD08078
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080642


Quant Time: Oct 18 01:16:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 18 01:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.528	142	4758391	77.001	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.675	216	2512731	83.087	ng/ul	99
40) Hexachlorocyclopentadiene	12.645	237	1490430	101.464	ng/ul	99
41) 2,4,6-Trichlorophenol	12.922	196	1658921	91.064	ng/ul	99
42) 2,4,5-Trichlorophenol	12.992	196	1752660	88.525	ng/ul	99
43) 1,1'-Biphenyl	13.322	154	5806670	77.746	ng/ul	100
44) 2-Chloronaphthalene	13.363	162	4665422	78.224	ng/ul	99
45) 2-Nitroaniline	13.575	65	1302284	102.358	ng/ul	99
47) Dimethylphthalate	13.951	163	5242415	79.415	ng/ul	99
48) 2,6-Dinitrotoluene	14.075	165	1139114	97.466	ng/ul	93
50) Acenaphthylene	14.210	152	6797517	77.538	ng/ul	99
51) 3-Nitroaniline	14.404	138	1096669	80.584	ng/ul	93
52) Acenaphthene	14.551	153	4674524	74.902	ng/ul	99
53) 2,4-Dinitrophenol	14.616	184	702789	93.080	ng/ul	95
55) 4-Nitrophenol	14.722	109	698256	82.108	ng/ul	91
56) Dibenzofuran	14.886	168	6189602	73.384	ng/ul	96
57) 2,4-Dinitrotoluene	14.863	165	1514793	90.183	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	15.116	232	1375572	89.140	ng/ul	98
59) Diethylphthalate	15.322	149	5002738	82.750	ng/ul	99
61) Fluorene	15.539	166	4581508	69.198	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.534	204	2287451	71.418	ng/ul	98
63) 4-Nitroaniline	15.575	138	829942	66.788	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.634	198	903890	88.025	ng/ul#	92
67) N-Nitrosodiphenylamine	15.751	169	4125464	77.482	ng/ul	100
68) 4-Bromophenyl-phenylether	16.433	248	1558495	89.035	ng/ul	100
69) Hexachlorobenzene	16.545	284	1798051	88.500	ng/ul	97
70) Atrazine	16.716	200	1388612	84.811	ng/ul	100
71) Pentachlorophenol	16.892	266	1109182	93.182	ng/ul	98
72) Phenanthrene	17.292	178	7320763	74.833	ng/ul	99
74) Anthracene	17.380	178	7232196	74.705	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.281	216	2490153	85.666	ng/ul	99
76) Pentachlorobenzene	14.804	250	2405950	84.278	ng/ul	98
77) Carbazole	17.657	167	6473991	74.979	ng/ul	98
78) Di-n-butylphthalate	18.204	149	7793396	90.955	ng/ul	99
80) Fluoranthene	19.263	202	7867728	82.755	ng/ul	98
82) Pyrene	19.616	202	7935078	78.867	ng/ul	99
83) Butylbenzylphthalate	20.486	149	3391615	106.339	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.257	252	2776344	83.190	ng/ul	100
85) Benzo(a)anthracene	21.321	228	7582535	79.540	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.245	149	4641992	107.962	ng/ul#	96
87) Chrysene	21.380	228	7137628	77.784	ng/ul	98
89) Di-n-octyl phthalate	22.168	149	8147840	96.928	ng/ul	100
90) Benzo(b)fluoranthene	23.015	252	8449633	79.503	ng/ul	99
91) Benzo(k)fluoranthene	23.068	252	8192185	78.364	ng/ul	99
93) Benzo(a)pyrene	23.651	252	7543102	79.552	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.274	276	9860194	82.242	ng/ul	99
95) Dibenzo(a,h)anthracene	26.292	278	8721522	81.087	ng/ul	99
96) Benzo(g,h,i)perylene	27.045	276	8922136	82.538	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 18 01:16:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 18 01:11:56 2022
Response via : Initial Calibration







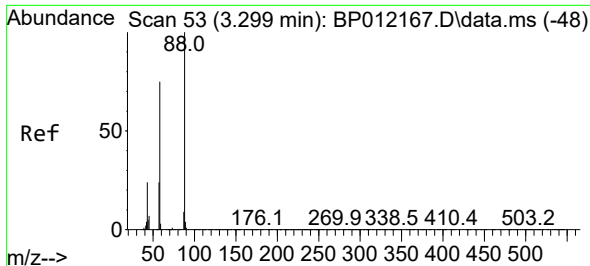

#2
 1,4-Dioxane
 Concen: 32.576 ng/uL
 RT: 3.299 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP012169.D
 Acq: 17 Oct 2022 17:12




Instrument :
 BNA_P
 ClientSampleId :
 SSTD080642


Tgt Ion: 88 Resp: 372912
 Ion Ratio Lower Upper
 88 100
 43 25.0 19.6 29.4
 58 71.3 59.1 88.7

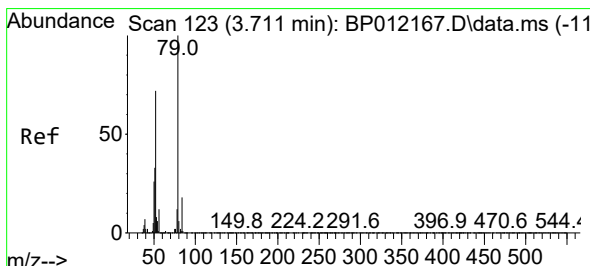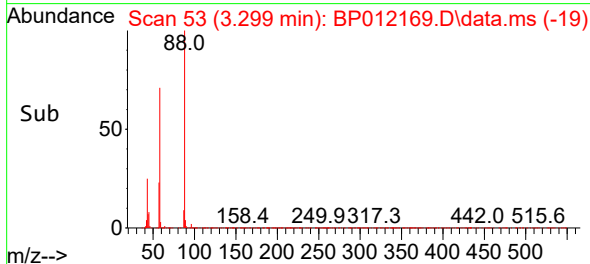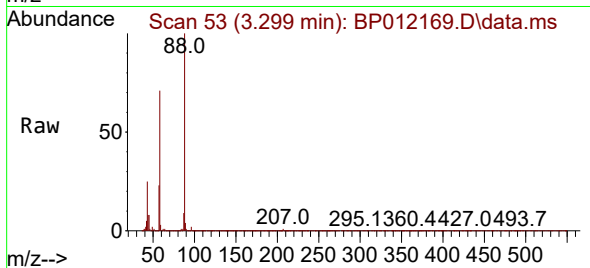

#5
 Pyridine
 Concen: 88.027 ng/uL
 RT: 3.705 min Scan# 122
 Delta R.T. -0.006 min
 Lab File: BP012169.D
 Acq: 17 Oct 2022 17:12

Tgt Ion: 79 Resp: 2440068
 Ion Ratio Lower Upper
 79 100
 52 70.1 57.9 86.9
 51 32.1 26.7 40.1


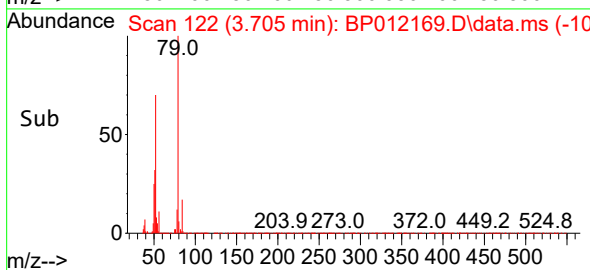

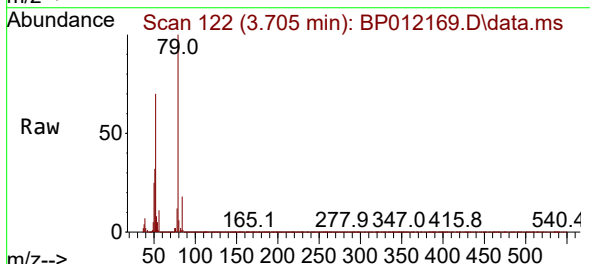




#6
Benzaldehyde
Concen: 74.620 ng/ul
RT: 6.981 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion: 77 Resp: 1207672
Ion Ratio Lower Upper
77 100
105 102.3 82.9 124.3
106 98.3 80.8 121.2

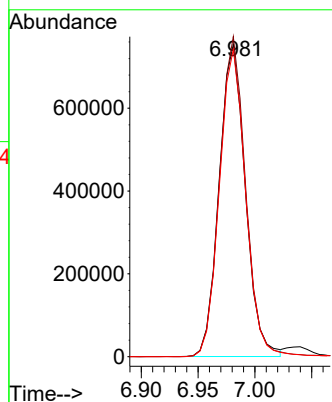

#8
Phenol
Concen: 87.290 ng/ul
RT: 7.040 min Scan# 689
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion: 94 Resp: 3161056
Ion Ratio Lower Upper
94 100
65 26.0 21.9 32.9
66 32.9 26.6 40.0



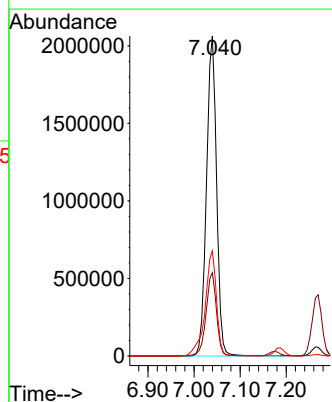
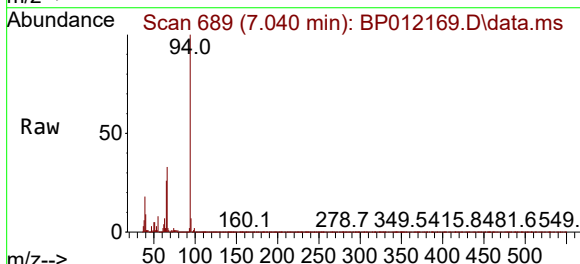




#10
Bis(2-Chloroethyl)ether
Concen: 86.759 ng/ul
RT: 7.269 min Scan# 71
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion: 93 Resp: 2478837
Ion Ratio Lower Upper
93 100
63 73.7 61.9 92.9
95 32.9 27.0 40.4



#12
2-Chlorophenol
Concen: 83.198 ng/ul
RT: 7.399 min Scan# 750
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:128 Resp: 2472299
Ion Ratio Lower Upper
128 100
64 44.5 37.2 55.8
130 32.2 25.8 38.8





#13

2-Methylphenol

Concen: 87.426 ng/ul

RT: 8.287 min Scan# 901

Delta R.T. -0.000 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :





SSTD080642

Tgt Ion:108 Resp: 2361333

Ion Ratio Lower Upper

108 100

107 88.0 70.2 105.2

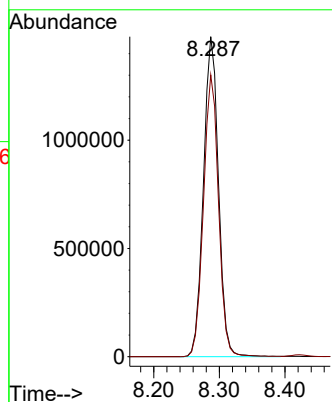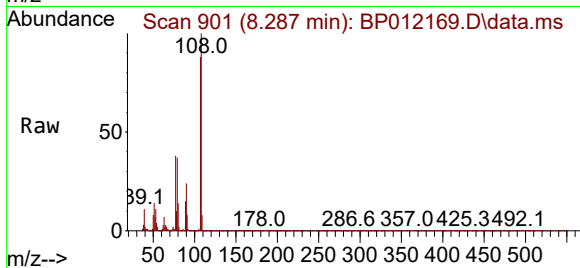

#14

2,2'-oxybis(1-Chloropropane)

Concen: 110.770 ng/ul

RT: 8.375 min Scan# 916

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12




Tgt Ion: 45 Resp: 3243975


Ion Ratio Lower Upper

45 100

77 14.9 12.5 18.7

79 11.8 9.4 14.2









#16
Acetophenone
Concen: 83.615 ng/ul
RT: 8.675 min Scan# 90
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:105 Resp: 3415473
Ion Ratio Lower Upper
105 100
77 74.0 59.8 89.6
51 24.0 20.4 30.6



#17
N-Nitroso-di-n-propylamine
Concen: 89.853 ng/ul
RT: 8.669 min Scan# 966
Delta R.T. 0.018 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion: 70 Resp: 1671681
Ion Ratio Lower Upper
70 100
42 52.4 42.6 64.0
101 10.3 7.8 11.6
130 22.3 17.3 25.9









#18
4-Methylphenol
Concen: 85.869 ng/ul
RT: 8.628 min Scan# 91
Delta R.T. 0.018 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:108 Resp: 2499813
Ion Ratio Lower Upper
108 100
107 109.7 88.9 133.3



#19
Hexachloroethane
Concen: 84.325 ng/ul
RT: 8.910 min Scan# 1007
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:117 Resp: 967290
Ion Ratio Lower Upper
117 100
201 99.6 73.9 110.9
199 61.9 47.0 70.6









#22
Nitrobenzene
Concen: 89.434 ng/ul
RT: 9.051 min Scan# 1031
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion: 77 Resp: 2625719
Ion Ratio Lower Upper
77 100
123 48.5 36.8 55.2
65 13.1 10.0 15.0



#23
Isophorone
Concen: 94.058 ng/ul
RT: 9.587 min Scan# 1122
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion: 82 Resp: 4898268
Ion Ratio Lower Upper
82 100
95 6.6 5.3 7.9
138 18.0 14.2 21.4









#25
2-Nitrophenol
Concen: 90.529 ng/ul
RT: 9.763 min Scan# 1151
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:139 Resp: 1381247
Ion Ratio Lower Upper
139 100
65 46.1 40.4 60.6
109 27.3 22.2 33.2



#26
2,4-Dimethylphenol
Concen: 85.351 ng/ul
RT: 9.822 min Scan# 1162
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:107 Resp: 2536171
Ion Ratio Lower Upper
107 100
121 50.7 41.2 61.8
122 88.2 70.5 105.7









#27
 Bis(2-Chloroethoxy)methane
 Concen: 87.918 ng/ul
 RT: 10.063 min Scan# 1203
 Delta R.T. 0.006 min
 Lab File: BP012169.D
 Acq: 17 Oct 2022 17:12




Instrument :
 BNA_P
 ClientSampleId :
 SSTD080642


Tgt Ion: 93 Resp: 3141900
 Ion Ratio Lower Upper
 93 100
 95 32.6 26.2 39.2
 123 11.3 8.5 12.7



#29
 2,4-Dichlorophenol
 Concen: 83.383 ng/ul
 RT: 10.293 min Scan# 1242
 Delta R.T. 0.006 min
 Lab File: BP012169.D
 Acq: 17 Oct 2022 17:12

Tgt Ion:162 Resp: 2205428
 Ion Ratio Lower Upper
 162 100
 164 65.3 52.1 78.1
 98 36.0 29.4 44.0



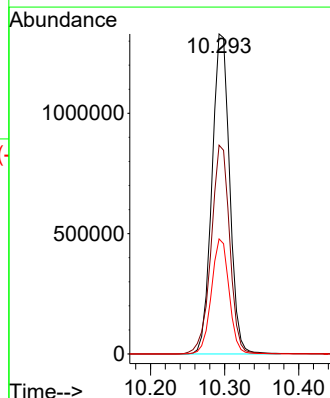
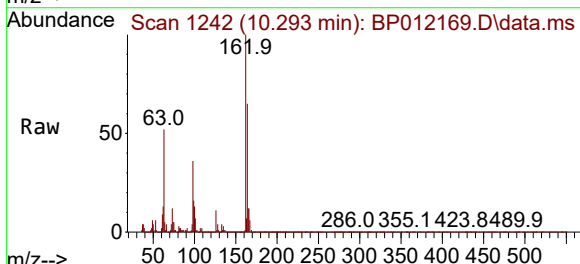




#30
Naphthalene
Concen: 76.615 ng/ul
RT: 10.693 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:128 Resp: 7341966
Ion Ratio Lower Upper
128 100
129 11.2 8.8 13.2
127 13.2 10.3 15.5



#32
4-Chloroaniline
Concen: 77.777 ng/ul
RT: 10.816 min Scan# 1331
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:127 Resp: 2974097
Ion Ratio Lower Upper
127 100
129 32.4 25.8 38.8




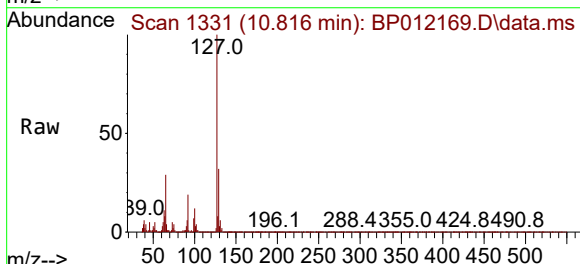


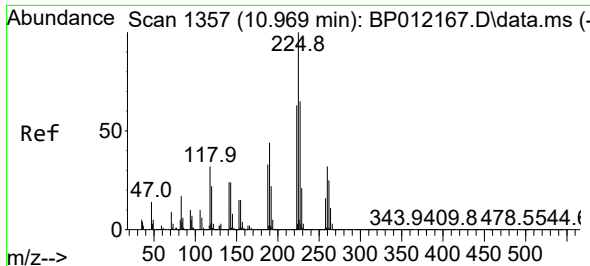

#33
Hexachlorobutadiene
Concen: 84.614 ng/ul
RT: 10.969 min Scan# 1
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:225 Resp: 1387792
Ion Ratio Lower Upper
225 100
223 63.9 50.4 75.6
227 64.3 51.9 77.9

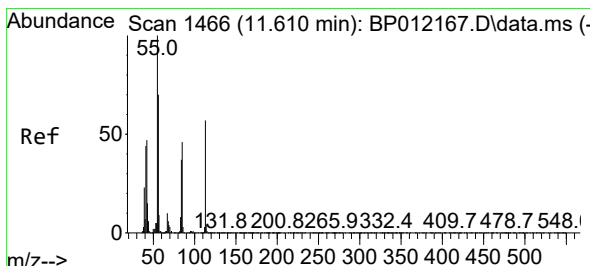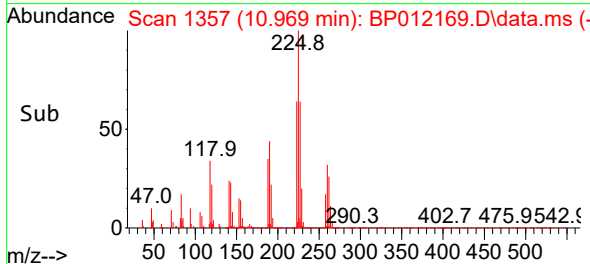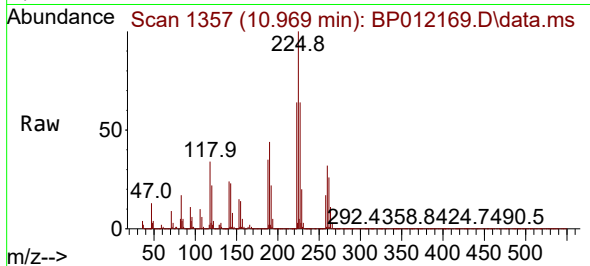

#34
Caprolactam
Concen: 47.318 ng/ul
RT: 11.634 min Scan# 1470
Delta R.T. 0.023 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:113 Resp: 343911
Ion Ratio Lower Upper
113 100
55 165.6 141.1 211.7
56 119.7 98.3 147.5


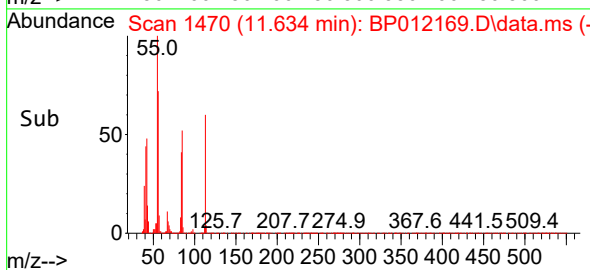

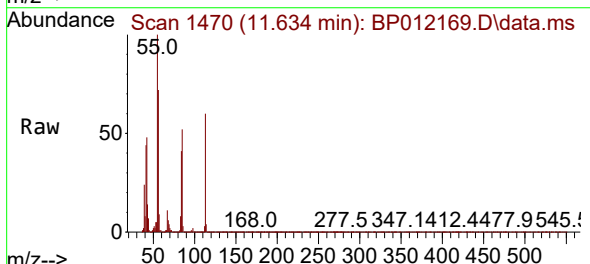




#35
4-Chloro-3-methylphenol
Concen: 89.827 ng/ul
RT: 11.945 min Scan# 1523
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:107 Resp: 2250838
Ion Ratio Lower Upper
107 100
144 26.8 21.0 31.4
142 83.1 65.1 97.7



#36
2-Methylnaphthalene
Concen: 78.523 ng/ul
RT: 12.304 min Scan# 1584
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:142 Resp: 4845397
Ion Ratio Lower Upper
142 100
141 87.9 71.3 106.9









#37
1-Methylnaphthalene
Concen: 77.001 ng/ul
RT: 12.528 min Scan# 1621
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:142 Resp: 4758391
Ion Ratio Lower Upper
142 100
141 91.7 73.1 109.7
116 3.8 2.8 4.2



#39
1,2,4,5-Tetrachlorobenzene
Concen: 83.087 ng/ul
RT: 12.675 min Scan# 1647
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:216 Resp: 2512731
Ion Ratio Lower Upper
216 100
214 78.6 62.5 93.7
179 20.5 16.8 25.2
108 16.8 14.1 21.1









#40
Hexachlorocyclopentadiene
Concen: 101.464 ng/ul
RT: 12.645 min Scan# 1642
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:237 Resp: 1490430
Ion Ratio Lower Upper
237 100
235 62.8 49.4 74.0
272 13.2 11.1 16.7

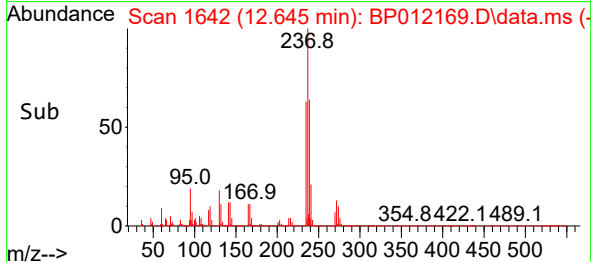

#41
2,4,6-Trichlorophenol
Concen: 91.064 ng/ul
RT: 12.922 min Scan# 1689
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:196 Resp: 1658921
Ion Ratio Lower Upper
196 100
198 96.1 77.6 116.4
200 31.4 23.8 35.8

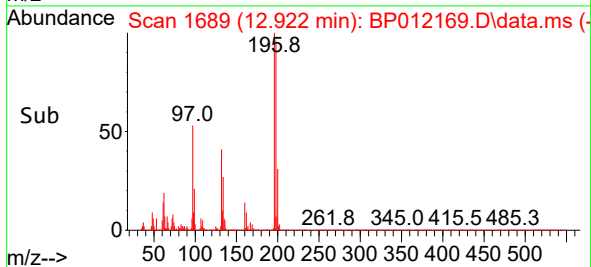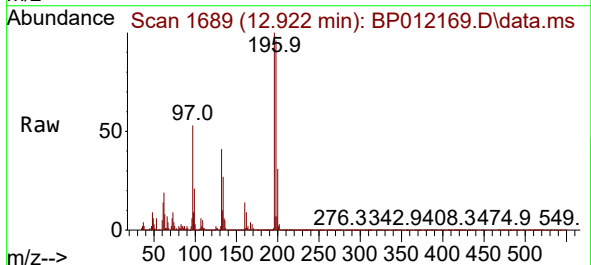

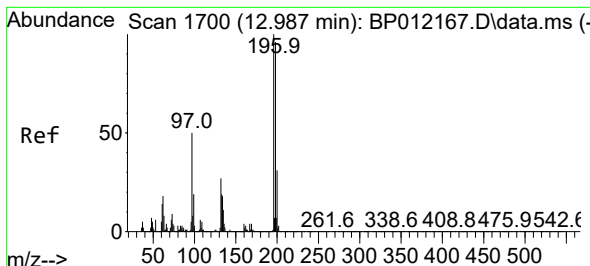

#42

2,4,5-Trichlorophenol

Concen: 88.525 ng/ul

RT: 12.992 min Scan# 1701

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:196 Resp: 1752660

Ion Ratio Lower Upper

196 100

198 95.0 76.7 115.1

200 31.1 24.4 36.6

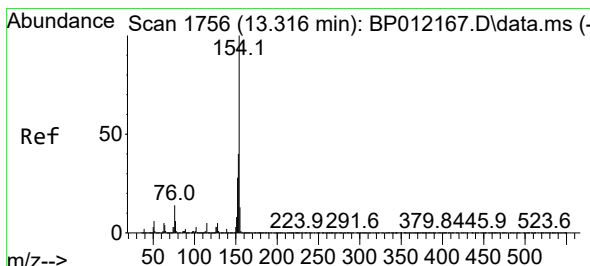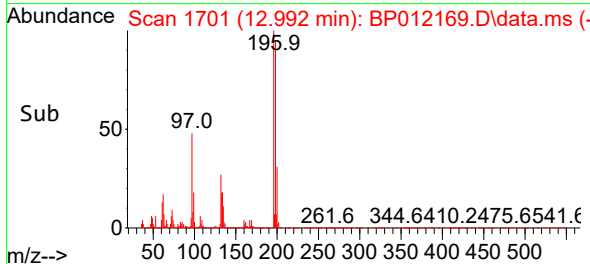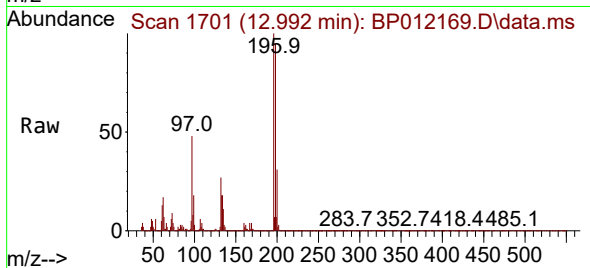

#43

1,1'-Biphenyl

Concen: 77.746 ng/ul

RT: 13.322 min Scan# 1757

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12




Tgt Ion:154 Resp: 5806670


Ion Ratio Lower Upper

154 100

153 40.2 32.3 48.5

76 13.4 11.0 16.6


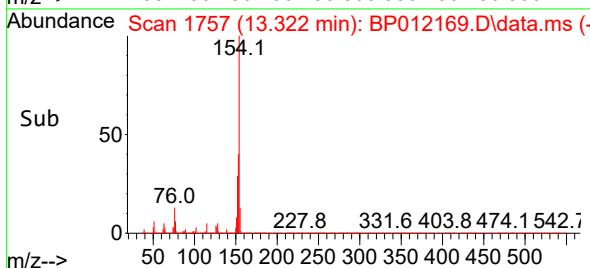
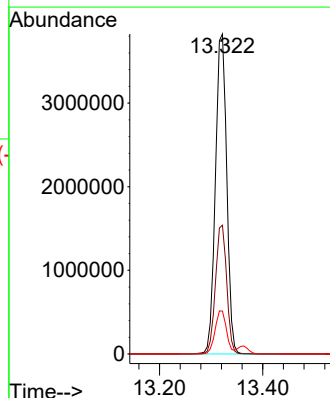
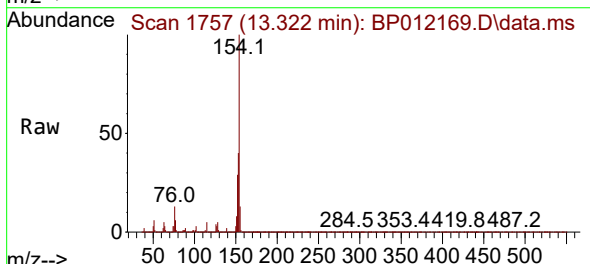




#44
2-Chloronaphthalene
Concen: 78.224 ng/ul
RT: 13.363 min Scan# 1763
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:162 Resp: 4665422
Ion Ratio Lower Upper
162 100
164 33.2 26.4 39.6
127 39.0 30.4 45.6



#45
2-Nitroaniline
Concen: 102.358 ng/ul
RT: 13.575 min Scan# 1800
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion: 65 Resp: 1302284
Ion Ratio Lower Upper
65 100
92 71.9 57.1 85.7
138 111.7 90.5 135.7

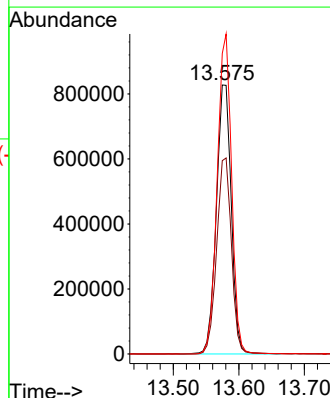



#47

Dimethylphthalate

Concen: 79.415 ng/ul

RT: 13.951 min Scan# 1864

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:163 Resp: 5242415

Ion Ratio Lower Upper

163 100

194 4.1 3.0 4.6

164 10.4 8.2 12.2

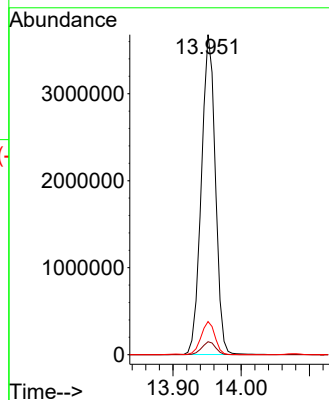

#48

2,6-Dinitrotoluene

Concen: 97.466 ng/ul

RT: 14.075 min Scan# 1885

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12




Tgt Ion:165 Resp: 1139114


Ion Ratio Lower Upper

165 100

89 54.9 48.2 72.4

121 21.0 19.0 28.4



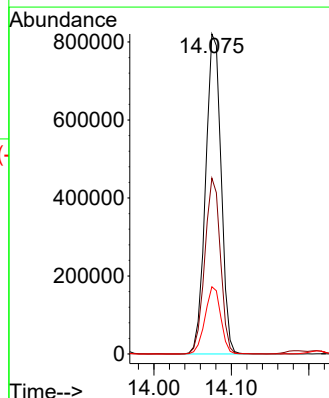





#50
Acenaphthylene
Concen: 77.538 ng/ul
RT: 14.210 min Scan# 1908
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:152 Resp: 6797517
Ion Ratio Lower Upper
152 100
151 20.4 15.9 23.9
153 13.6 10.6 16.0



#51
3-Nitroaniline
Concen: 80.584 ng/ul
RT: 14.404 min Scan# 1941
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:138 Resp: 1096669
Ion Ratio Lower Upper
138 100
108 9.9 9.4 14.2
92 112.9 96.6 144.8



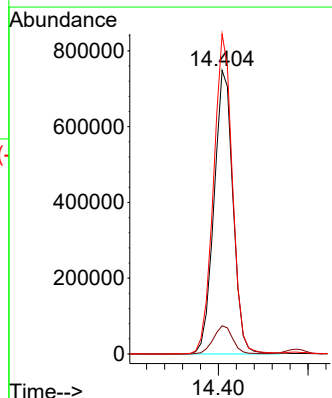
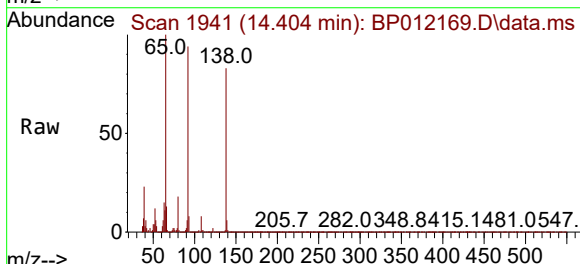




#52
Acenaphthene
Concen: 74.902 ng/ul
RT: 14.551 min Scan# 1966
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:153 Resp: 4674524
Ion Ratio Lower Upper
153 100
152 48.9 38.8 58.2
154 89.6 71.3 106.9



#53
2,4-Dinitrophenol
Concen: 93.080 ng/ul
RT: 14.616 min Scan# 1977
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:184 Resp: 702789
Ion Ratio Lower Upper
184 100
63 57.5 50.5 75.7
154 58.7 45.8 68.8




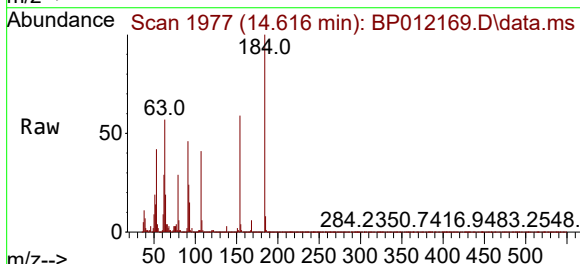




#55
4-Nitrophenol
Concen: 82.108 ng/ul
RT: 14.722 min Scan# 1995
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:109 Resp: 698256
Ion Ratio Lower Upper
109 100
139 147.4 126.6 189.8
65 133.2 117.1 175.7

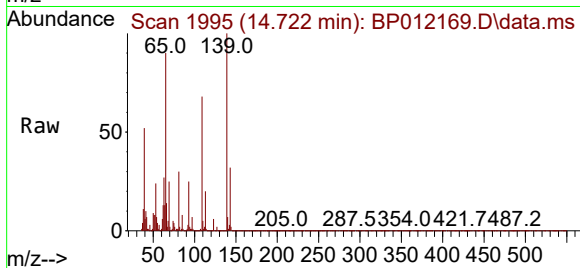

#56
Dibenzofuran
Concen: 73.384 ng/ul
RT: 14.886 min Scan# 2023
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:168 Resp: 6189602
Ion Ratio Lower Upper
168 100
139 38.0 28.6 42.8









#57
2,4-Dinitrotoluene
Concen: 90.183 ng/ul
RT: 14.863 min Scan# 2018
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:165 Resp: 1514793
Ion Ratio Lower Upper
165 100
63 41.4 35.5 53.3
182 2.6 1.9 2.9



#58
2,3,4,6-Tetrachlorophenol
Concen: 89.140 ng/ul
RT: 15.116 min Scan# 2062
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:232 Resp: 1375572
Ion Ratio Lower Upper
232 100
131 44.7 37.3 55.9
130 2.3 1.8 2.6
166 30.4 24.7 37.1



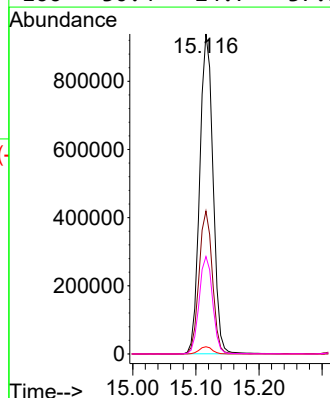
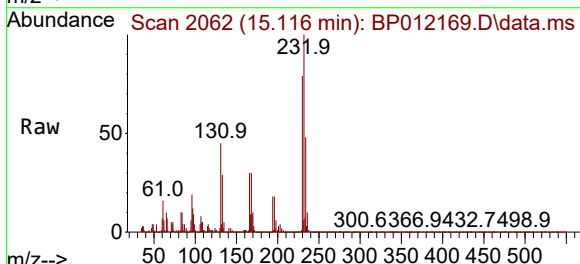




#59
Diethylphthalate
Concen: 82.750 ng/ul
RT: 15.322 min Scan# 2095
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:149 Resp: 5002738
Ion Ratio Lower Upper
149 100
177 22.6 17.7 26.5
150 12.5 10.0 15.0

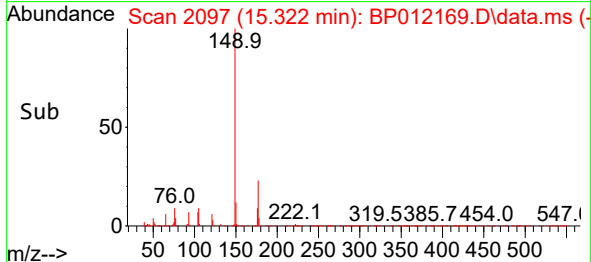

#61
Fluorene
Concen: 69.198 ng/ul
RT: 15.539 min Scan# 2134
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:166 Resp: 4581508
Ion Ratio Lower Upper
166 100
165 96.5 78.2 117.2
167 13.6 11.0 16.4


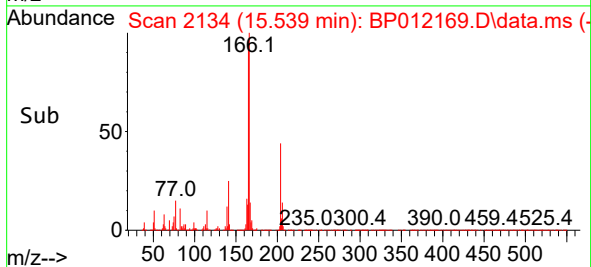

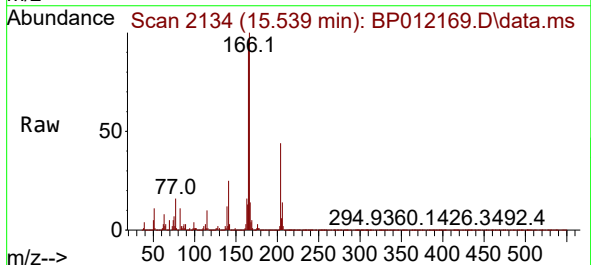




#62
4-Chlorophenyl-phenylether
Concen: 71.418 ng/ul
RT: 15.534 min Scan# 2133
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:204 Resp: 2287451
Ion Ratio Lower Upper
204 100
206 33.2 26.3 39.5
141 58.3 45.4 68.0



#63
4-Nitroaniline
Concen: 66.788 ng/ul
RT: 15.575 min Scan# 2140
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:138 Resp: 829942
Ion Ratio Lower Upper
138 100
92 51.8 42.1 63.1
108 71.1 58.0 87.0







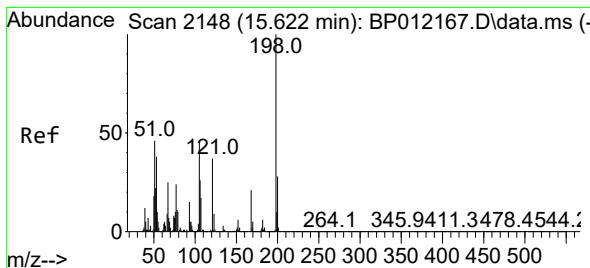

#66
4,6-Dinitro-2-methylphenol
Concen: 88.025 ng/ul
RT: 15.634 min Scan# 2148
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:198 Resp: 903890
Ion Ratio Lower Upper
198 100
182 3.8 5.0 7.4#
77 21.1 19.9 29.9

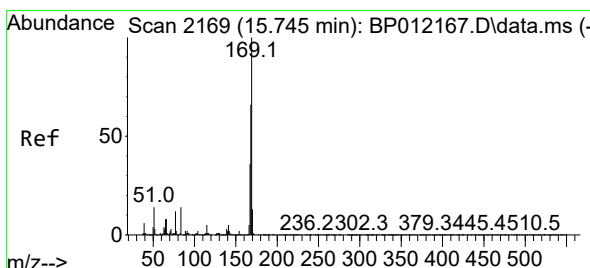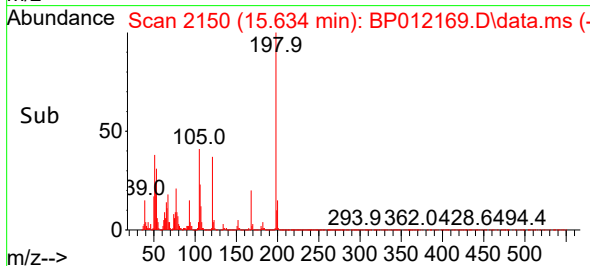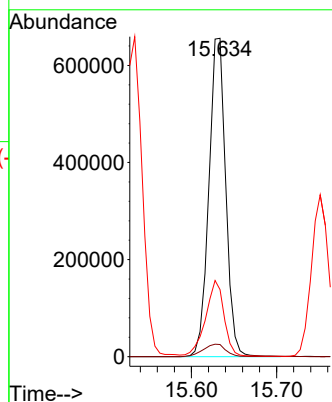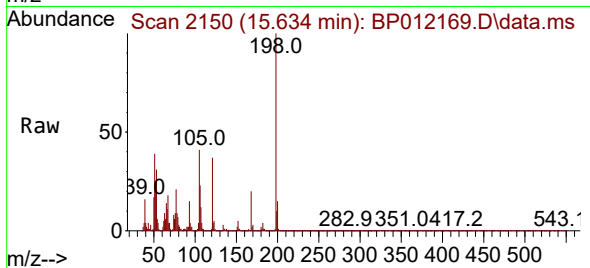

#67
N-Nitrosodiphenylamine
Concen: 77.482 ng/ul
RT: 15.751 min Scan# 2170
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:169 Resp: 4125464
Ion Ratio Lower Upper
169 100
168 65.7 52.7 79.1
167 36.5 29.0 43.4


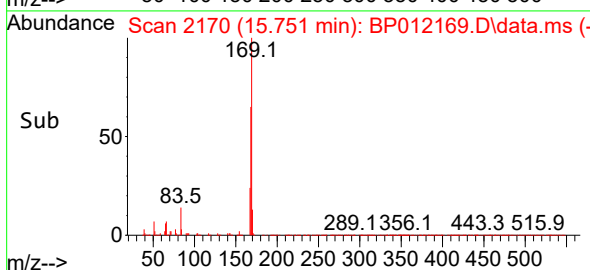

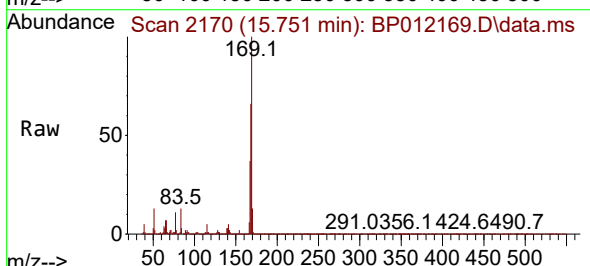




#68
4-Bromophenyl-phenylether
Concen: 89.035 ng/ul
RT: 16.433 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:248 Resp: 1558495
Ion Ratio Lower Upper
248 100
250 97.3 78.1 117.1
141 68.6 54.5 81.7



#69
Hexachlorobenzene
Concen: 88.500 ng/ul
RT: 16.545 min Scan# 2305
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:284 Resp: 1798051
Ion Ratio Lower Upper
284 100
142 33.3 29.6 44.4
249 31.0 24.8 37.2

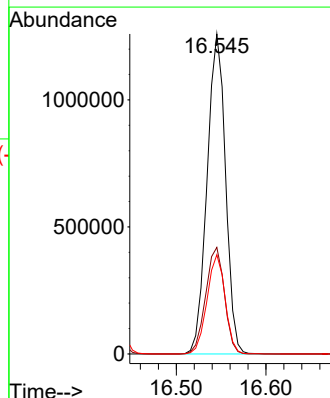



#70

Atrazine

Concen: 84.811 ng/ul

RT: 16.716 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:200 Resp: 1388612

Ion Ratio Lower Upper

200 100

173 26.3 21.0 31.4

215 48.4 39.0 58.6

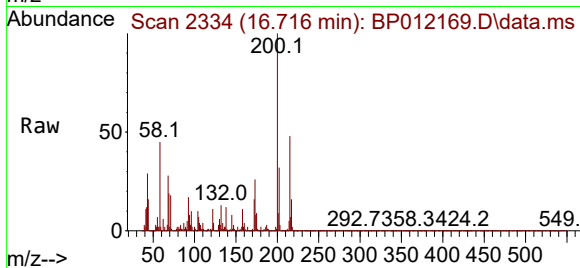

#71

Pentachlorophenol

Concen: 93.182 ng/ul

RT: 16.892 min Scan# 2364

Delta R.T. -0.000 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12




Tgt Ion:266 Resp: 1109182


Ion Ratio Lower Upper

266 100

264 63.3 48.7 73.1

268 64.1 50.6 75.8




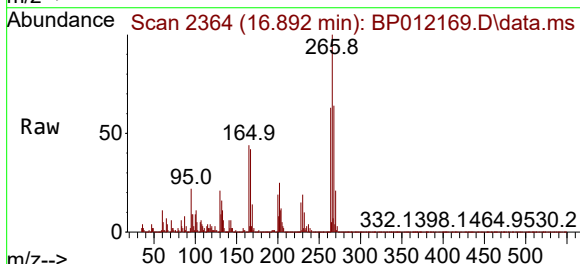




#72
Phenanthrene
Concen: 74.833 ng/ul
RT: 17.292 min Scan# 2431
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:178 Resp: 7320763
Ion Ratio Lower Upper
178 100
179 15.9 12.3 18.5
176 19.9 15.4 23.2

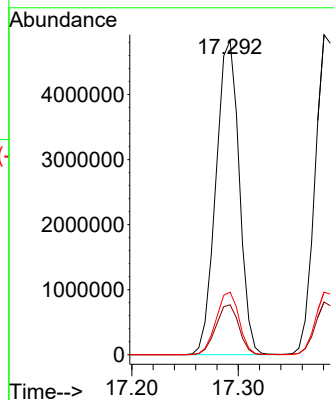

#74
Anthracene
Concen: 74.705 ng/ul
RT: 17.380 min Scan# 2447
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:178 Resp: 7232196
Ion Ratio Lower Upper
178 100
179 16.5 12.2 18.2
176 19.5 15.0 22.6



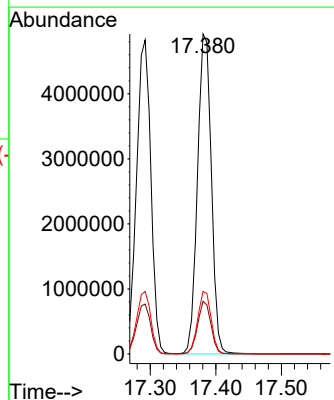





#75
1,2,3,4-Tetrachlorobenzene
Concen: 85.666 ng/uL
RT: 13.281 min Scan# 1750
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:216 Resp: 2490153
Ion Ratio Lower Upper
216 100
214 79.3 63.6 95.4
218 48.8 38.4 57.6



#76
Pentachlorobenzene
Concen: 84.278 ng/uL
RT: 14.804 min Scan# 2009
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:250 Resp: 2405950
Ion Ratio Lower Upper
250 100
248 62.8 49.0 73.4
252 63.7 49.8 74.6




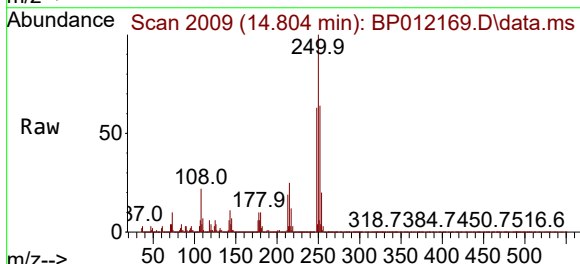




#77
Carbazole
Concen: 74.979 ng/ul
RT: 17.657 min Scan# 2494
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:167 Resp: 6473991
Ion Ratio Lower Upper
167 100
166 21.6 16.6 24.8
139 13.4 10.1 15.1



#78
Di-n-butylphthalate
Concen: 90.955 ng/ul
RT: 18.204 min Scan# 2587
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:149 Resp: 7793396
Ion Ratio Lower Upper
149 100
150 9.5 7.0 10.6
104 4.9 3.8 5.8

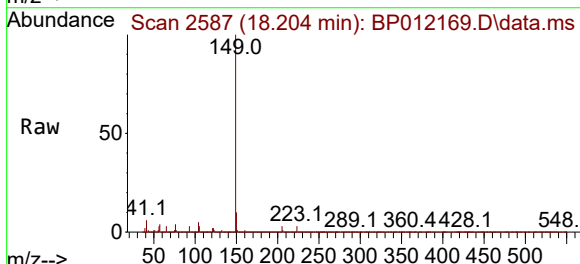



#80

Fluoranthene

Concen: 82.755 ng/ul

RT: 19.263 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:202 Resp: 7867728

Ion Ratio Lower Upper

202 100

101 11.9 10.1 15.1

100 8.9 7.5 11.3



#82

Pyrene

Concen: 78.867 ng/ul

RT: 19.616 min Scan# 2827

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12




Tgt Ion:202 Resp: 7935078


Ion Ratio Lower Upper

202 100

101 14.2 11.5 17.3

100 11.3 9.2 13.8









#83
Butylbenzylphthalate
Concen: 106.339 ng/ul
RT: 20.486 min Scan# 2975
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:149 Resp: 3391615
Ion Ratio Lower Upper
149 100
91 67.8 56.5 84.7
206 21.4 16.2 24.4



#84
3,3'-Dichlorobenzidine
Concen: 83.190 ng/ul
RT: 21.257 min Scan# 3106
Delta R.T. -0.000 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:252 Resp: 2776344
Ion Ratio Lower Upper
252 100
254 64.5 51.4 77.0
126 11.8 9.3 13.9





#85

Benzo(a)anthracene

Concen: 79.540 ng/ul

RT: 21.321 min Scan# 3117

Delta R.T. -0.000 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:228 Resp: 7582535

Ion Ratio Lower Upper

228 100

229 20.8 16.1 24.1

226 28.9 21.7 32.5

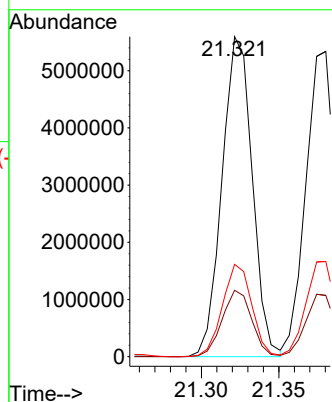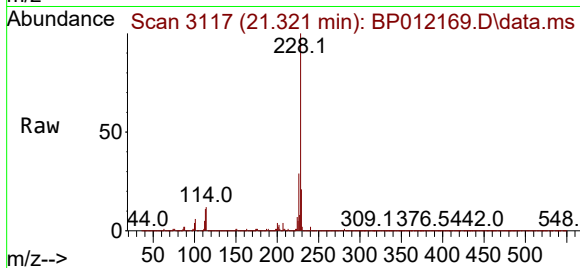

#86

Bis(2-ethylhexyl)phthalate

Concen: 107.962 ng/ul

RT: 21.245 min Scan# 3104

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12




Tgt Ion:149 Resp: 4641992


Ion Ratio Lower Upper

149 100

167 27.9 20.7 31.1

279 4.9 3.0 4.4#





#87

Chrysene

Concen: 77.784 ng/ul

RT: 21.380 min Scan# 3126

Delta R.T. 0.006 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:228 Resp: 7137628

Ion Ratio Lower Upper

228 100

226 31.2 23.8 35.8

229 20.1 15.9 23.9



#89

Di-n-octyl phthalate

Concen: 96.928 ng/ul




RT: 22.168 min Scan# 3261


Delta R.T. -0.000 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Tgt Ion:149 Resp: 8147840


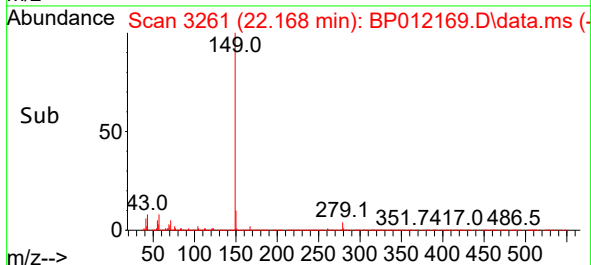

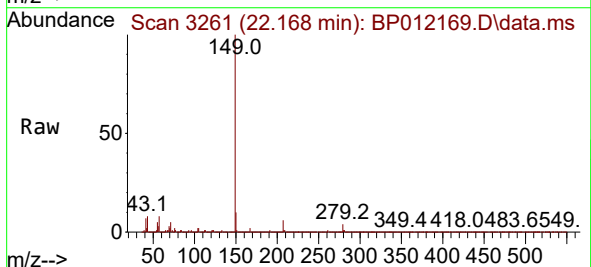




#90
Benzo(b)fluoranthene
Concen: 79.503 ng/ul
RT: 23.015 min Scan# 3404
Delta R.T. 0.006 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12




Instrument :
BNA_P
ClientSampleId :
SSTD080642


Tgt Ion:252 Resp: 8449633
Ion Ratio Lower Upper
252 100
253 22.6 17.5 26.3
125 10.7 8.6 13.0



#91
Benzo(k)fluoranthene
Concen: 78.364 ng/ul
RT: 23.068 min Scan# 3414
Delta R.T. 0.012 min
Lab File: BP012169.D
Acq: 17 Oct 2022 17:12

Tgt Ion:252 Resp: 8192185
Ion Ratio Lower Upper
252 100
253 22.4 17.4 26.2
125 10.3 8.8 13.2





#93

Benzo(a)pyrene

Concen: 79.552 ng/ul

RT: 23.651 min Scan# 3

Delta R.T. 0.012 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:252 Resp: 7543102

Ion Ratio Lower Upper

252 100

253 22.2 17.4 26.0

125 11.4 9.6 14.4



#94

Indeno(1,2,3-cd)pyrene

Concen: 82.242 ng/ul

RT: 26.274 min Scan# 3959

Delta R.T. 0.018 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12




Tgt Ion:276 Resp: 9860194


Ion Ratio Lower Upper

276 100

138 26.1 20.7 31.1

277 25.9 19.7 29.5





#95

Dibenzo(a,h)anthracene

Concen: 81.087 ng/ul

RT: 26.292 min Scan# 3958

Delta R.T. 0.023 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Instrument :

BNA_P

ClientSampleId :

SSTD080642





Tgt Ion:278 Resp: 8721522

Ion Ratio Lower Upper

278 100

139 16.5 13.5 20.3

279 24.4 19.2 28.8



#96

Benzo(g,h,i)perylene

Concen: 82.538 ng/ul

RT: 27.045 min Scan# 4090

Delta R.T. 0.023 min

Lab File: BP012169.D

Acq: 17 Oct 2022 17:12

Tgt Ion:276 Resp: 8922136

Ion Ratio Lower Upper

276 100

138 22.5 18.7 28.1

277 24.4 19.1 28.7

