


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007502.D
Acq On : 19 Oct 2021 21:02
Operator : CG/JU
Sample : M4196-16
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD2

Manual Integrations
APPROVED

mohammad
10/20/2021 1:56:51 PM

Quant Time: Oct 20 01:05:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 18 11:26:58 2021
Response via : Initial Calibration

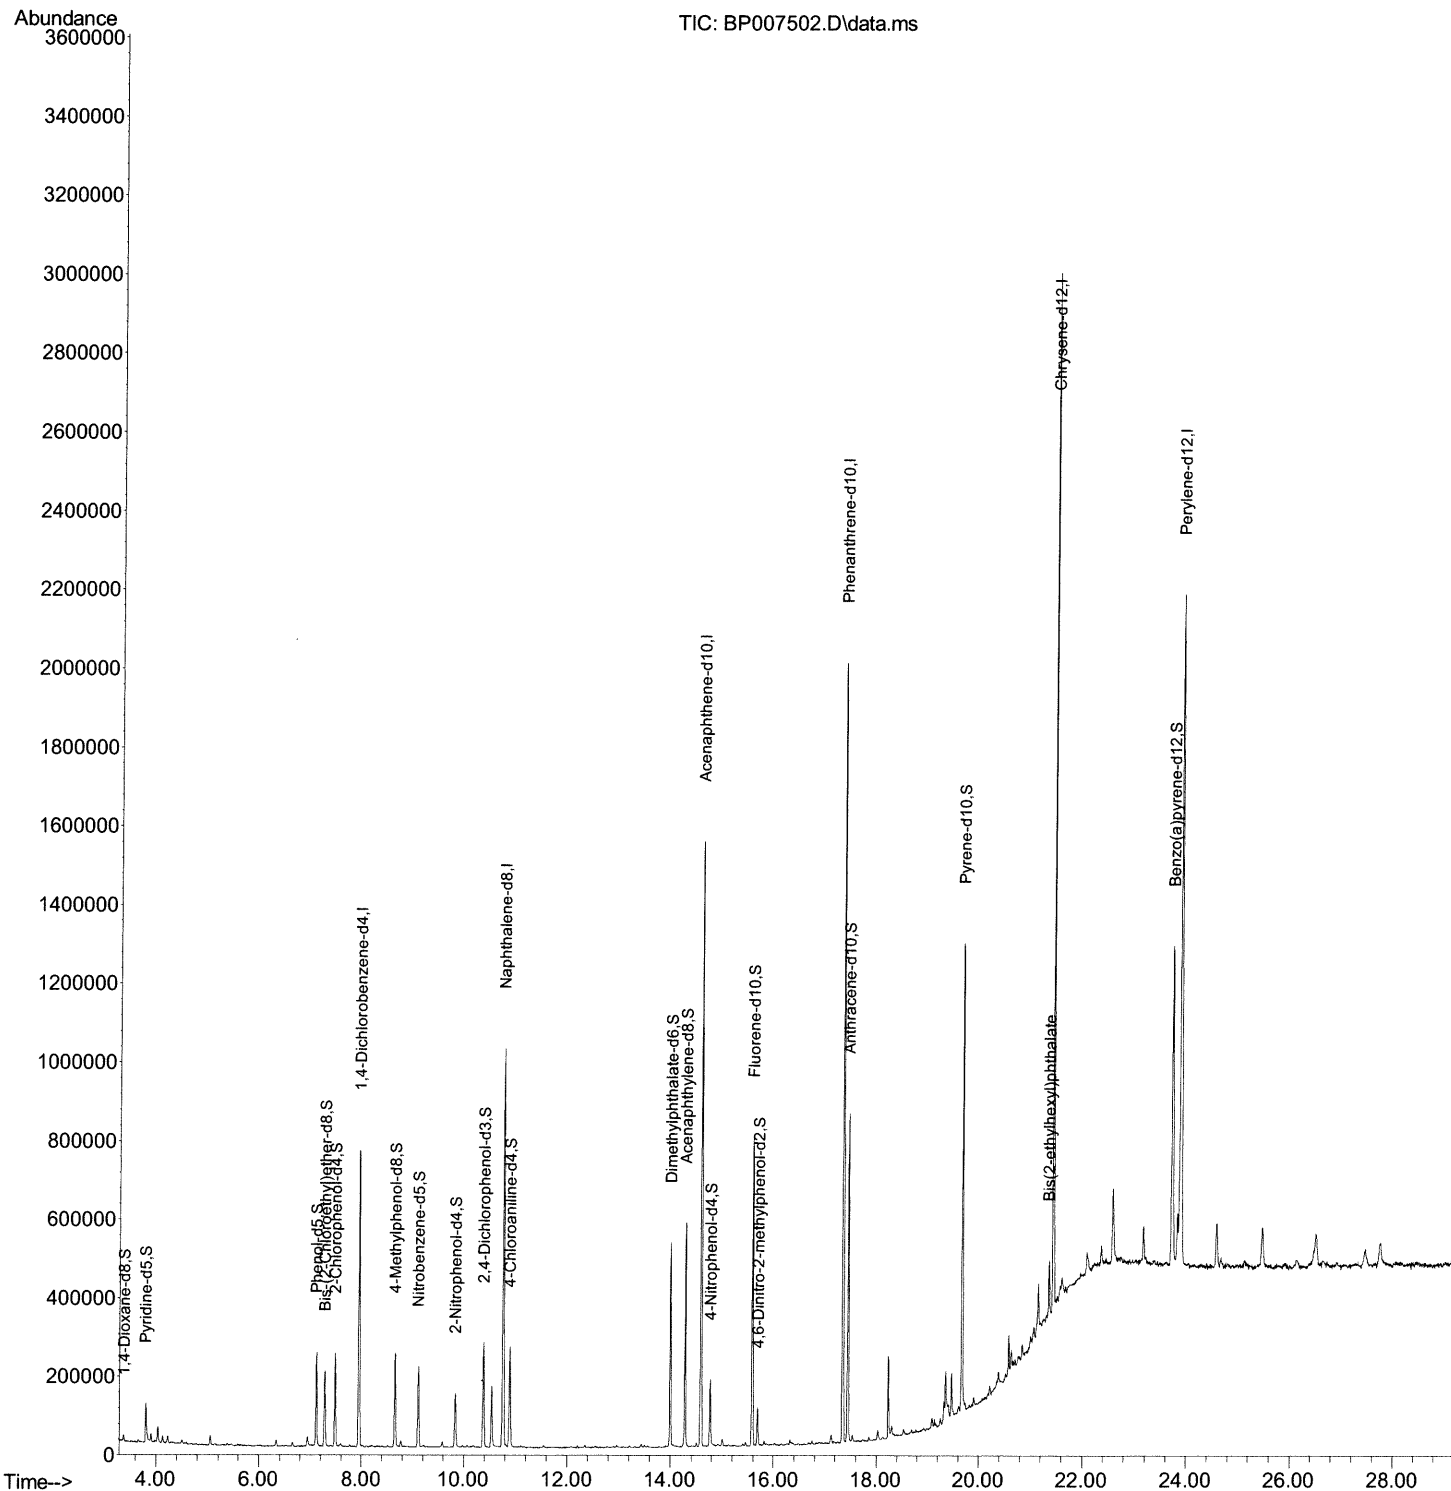

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007502.D
Acq On : 19 Oct 2021 21:02
Operator : CG/JU
Sample : M4196-16
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD2

Manual Integrations
APPROVED

mohammad
10/20/2021 1:56:51 PM

Quant Time: Oct 20 01:05:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 18 11:26:58 2021
Response via : Initial Calibration

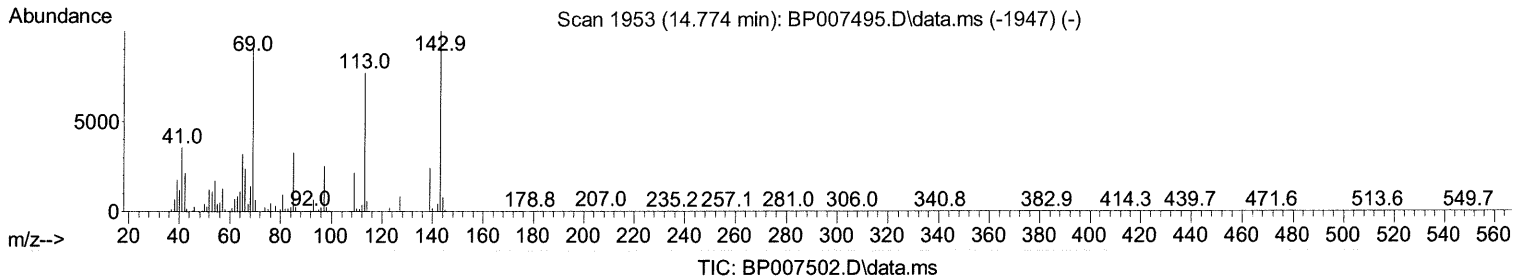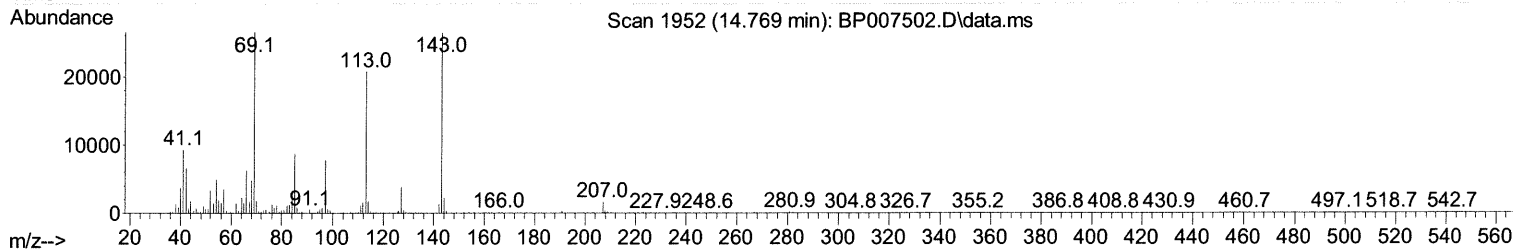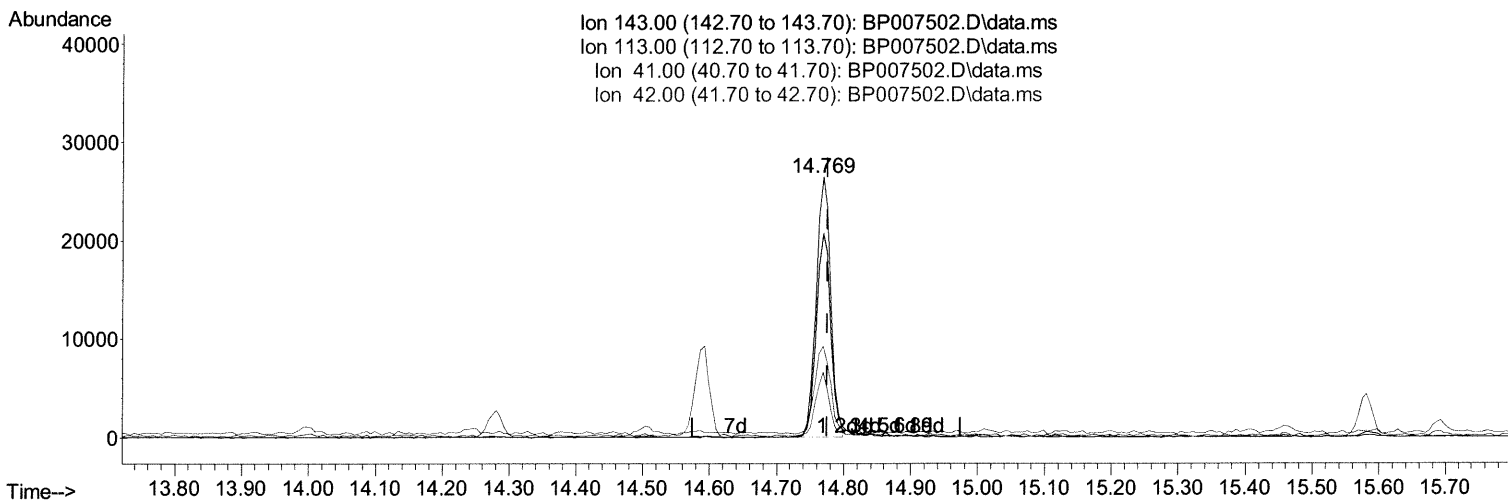

(54) 4-Nitrophenol-d4 (S)

14.769min (-0.006) 6.49 ng/ul

response 39784

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.90	78.43
41.00	39.60	35.13
42.00	25.40	25.17

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007502.D
Acq On : 19 Oct 2021 21:02
Operator : CG/JU
Sample : M4196-16
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD2

Manual Integrations
APPROVED

mohammad
10/20/2021 1:56:51 PM

Quant Time: Oct 20 01:05:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 18 11:26:58 2021
Response via : Initial Calibration

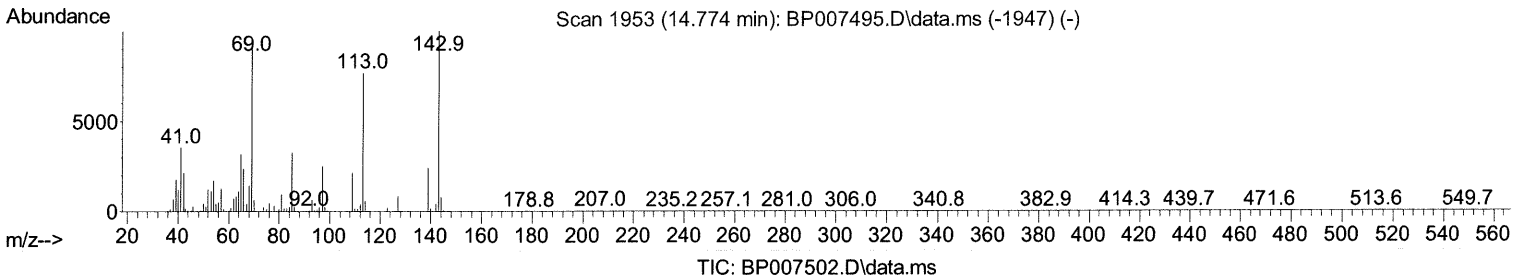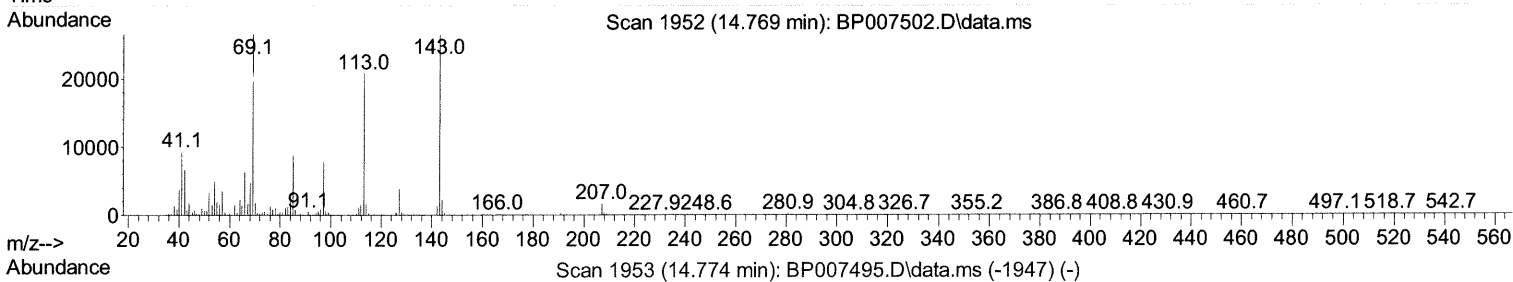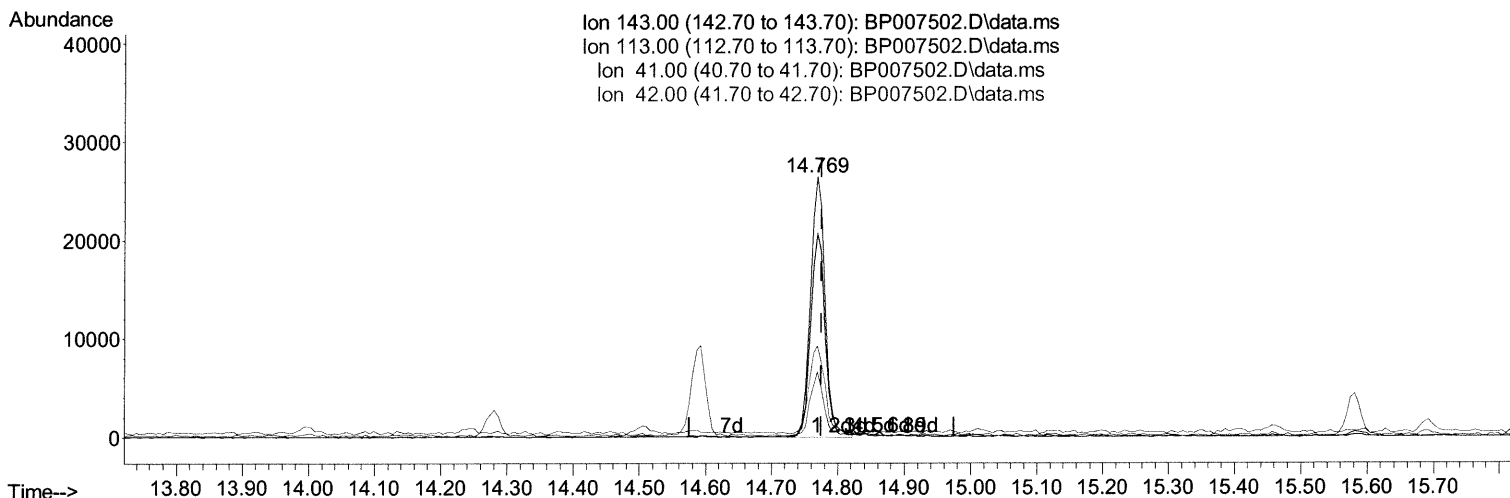

TIC: BP007502.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (-0.006) 6.60 ng/ul m 10/21/21 JU

response 40418

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.90	78.43
41.00	39.60	35.13
42.00	25.40	25.17

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007502.D
 Acq On : 19 Oct 2021 21:02
 Operator : CG/JU
 Sample : M4196-16
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD2

Manual Integrations
 APPROVED

mohammad
 10/20/2021 1:56:51 PM

Quant Time: Oct 20 01:05:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 18 11:26:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	210107	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	839938	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.592	164	551796	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1196817	20.000	ng/ul	-0.01
79) Chrysene-d12	21.427	240	1282462	20.000	ng/ul	-0.01
88) Perylene-d12	23.874	264	1308622	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	7527	1.415	ng/uL	0.00
4) Pyridine-d5	3.799	84	52607	3.613	ng/ul	0.00
7) Phenol-d5	7.110	99	135928	8.284	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	82289	8.408	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	109073	8.450	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	88960	7.039	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	48431	9.111	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	45650	9.194	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	98782	8.157	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	137795	8.414	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	339675	8.898	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	396101	8.256	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	40418m >	6.598	ng/ul >	0.00 10/20/2021
60) Fluorene-d10	15.580	176	302434	9.467	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.692	200	21392	4.461	ng/ul	-0.01
73) Anthracene-d10	17.439	188	476813	9.381	ng/ul	-0.01
81) Pyrene-d10	19.668	212	641518	10.006	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.715	264	606358	9.312	ng/ul	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.345	149	48309	1.073	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed