


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007538.D
Acq On : 20 Oct 2021 20:24
Operator : CG/JU
Sample : M4246-11
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT49

Manual Integrations
APPROVED

mohammad
10/21/2021 11:15:59 AM

Quant Time: Oct 21 01:02:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

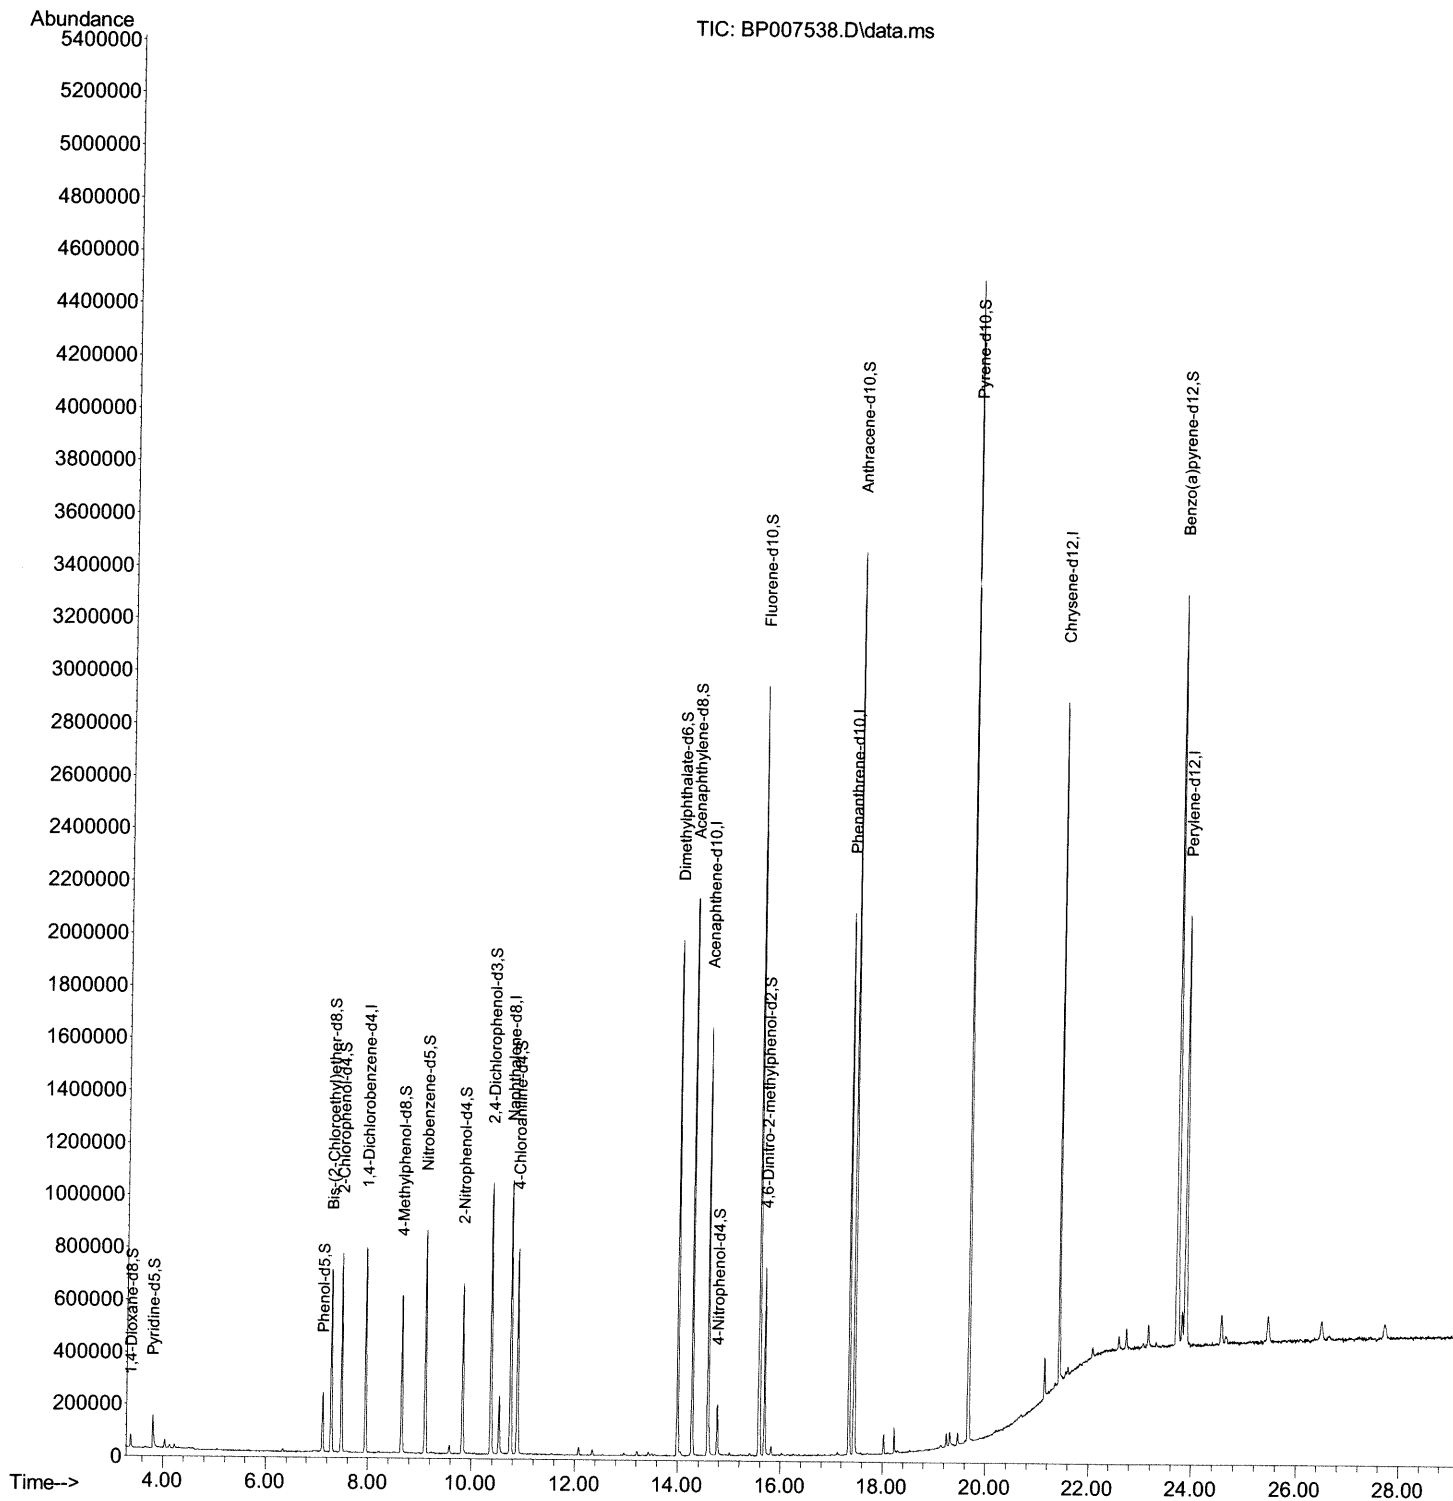

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007538.D
Acq On : 20 Oct 2021 20:24
Operator : CG/JU
Sample : M4246-11
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT49

Manual Integrations
APPROVED

mohammad
10/21/2021 11:15:59 AM

Quant Time: Oct 21 01:02:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

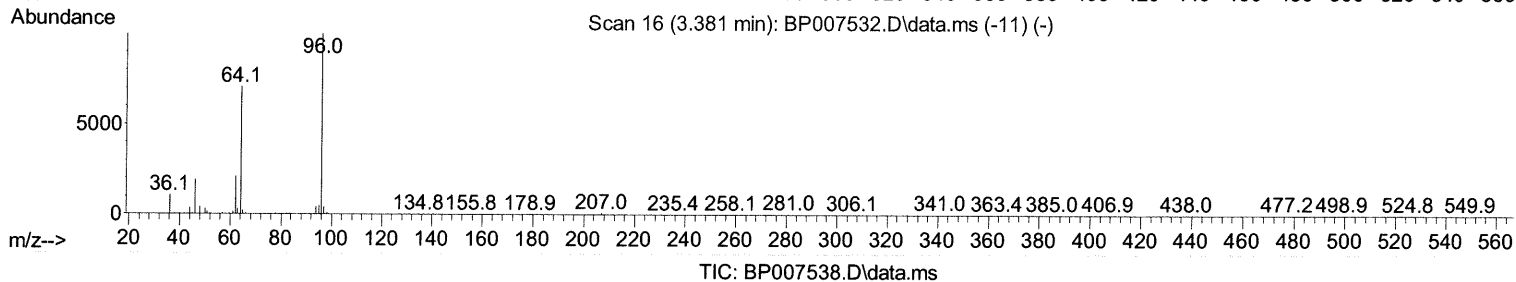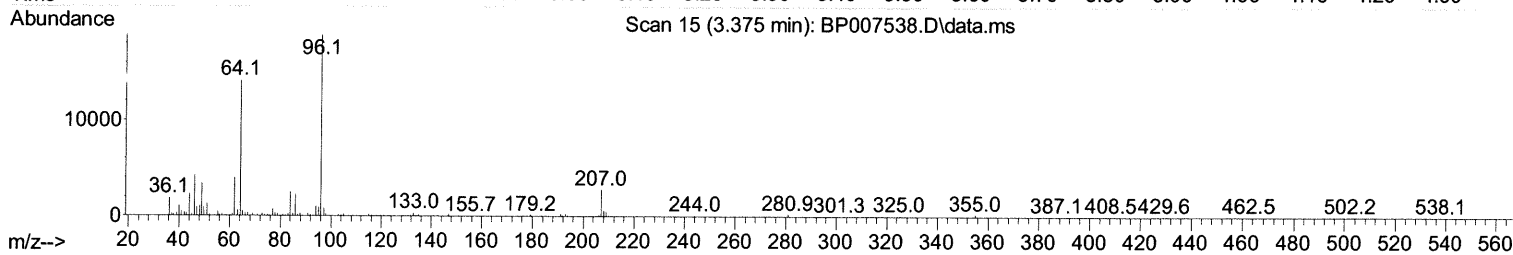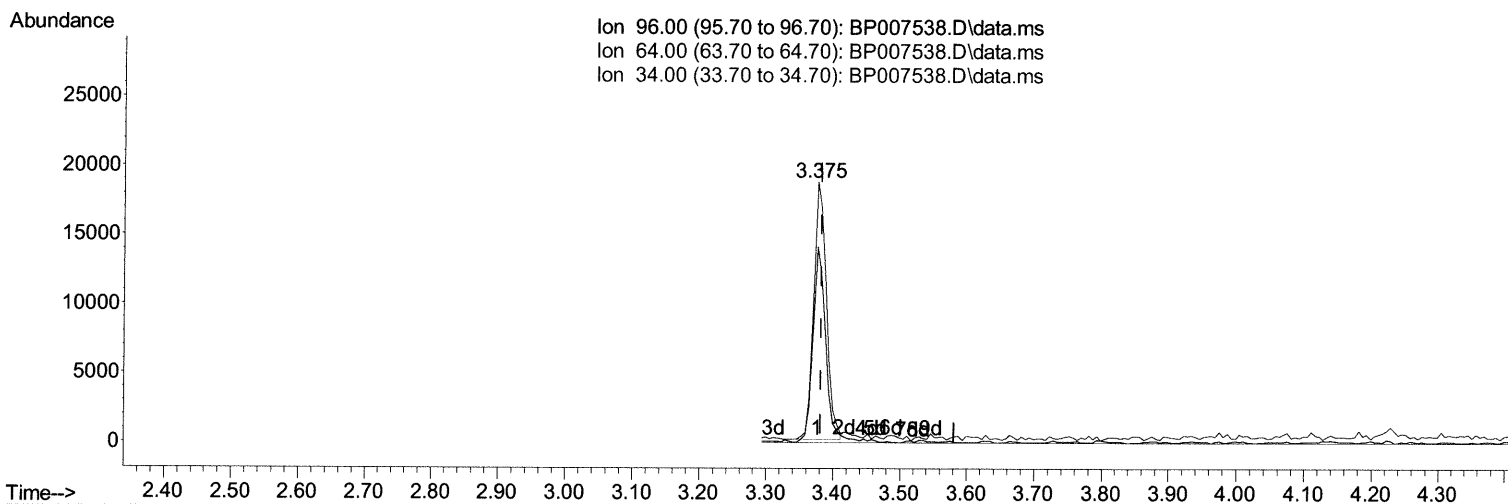

(3) 1,4-Dioxane-d8 (S)

3.375min (-0.006) 4.59 ng/uL

response 24996

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	75.07
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007538.D
 Acq On : 20 Oct 2021 20:24
 Operator : CG/JU
 Sample : M4246-11
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YAT49

Manual Integrations
 APPROVED

mohammad
 10/21/2021 11:15:59 AM

Quant Time: Oct 21 01:02:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

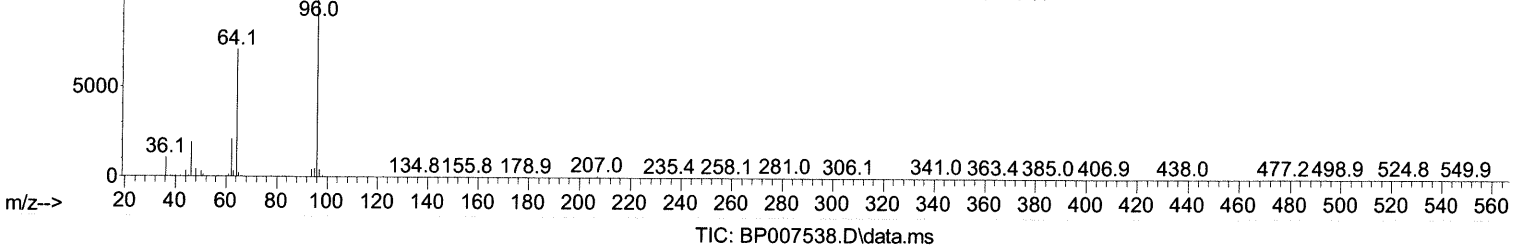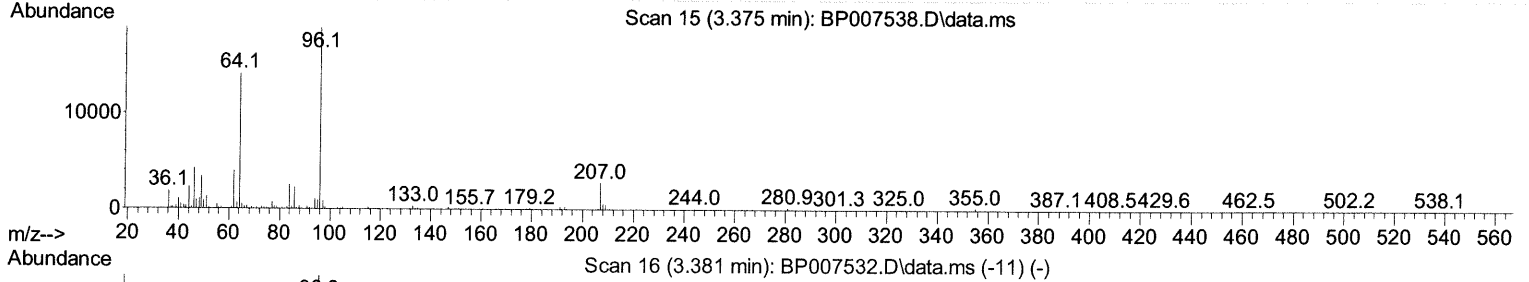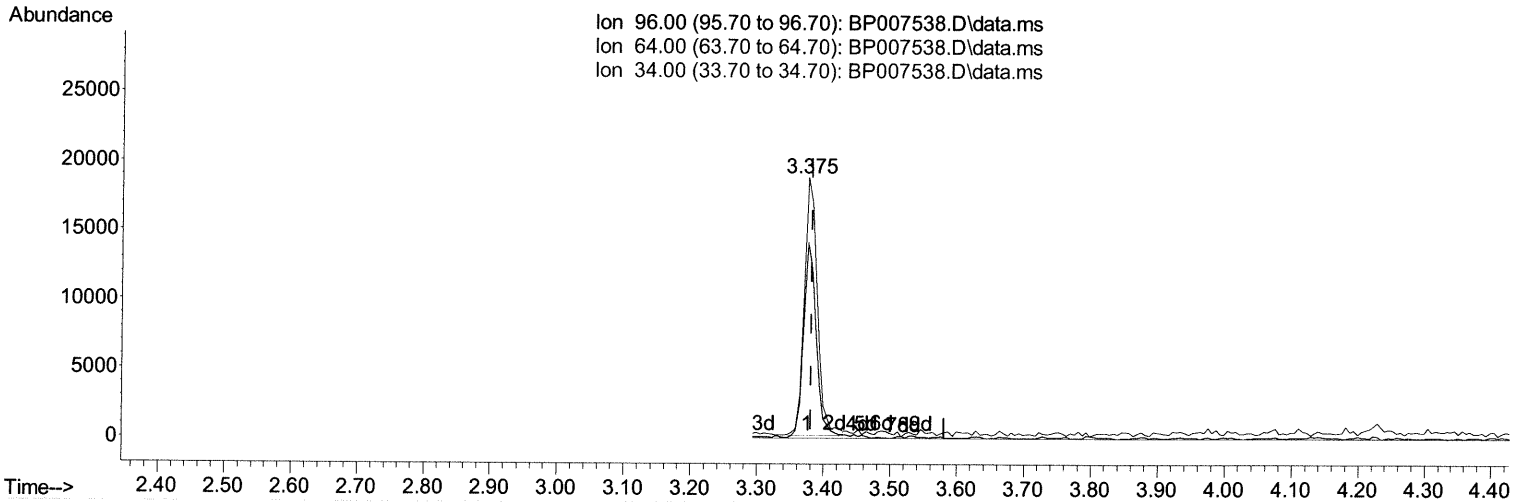

(3) 1,4-Dioxane-d8 (S)

3.375min (-0.006) 4.71 ng/uL m 10/22/21 JU

response 25646

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	75.07
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007538.D
 Acq On : 20 Oct 2021 20:24
 Operator : CG/JU
 Sample : M4246-11
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YAT49

Manual Integrations
 APPROVED

mohammad
 10/21/2021 11:15:59 AM

Quant Time: Oct 21 01:02:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.952	152	215122	20.000 ng/ul	0.00
20) Naphthalene-d8	10.757	136	872910	20.000 ng/ul	0.00
38) Acenaphthene-d10	14.587	164	562567	20.000 ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1205765	20.000 ng/ul	0.00
79) Chrysene-d12	21.421	240	1260256	20.000 ng/ul	0.00
88) Perylene-d12	23.868	264	1298473	20.000 ng/ul	0.00

System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.375	96	25646m	4.709 ng/ul	0.00 10/22/21
4) Pyridine-d5	3.799	84	75153	5.041 ng/ul	0.00
7) Phenol-d5	7.110	99	126878	7.552 ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	311004	31.038 ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	342640	25.926 ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	231876	17.919 ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	206925	37.458 ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	207614	40.236 ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	382612	30.401 ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	412771	24.253 ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	1320718	33.934 ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1565564	32.007 ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	46395	7.429 ng/ul	0.00
60) Fluorene-d10	15.581	176	1138095	34.942 ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	158469	32.800 ng/ul	0.00
73) Anthracene-d10	17.439	188	1957375	38.225 ng/ul	0.00
81) Pyrene-d10	19.669	212	2313876	36.727 ng/ul	0.00
92) Benzo(a)pyrene-d12	23.715	264	2282731	35.331 ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed