


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007542.D
Acq On : 20 Oct 2021 23:47
Operator : CG/JU
Sample : M4182-03
Misc :
ALS Vial : 99 Sample Multiplier: 1


Quant Time: Oct 21 01:05:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

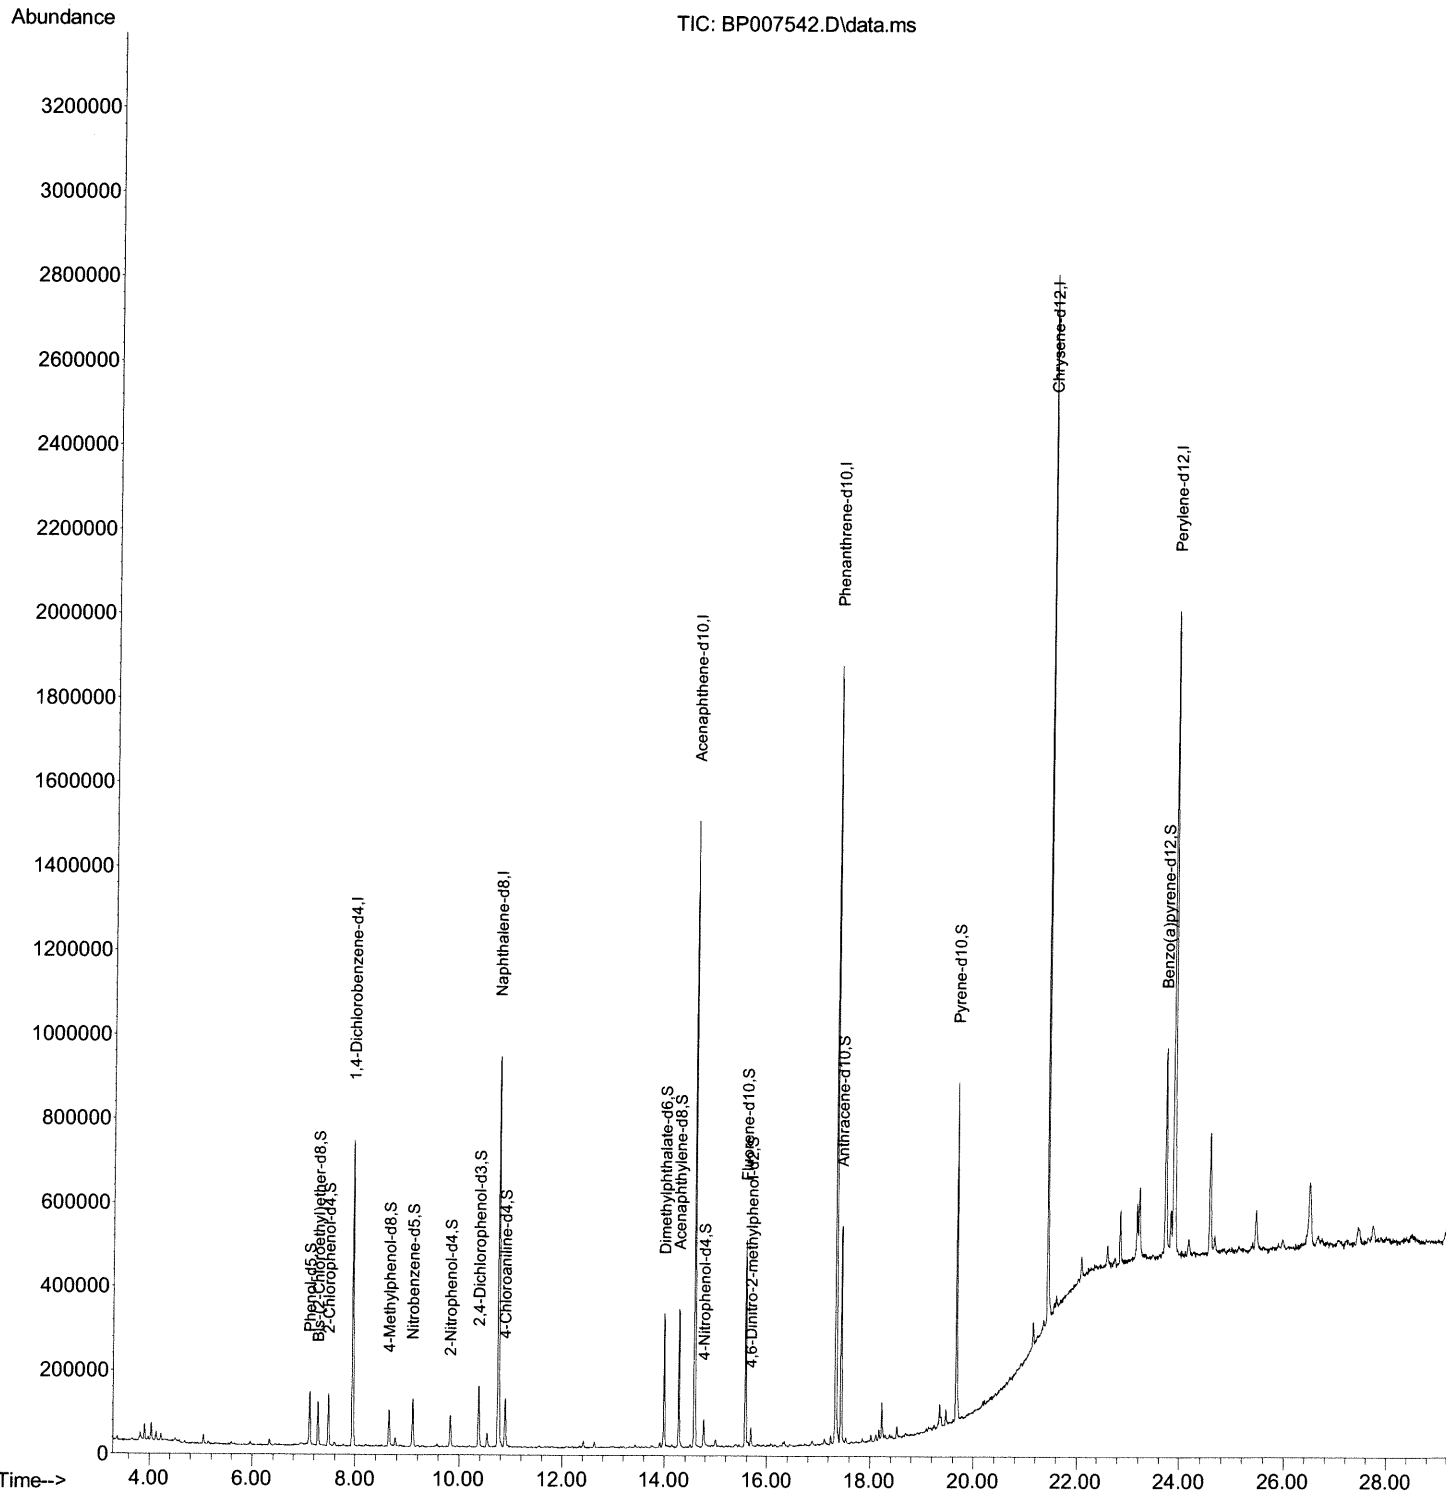

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007542.D
 Acq On : 20 Oct 2021 23:47
 Operator : CG/JU
 Sample : M4182-03
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Quant Time: Oct 21 01:05:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

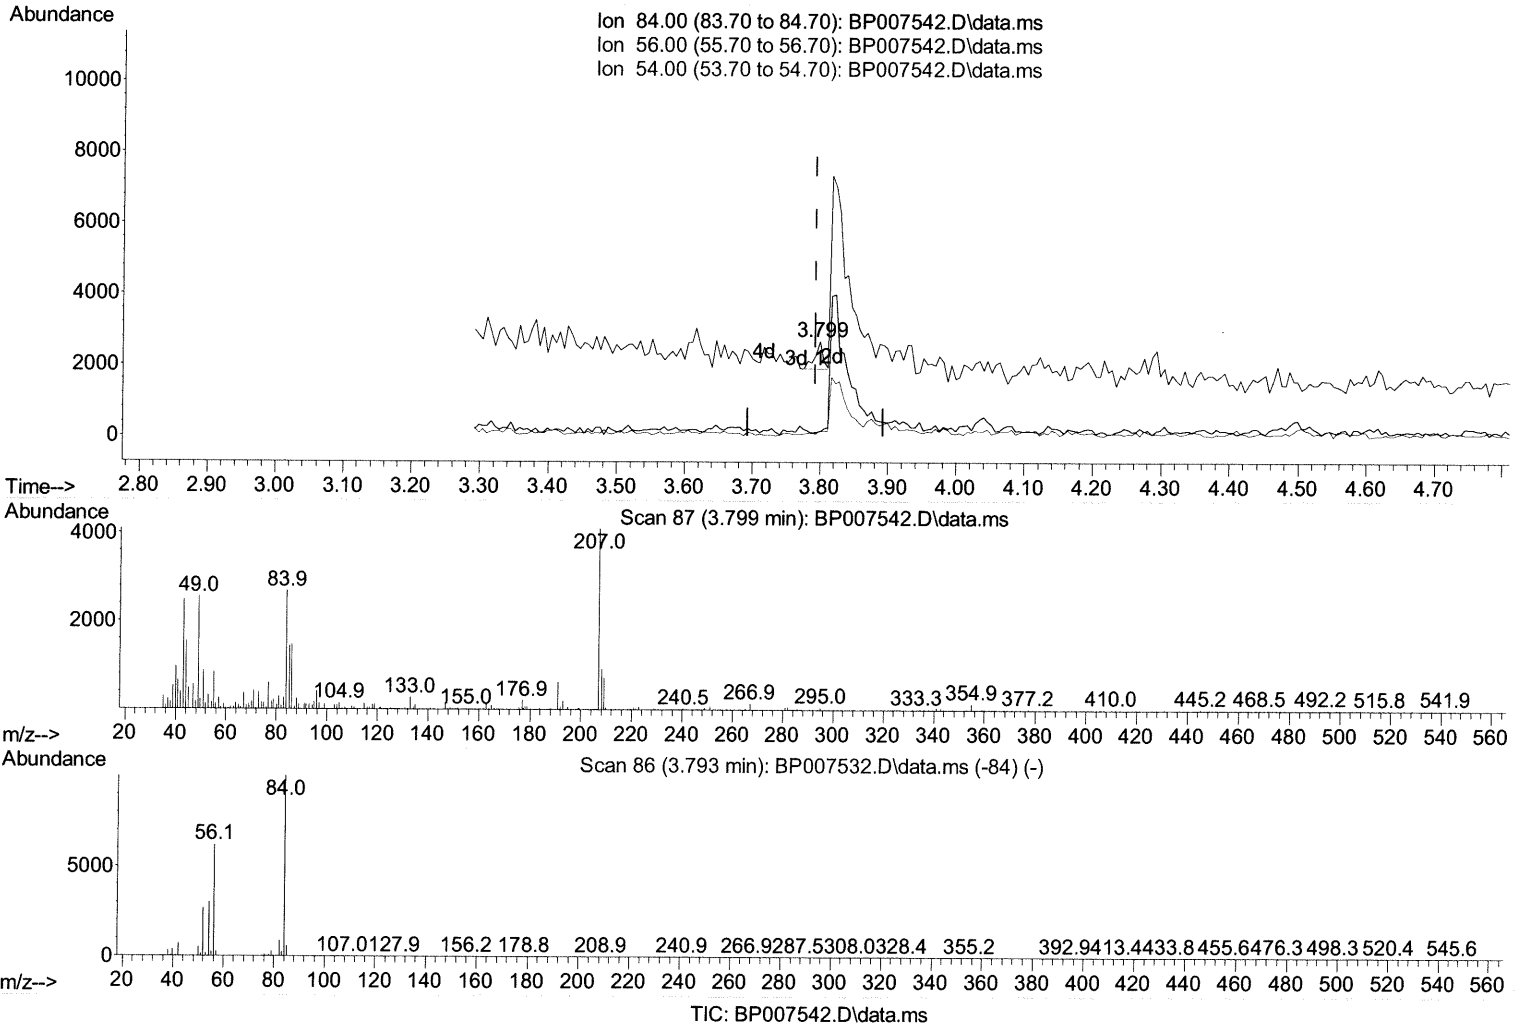

(4) Pyridine-d5 (S)

3.799min (+ 0.006) 0.05 ng/ul




response 662

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	4.71#
54.00	31.70	5.72#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007542.D
 Acq On : 20 Oct 2021 23:47
 Operator : CG/JU
 Sample : M4182-03
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Quant Time: Oct 21 01:05:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

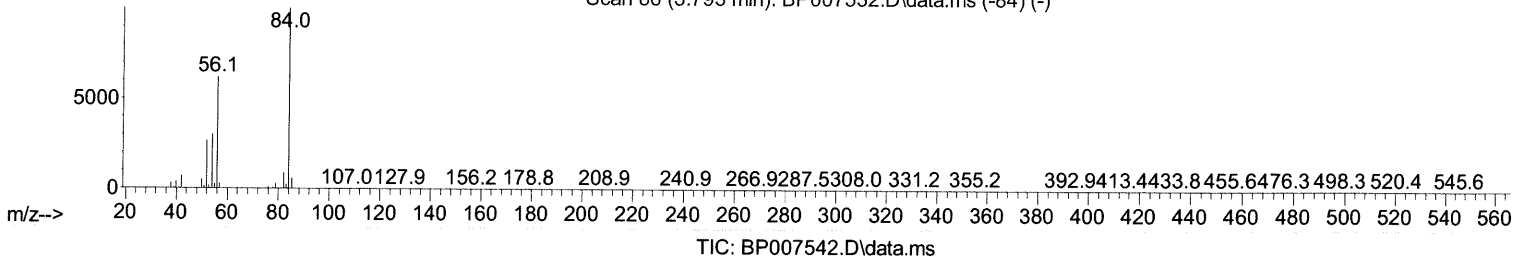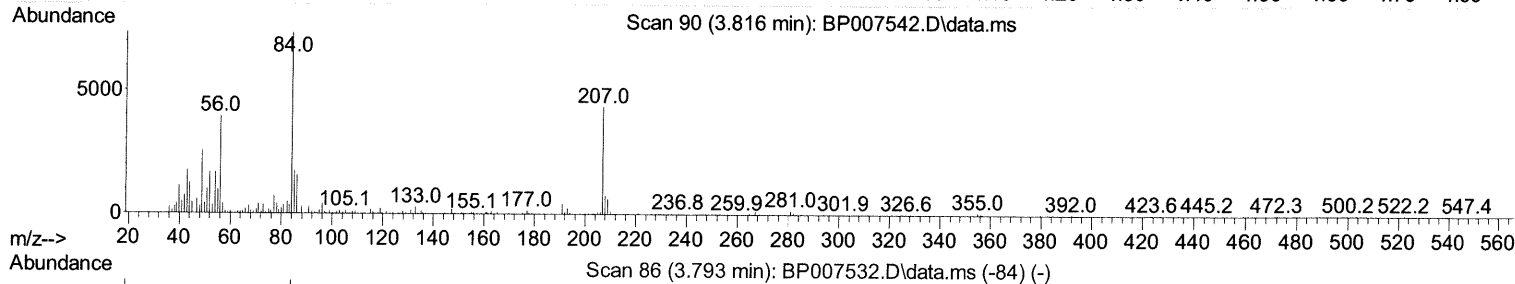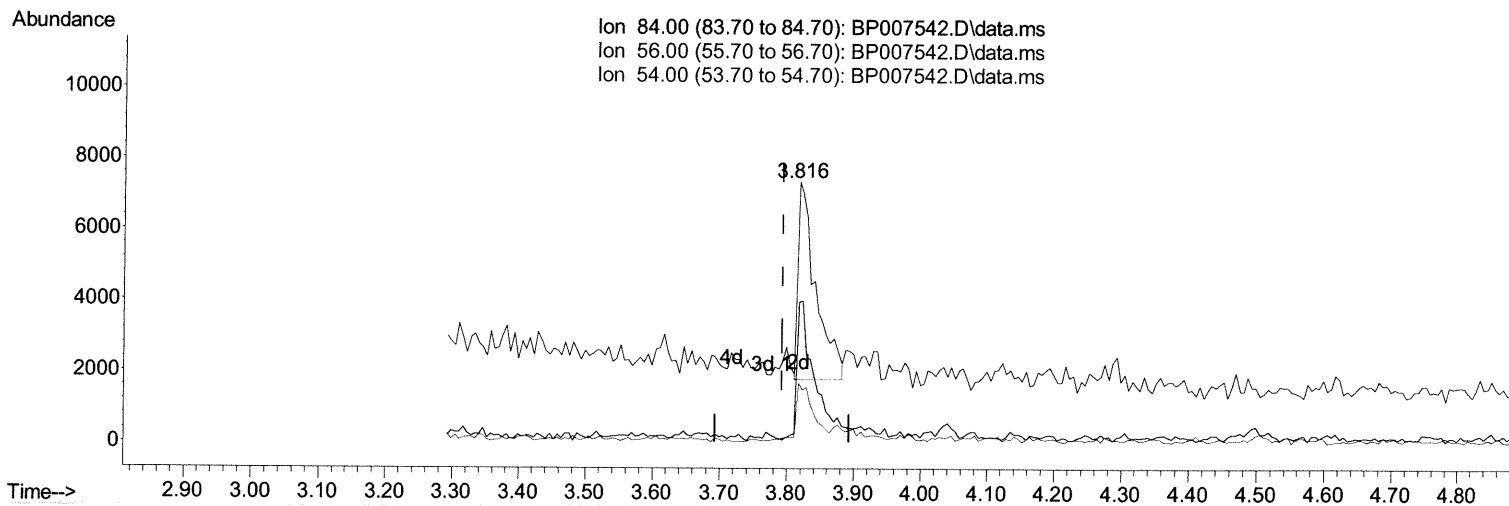

(4) Pyridine-d5 (S)

3.816min (+ 0.024) 0.75 ng/ul m 10/20/21 JU

response 10210

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	53.88
54.00	31.70	22.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP101821\

Data File : BP007542.D

Acq On : 20 Oct 2021 23:47

Operator : CG/JU

Sample : M4182-03

Misc :

ALS Vial : 99 Sample Multiplier: 1

Quant Time: Oct 21 01:05:28 2021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Oct 20 10:49:33 2021

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	196793	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	797923	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	508190	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1109649	20.000	ng/ul	0.00
79) Chrysene-d12	21.421	240	1157668	20.000	ng/ul	0.00
88) Perylene-d12	23.868	264	1177959	20.000	ng/ul	0.00

System Monitoring Compounds

3)	1,4-Dioxane-d8	3.381	96	4537	0.911 ng/uL	0.00
4)	Pyridine-d5	3.816	84	10210m	0.749 ng/uL	0.02
7)	Phenol-d5	7.110	99	71085	4.625 ng/uL	0.00
9)	Bis-(2-Chloroethyl)eth...	7.275	67	45914	5.009 ng/uL	0.00
11)	2-Chlorophenol-d4	7.481	132	57762	4.778 ng/uL	0.00
15)	4-Methylphenol-d8	8.657	113	32980	2.786 ng/uL	0.00
21)	Nitrobenzene-d5	9.104	128	25989	5.147 ng/uL	0.00
24)	2-Nitrophenol-d4	9.834	143	24567	5.209 ng/uL	0.00
28)	2,4-Dichlorophenol-d3	10.375	165	55480	4.822 ng/uL	0.00
31)	4-Chloroaniline-d4	10.887	131	60689	3.901 ng/uL	0.00
46)	Dimethylphthalate-d6	13.992	166	213129	6.062 ng/uL	0.00
49)	Acenaphthylene-d8	14.275	160	240215	5.437 ng/uL	0.00
54)	4-Nitrophenol-d4	14.769	143	16392	2.906 ng/uL	0.00
60)	Fluorene-d10	15.581	176	193282	6.569 ng/uL	0.00
65)	4,6-Dinitro-2-methylph...	15.686	200	10505	2.363 ng/uL	0.00
73)	Anthracene-d10	17.439	188	305425	6.481 ng/uL	0.00
81)	Pyrene-d10	19.669	212	398147	6.880 ng/uL	0.00
92)	Benzo(a)pyrene-d12	23.710	264	369424	6.303 ng/uL	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed