

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007492.D
 Acq On : 19 Oct 2021 14:13
 Operator : CG/JU
 Sample : M4196-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGA5

Quant Time: Oct 19 14:44:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 18 11:26:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	198036	20.00	ng/ul	0.00
20) Naphthalene-d8	10.758	136	782984	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	495111	20.00	ng/ul	-0.01
64) Phenanthrene-d10	17.345	188	1076836	20.00	ng/ul	0.00
79) Chrysene-d12	21.428	240	1145981	20.00	ng/ul	-0.01
88) Perylene-d12	23.880	264	1171731	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	25553	5.10	ng/uL	0.00
4) Pyridine-d5	3.793	84	344569	25.10	ng/ul	0.00
7) Phenol-d5	7.111	99	579031	37.44	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	311137	33.73	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	437439	35.95	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	461096	38.71	ng/ul	0.00
21) Nitrobenzene-d5	9.111	128	206486	41.67	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	211127	45.62	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	440810	39.05	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	560439	36.71	ng/ul	0.00
46) Dimethylphthalate-d6	13.999	166	1263486	36.89	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	1604610	37.27	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	210857	38.36	ng/ul	0.00
60) Fluorene-d10	15.581	176	1107013	38.62	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.693	200	123476	28.62	ng/ul	-0.01
73) Anthracene-d10	17.445	188	1768616	38.67	ng/ul	0.00
81) Pyrene-d10	19.675	212	2079615	36.30	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.722	264	2119121	36.35	ng/ul	-0.01
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.351	149	161958	4.03	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007492.D
Acq On : 19 Oct 2021 14:13
Operator : CG/JU
Sample : M4196-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGA5

Quant Time: Oct 19 14:44:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 18 11:26:58 2021
Response via : Initial Calibration

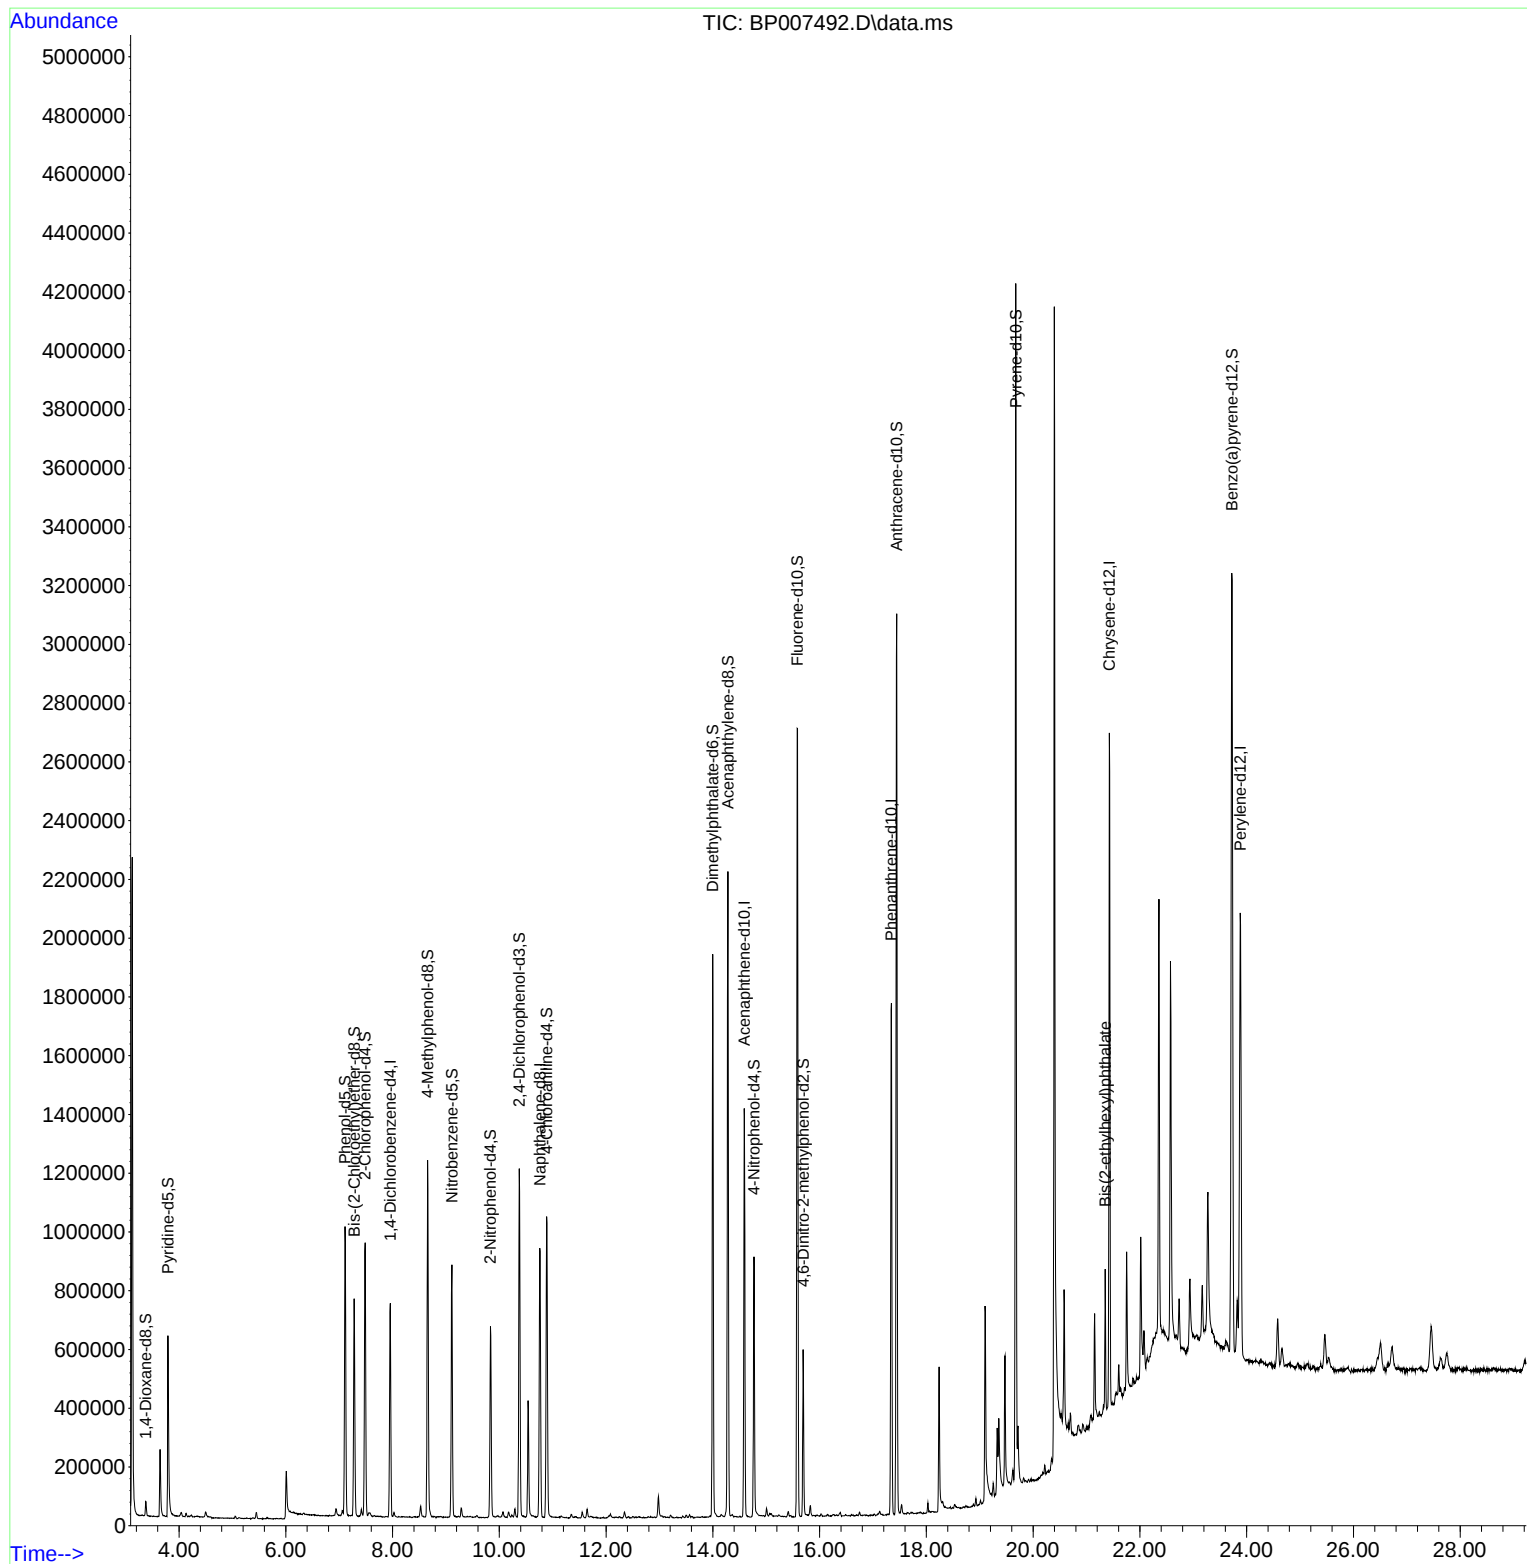

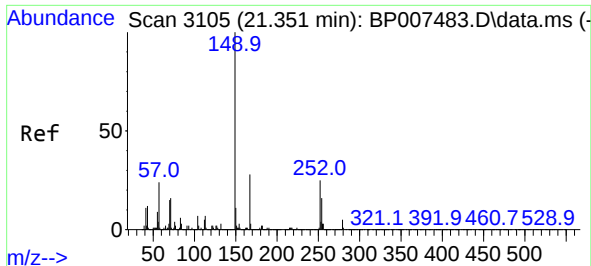

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.03 ng/ul
 RT: 21.351 min Scan# 3105
 Delta R.T. -0.006 min
 Lab File: BP007492.D
 Acq: 19 Oct 2021 14:13

Instrument :
 BNA_P
 ClientSampleId :
 JDGA5

Tgt Ion:149 Resp: 161958
 Ion Ratio Lower Upper
 149 100
 167 30.2 22.6 33.8
 279 4.3 3.3 4.9

