

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007502.D
 Acq On : 19 Oct 2021 21:02
 Operator : CG/JU
 Sample : M4196-16
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD2

Manual Integrations
 APPROVED

mohammad
 10/20/2021 1:56:51 PM

Quant Time: Oct 20 01:05:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 18 11:26:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	210107	20.00	ng/ul	0.00
20) Naphthalene-d8	10.757	136	839938	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.592	164	551796	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1196817	20.00	ng/ul	-0.01
79) Chrysene-d12	21.427	240	1282462	20.00	ng/ul	-0.01
88) Perylene-d12	23.874	264	1308622	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	7527	1.41	ng/uL	0.00
4) Pyridine-d5	3.799	84	52607	3.61	ng/ul	0.00
7) Phenol-d5	7.110	99	135928	8.28	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	82289	8.41	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	109073	8.45	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	88960	7.04	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	48431	9.11	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	45650	9.19	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	98782	8.16	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	137795	8.41	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	339675	8.90	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	396101	8.26	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	40418m	6.60	ng/ul	0.00
60) Fluorene-d10	15.580	176	302434	9.47	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.692	200	21392	4.46	ng/ul	-0.01
73) Anthracene-d10	17.439	188	476813	9.38	ng/ul	-0.01
81) Pyrene-d10	19.668	212	641518	10.01	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.715	264	606358	9.31	ng/ul	-0.02
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.345	149	48309	1.07	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007502.D
Acq On : 19 Oct 2021 21:02
Operator : CG/JU
Sample : M4196-16
Misc :
ALS Vial : 53 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
JDGD2

Manual Integrations
APPROVED

mohammad
10/20/2021 1:56:51 PM

Quant Time: Oct 20 01:05:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 18 11:26:58 2021
Response via : Initial Calibration

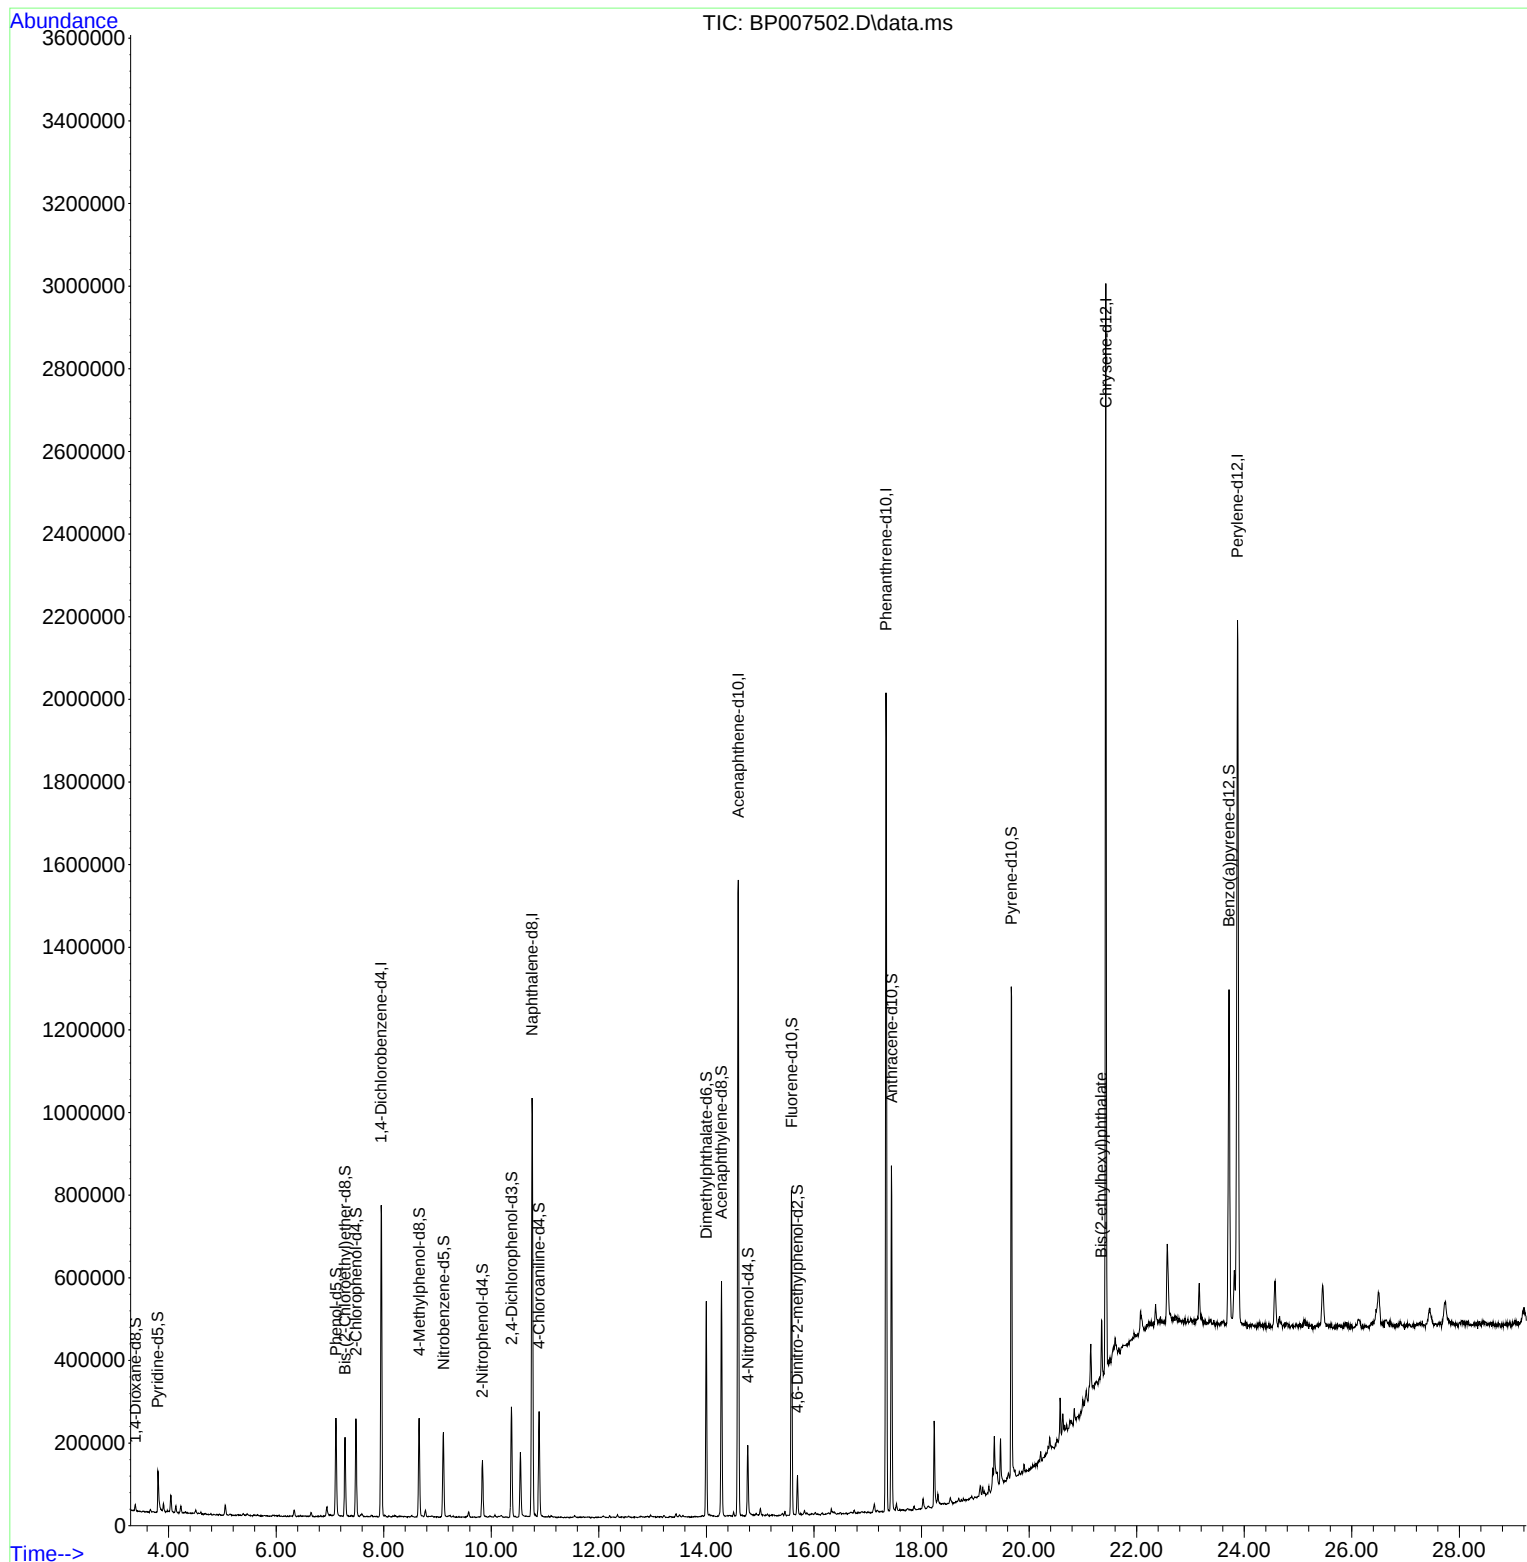

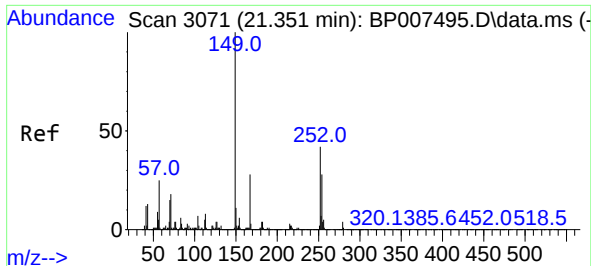

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.07 ng/ul
 RT: 21.345 min Scan# 3070
 Delta R.T. -0.012 min
 Lab File: BP007502.D
 Acq: 19 Oct 2021 21:02

Tgt Ion:149 Resp: 48309
 Ion Ratio Lower Upper
 149 100
 167 27.2 22.6 33.8
 279 3.8 3.3 4.9

Instrument :
 BNA_P
 ClientSampleId :
 JDGD2

Manual Integrations
 APPROVED

mohammad
 10/20/2021 1:56:51 PM

