

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007496.D
 Acq On : 19 Oct 2021 16:30
 Operator : CG/JU
 Sample : PB139906BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK906

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	11	16	24	rVB	50319	69690	1.54%	0.150%
2	3.793	83	86	102	rBV	647116	944091	20.89%	2.037%
3	4.134	140	144	147	rVB	12237	14174	0.31%	0.031%
4	6.993	626	630	636	rBV9	2215	4587	0.10%	0.010%
5	7.116	644	651	661	rBV	747121	1181376	26.14%	2.549%
6	7.281	673	679	691	rVB	581629	911911	20.18%	1.968%
7	7.487	707	714	722	rVB	757257	1186239	26.25%	2.560%
8	7.958	783	794	803	rBV	665638	1048373	23.20%	2.262%
9	8.658	903	913	924	rBV	905179	1484942	32.86%	3.205%
10	9.110	983	990	999	rBV	670647	1099291	24.33%	2.372%
11	9.840	1106	1114	1122	rBV	507950	859709	19.02%	1.855%
12	10.381	1197	1206	1214	rBV	872859	1476951	32.68%	3.187%
13	10.763	1261	1271	1281	rVB	871196	1493157	33.04%	3.222%
14	10.893	1285	1293	1303	rBV	825803	1412850	31.26%	3.049%
15	11.557	1398	1406	1412	rBV	3055	8924	0.20%	0.019%
16	12.346	1533	1540	1548	rBV	17836	33434	0.74%	0.072%
17	13.569	1741	1748	1752	rVB8	4344	6750	0.15%	0.015%
18	13.934	1803	1810	1814	rBV10	8333	18174	0.40%	0.039%
19	13.998	1815	1821	1828	rBV	1533168	2149621	47.57%	4.639%
20	14.281	1862	1869	1878	rBV	1710947	2589303	57.30%	5.588%
21	14.593	1915	1922	1931	rBV	1349838	2016415	44.62%	4.351%
22	14.775	1945	1953	1964	rBV	760388	1099648	24.33%	2.373%
23	14.998	1988	1991	1996	rBV7	3710	4683	0.10%	0.010%
24	15.257	2031	2035	2040	rVB8	3787	6182	0.14%	0.013%
25	15.587	2083	2091	2100	rBV	2201317	3212950	71.10%	6.934%
26	15.692	2103	2109	2120	rBV	402323	588247	13.02%	1.269%
27	15.828	2127	2132	2138	rVB	28894	45384	1.00%	0.098%
28	16.151	2184	2187	2191	rBV6	3391	4822	0.11%	0.010%
29	16.257	2200	2205	2211	rVB9	5593	11527	0.26%	0.025%
30	16.369	2221	2224	2228	rBV6	3912	7168	0.16%	0.015%
31	17.022	2333	2335	2344	rVB9	4684	7317	0.16%	0.016%
32	17.128	2347	2353	2359	rVV	9800	15989	0.35%	0.035%
33	17.345	2382	2390	2397	rBV	1777154	2447358	54.16%	5.281%
34	17.445	2400	2407	2422	rVB	2471384	3616486	80.03%	7.804%
35	17.575	2426	2429	2436	rVB4	23214	34612	0.77%	0.075%
36	18.239	2538	2542	2547	rBV7	12496	18628	0.41%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007496.D
 Acq On : 19 Oct 2021 16:30
 Operator : CG/JU
 Sample : PB139906BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK906

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	19.098	2685	2688	2692	rVB6	17764	20291	0.45%	0.044%
38	19.251	2711	2714	2719	rVB2	38707	48563	1.07%	0.105%
39	19.322	2722	2726	2729	rBV	48954	71232	1.58%	0.154%
40	19.357	2729	2732	2740	rVB5	32798	69431	1.54%	0.150%
41	19.598	2769	2773	2780	rBV5	51048	110118	2.44%	0.238%
42	19.675	2780	2786	2795	rVV	3258477	4439600	98.24%	9.581%
43	19.822	2807	2811	2815	rBV4	36078	53502	1.18%	0.115%
44	21.427	3079	3084	3093	rBV	2071595	2894085	64.04%	6.245%
45	23.727	3467	3475	3484	rVB	2230070	4519028	100.00%	9.752%
46	23.880	3495	3501	3510	rVB2	1393352	2982031	65.99%	6.435%




Sum of corrected areas: 46338844

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007496.D
Acq On : 19 Oct 2021 16:30
Operator : CG/JU
Sample : PB139906BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK906

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

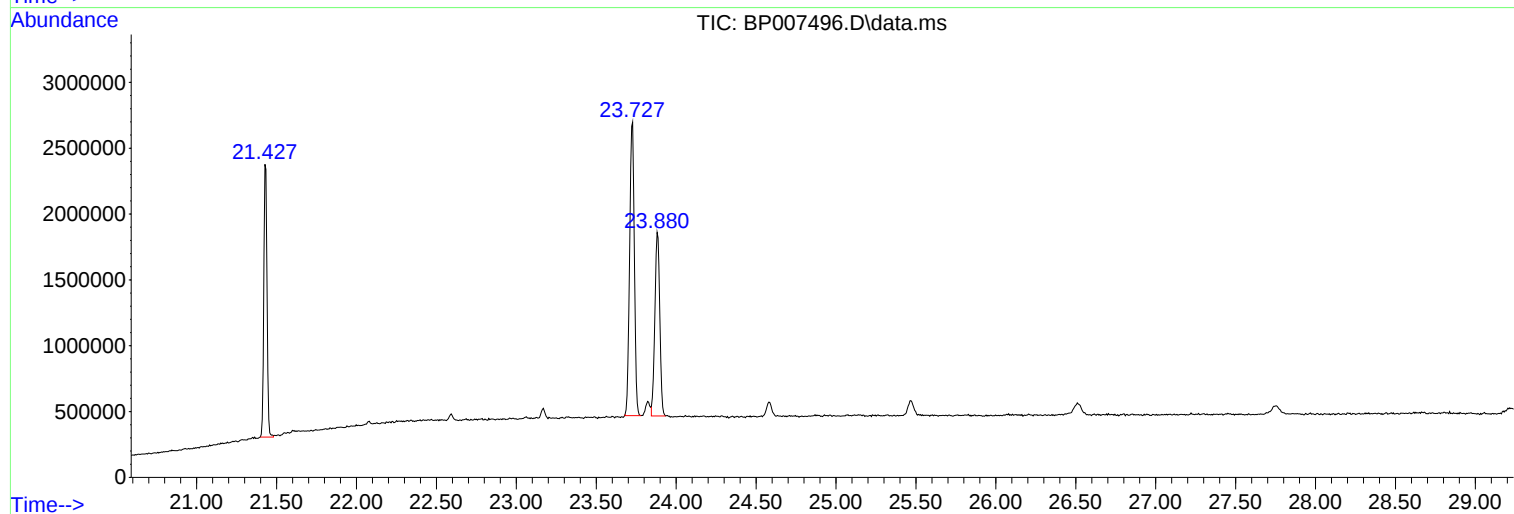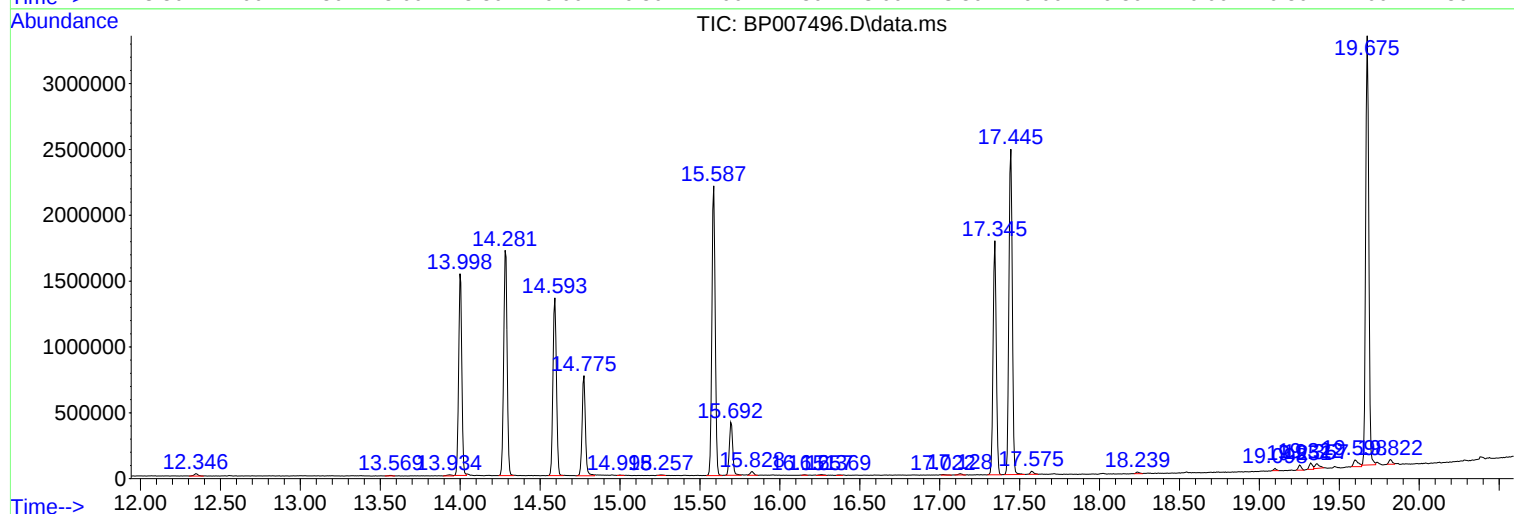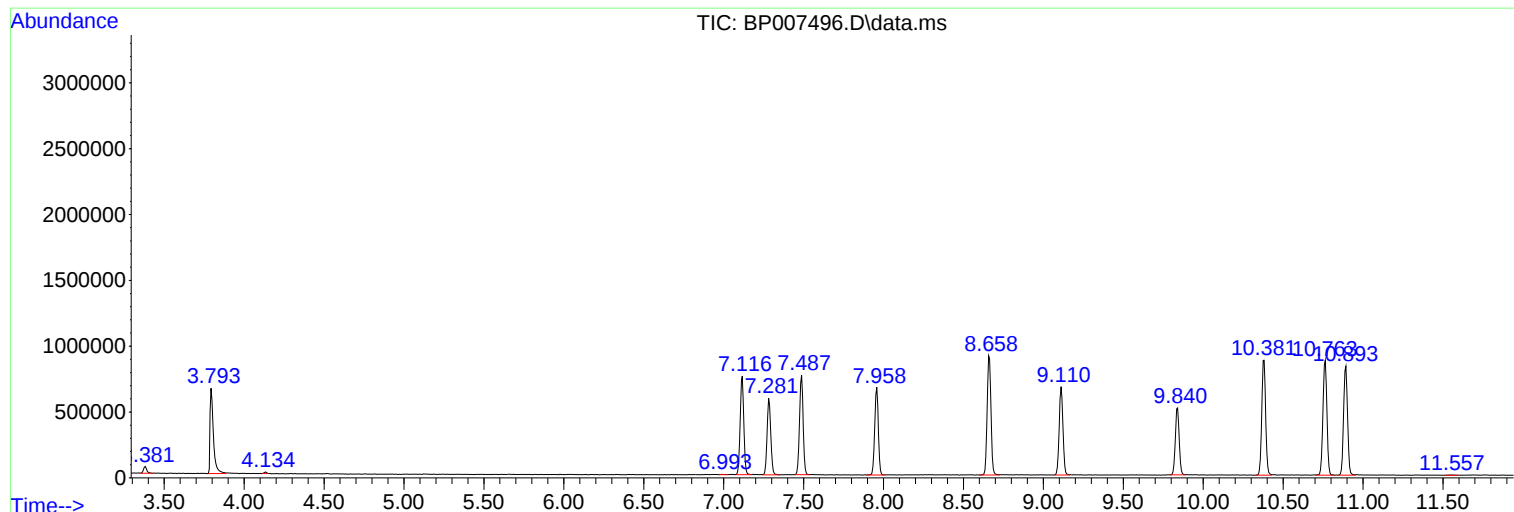

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007496.D
Acq On : 19 Oct 2021 16:30
Operator : CG/JU
Sample : PB139906BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK906

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007496.D
Acq On : 19 Oct 2021 16:30
Operator : CG/JU
Sample : PB139906BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK906

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
