

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007502.D
 Acq On : 19 Oct 2021 21:02
 Operator : CG/JU
 Sample : M4196-16
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	19	rVB	14736	17979	0.50%	0.064%
2	3.663	60	64	67	rBV4	7991	12796	0.36%	0.046%
3	3.799	84	87	97	rBV	100672	157867	4.41%	0.563%
4	3.905	101	105	111	rVB	21647	29859	0.83%	0.106%
5	4.040	124	128	133	rVB2	39709	56448	1.58%	0.201%
6	4.134	140	144	149	rVB	17323	22442	0.63%	0.080%
7	4.228	154	160	165	rBV3	18036	28967	0.81%	0.103%
8	4.505	202	207	213	rVB8	9715	15303	0.43%	0.055%
9	4.599	221	223	229	rVB2	5886	5985	0.17%	0.021%
10	4.940	279	281	286	rBV5	3128	4089	0.11%	0.015%
11	5.052	294	300	306	rBV	25388	40907	1.14%	0.146%
12	5.387	352	357	363	rBV4	5322	10087	0.28%	0.036%
13	5.463	367	370	374	rVB5	3317	4887	0.14%	0.017%
14	5.587	387	391	392	rBV4	4147	4621	0.13%	0.016%
15	5.787	419	425	429	rVB9	2282	5229	0.15%	0.019%
16	5.940	446	451	456	rBV8	3255	8003	0.22%	0.029%
17	6.334	513	518	523	rBV3	15368	24574	0.69%	0.088%
18	6.446	533	537	541	rBV7	3047	4709	0.13%	0.017%
19	6.646	568	571	577	rVB4	10129	15049	0.42%	0.054%
20	6.946	616	622	628	rBV2	22696	41612	1.16%	0.148%
21	7.110	643	650	662	rVB	237080	383719	10.72%	1.367%
22	7.281	673	679	687	rBV	191704	301486	8.42%	1.074%
23	7.399	696	699	704	rVB7	3158	4839	0.14%	0.017%
24	7.481	706	713	725	rVV	237300	379374	10.60%	1.352%
25	7.569	725	728	729	rVV3	4362	4513	0.13%	0.016%
26	7.593	729	732	739	rVB6	7226	11503	0.32%	0.041%
27	7.769	758	762	768	rVB4	4219	6742	0.19%	0.024%
28	7.951	785	793	802	rBV	754867	1210496	33.83%	4.314%
29	8.204	835	836	842	rVB6	3788	5320	0.15%	0.019%
30	8.522	887	890	895	rVB7	3420	4213	0.12%	0.015%
31	8.657	906	913	921	rBV	239178	378570	10.58%	1.349%
32	8.775	926	933	939	rVB	16169	26334	0.74%	0.094%
33	9.110	982	990	1000	rBV	205483	345062	9.64%	1.230%
34	9.210	1003	1007	1009	rVV5	3348	5965	0.17%	0.021%
35	9.581	1060	1070	1075	rBV2	13361	26576	0.74%	0.095%
36	9.834	1105	1113	1120	rBV	137236	233369	6.52%	0.832%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007502.D
 Acq On : 19 Oct 2021 21:02
 Operator : CG/JU
 Sample : M4196-16
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	9.975	1134	1137	1143	rVB8	3316	5472	0.15%	0.019%
38	10.069	1147	1153	1159	rBV10	6072	9761	0.27%	0.035%
39	10.187	1167	1173	1178	rVB9	4600	11095	0.31%	0.040%
40	10.375	1198	1205	1213	rBV	267269	446271	12.47%	1.590%
41	10.540	1224	1233	1243	rBV	157286	256824	7.18%	0.915%
42	10.757	1262	1270	1279	rBV	1012890	1712746	47.86%	6.103%
43	10.816	1279	1280	1285	rVB4	6186	5738	0.16%	0.020%
44	10.887	1285	1292	1302	rBV	254361	431088	12.05%	1.536%
45	11.063	1318	1322	1326	rVB7	3528	4408	0.12%	0.016%
46	11.110	1326	1330	1336	rBV9	4234	8707	0.24%	0.031%
47	11.545	1399	1404	1412	rVB9	4885	8949	0.25%	0.032%
48	12.081	1488	1495	1503	rVB9	3855	9081	0.25%	0.032%
49	12.198	1511	1515	1519	rBV5	5083	7236	0.20%	0.026%
50	12.345	1533	1540	1545	rBV4	7280	11876	0.33%	0.042%
51	12.904	1632	1635	1639	rVB6	2974	3993	0.11%	0.014%
52	12.963	1642	1645	1650	rVV6	4901	6383	0.18%	0.023%
53	13.151	1674	1677	1682	rVB7	2771	5068	0.14%	0.018%
54	13.210	1682	1687	1692	rVB8	5072	9931	0.28%	0.035%
55	13.439	1720	1726	1730	rBV7	8461	14906	0.42%	0.053%
56	13.498	1732	1736	1743	rVB8	5306	9016	0.25%	0.032%
57	13.563	1743	1747	1752	rBV8	3479	5491	0.15%	0.020%
58	13.922	1804	1808	1812	rBV7	2760	4216	0.12%	0.015%
59	13.998	1812	1821	1829	rBV	520545	705361	19.71%	2.514%
60	14.281	1859	1869	1877	rBV	568862	829970	23.19%	2.958%
61	14.504	1904	1907	1911	rBV3	10694	13132	0.37%	0.047%
62	14.592	1913	1922	1929	rBV	1539180	2343889	65.50%	8.353%
63	14.769	1944	1952	1963	rBV	171496	274754	7.68%	0.979%
64	14.922	1975	1978	1981	rBV5	4449	5637	0.16%	0.020%
65	15.004	1985	1992	1997	rBV5	16606	27014	0.75%	0.096%
66	15.063	1999	2002	2006	rVB5	2546	4017	0.11%	0.014%
67	15.133	2009	2014	2019	rVB9	4925	8324	0.23%	0.030%
68	15.416	2058	2062	2065	rVB6	5792	8559	0.24%	0.031%
69	15.457	2065	2069	2074	rVB4	11277	16416	0.46%	0.058%
70	15.580	2083	2090	2098	rBV	786941	1127707	31.51%	4.019%
71	15.692	2103	2109	2117	rVV	95789	136270	3.81%	0.486%
72	15.822	2127	2131	2136	rBV6	8881	12405	0.35%	0.044%
73	15.863	2136	2138	2143	rVB5	3957	4934	0.14%	0.018%
74	16.022	2161	2165	2169	rBV7	4728	7047	0.20%	0.025%
75	16.151	2181	2187	2192	rBV8	5583	12158	0.34%	0.043%
76	16.322	2213	2216	2219	rBV3	12645	15298	0.43%	0.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007502.D
 Acq On : 19 Oct 2021 21:02
 Operator : CG/JU
 Sample : M4196-16
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

77	16.380	2225	2226	2233	rVB7	5519	6945	0.19%	0.025%
78	16.751	2286	2289	2294	rVB7	8439	11877	0.33%	0.042%
79	17.122	2346	2352	2358	rBV4	21101	38761	1.08%	0.138%
80	17.174	2358	2361	2366	rVB6	4748	7816	0.22%	0.028%
81	17.339	2383	2389	2396	rBV	1981598	2884014	80.59%	10.277%
82	17.439	2400	2406	2417	rVV2	836107	1205122	33.68%	4.295%
83	17.533	2419	2422	2428	rVB8	16845	23112	0.65%	0.082%
84	17.863	2474	2478	2480	rBV4	10081	12838	0.36%	0.046%
85	18.027	2501	2506	2513	rBV4	23946	39105	1.09%	0.139%
86	18.233	2537	2541	2548	rBV	207070	280035	7.83%	0.998%
87	18.304	2550	2553	2558	rVB	23323	31914	0.89%	0.114%
88	19.092	2682	2687	2692	rBV9	25890	47519	1.33%	0.169%
89	19.139	2692	2695	2698	rVV4	17604	19901	0.56%	0.071%
90	19.251	2711	2714	2719	rBV6	17879	23513	0.66%	0.084%
91	19.321	2723	2726	2728	rBV2	42945	52048	1.45%	0.185%
92	19.351	2728	2731	2738	rVV2	97344	146675	4.10%	0.523%
93	19.468	2747	2751	2761	rBV2	108429	152345	4.26%	0.543%
94	19.668	2780	2785	2791	rBV	1189496	1632491	45.62%	5.817%
95	20.574	2936	2939	2943	rBV	91011	96967	2.71%	0.346%
96	21.345	3068	3070	3076	rVB	133732	155922	4.36%	0.556%
97	21.427	3079	3084	3089	rVV	2623379	3386993	94.64%	12.070%
98	22.568	3275	3278	3286	rVB3	169853	303392	8.48%	1.081%
99	23.715	3467	3473	3484	rVB2	796205	1543295	43.12%	5.500%
100	23.874	3494	3500	3511	rVB2	1700539	3578669	100.00%	12.753%




Sum of corrected areas: 28061911

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007502.D
Acq On : 19 Oct 2021 21:02
Operator : CG/JU
Sample : M4196-16
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

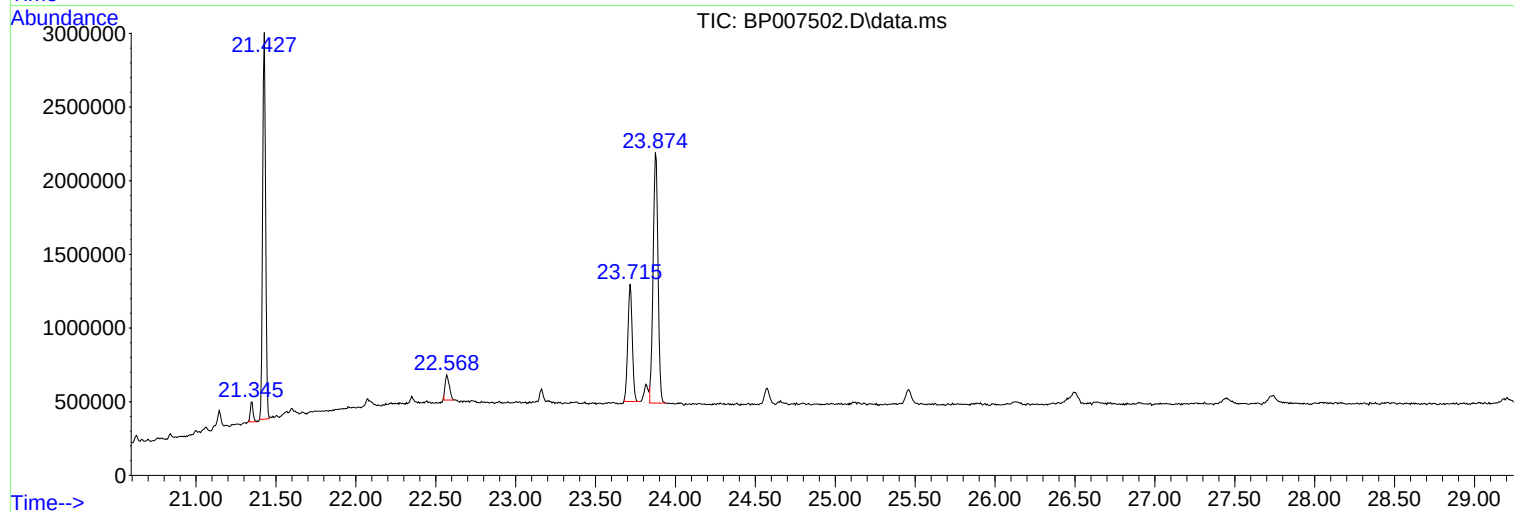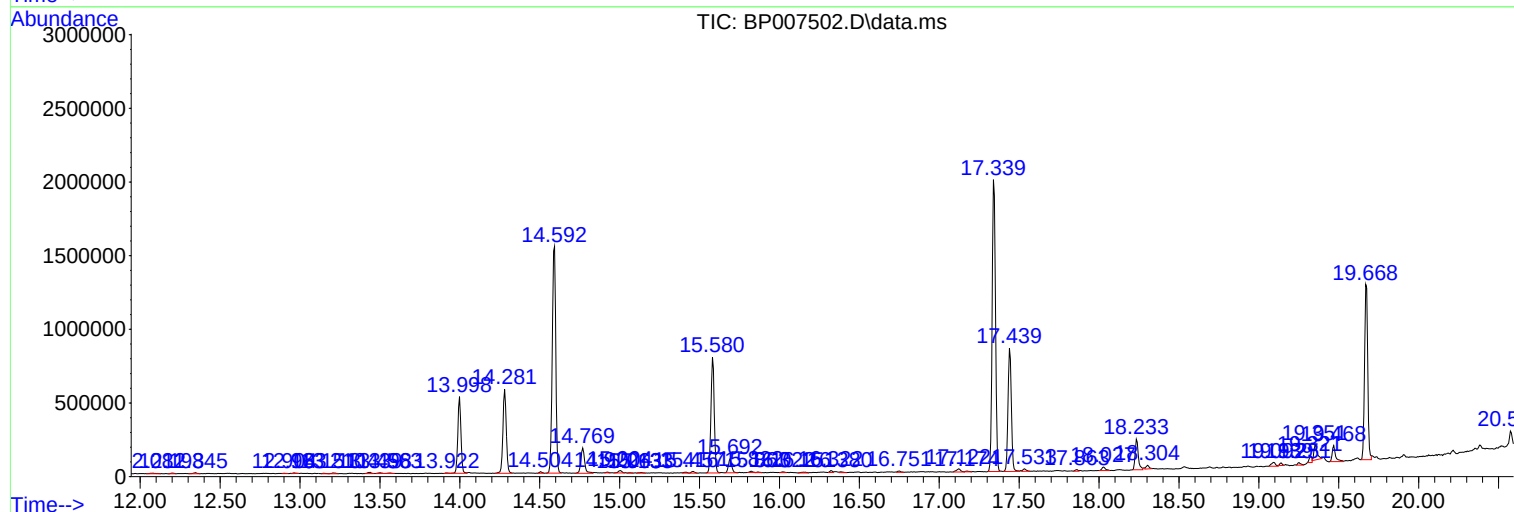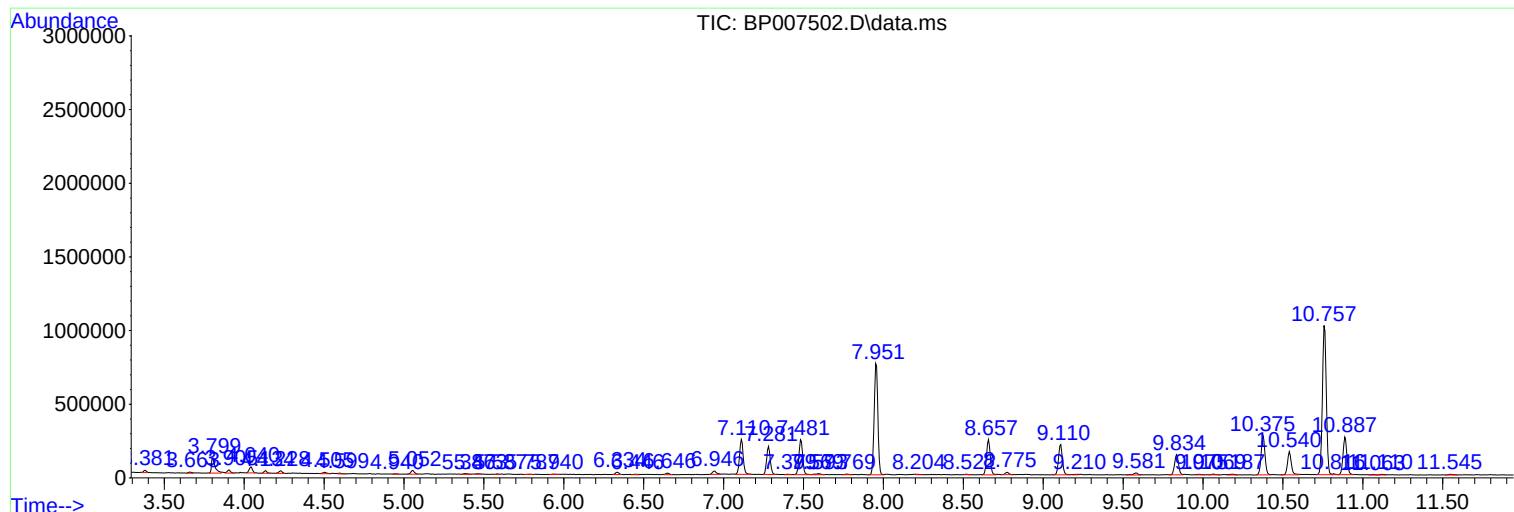

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007502.D
Acq On : 19 Oct 2021 21:02
Operator : CG/JU
Sample : M4196-16
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.540	3.00 ng/ul	256824	Naphthalene-d8	10.757

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	91
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	72

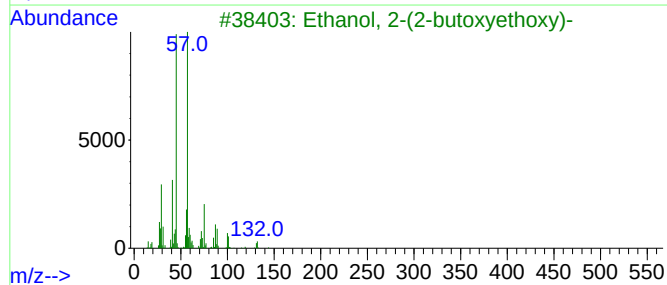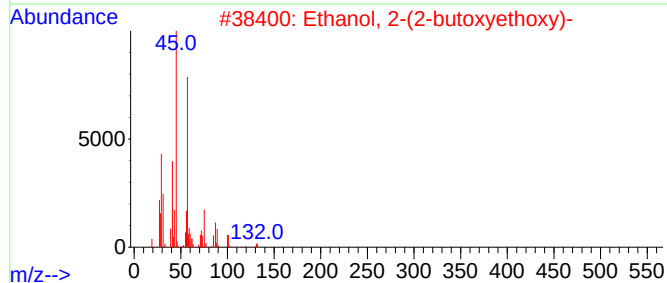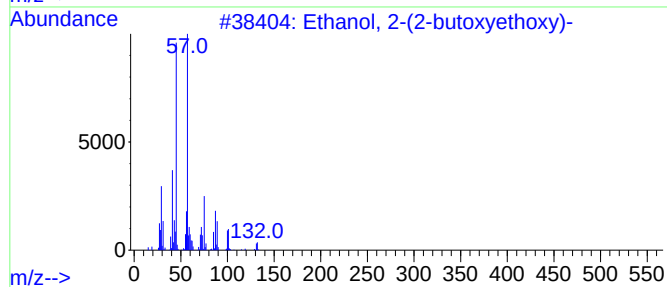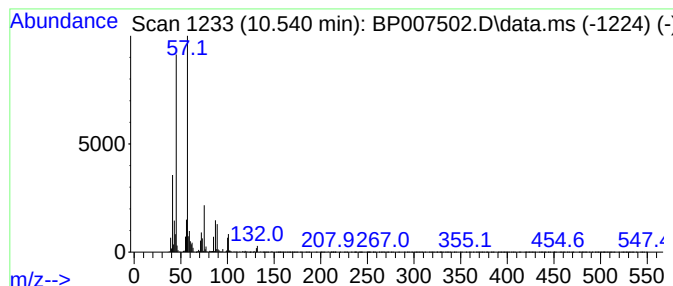

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007502.D
Acq On : 19 Oct 2021 21:02
Operator : CG/JU
Sample : M4196-16
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.540	3.0	ng/ul	256824	2	10.757	1712750	20.0