

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007510.D
 Acq On : 20 Oct 2021 04:23
 Operator : CG/JU
 Sample : PB140007BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	11	15	22	rVB	58336	79548	1.35%	0.132%
2	3.793	82	86	108	rBV	825755	1256947	21.40%	2.080%
3	4.134	140	144	148	rVB	15321	21096	0.36%	0.035%
4	7.111	643	650	660	rBV	986715	1501128	25.56%	2.484%
5	7.281	672	679	690	rVB	745147	1183422	20.15%	1.958%
6	7.481	706	713	722	rBV	966135	1520919	25.90%	2.516%
7	7.952	785	793	802	rVB	873356	1381604	23.53%	2.286%
8	8.658	905	913	924	rBV	1191986	1898723	32.33%	3.142%
9	9.111	982	990	1003	rBV	861981	1442336	24.56%	2.386%
10	9.834	1106	1113	1128	rBV	675561	1122050	19.11%	1.857%
11	10.375	1196	1205	1214	rBV	1149209	1903822	32.42%	3.150%
12	10.758	1262	1270	1278	rBV	1169073	1973424	33.61%	3.265%
13	10.887	1284	1292	1304	rBV	1097992	1834434	31.24%	3.035%
14	12.346	1534	1540	1546	rVB3	24740	43808	0.75%	0.072%
15	12.552	1570	1575	1579	rVB7	3353	6041	0.10%	0.010%
16	13.322	1702	1706	1710	rBV7	4221	6976	0.12%	0.012%
17	13.551	1743	1745	1752	rVB6	4757	7718	0.13%	0.013%
18	13.999	1814	1821	1835	rVB	2041346	2817110	47.97%	4.661%
19	14.281	1858	1869	1880	rBV	2277577	3362973	57.27%	5.564%
20	14.587	1913	1921	1931	rBV	1806585	2704591	46.06%	4.475%
21	14.769	1944	1952	1971	rBV	1008116	1444822	24.60%	2.391%
22	14.998	1988	1991	1998	rVB9	4288	8697	0.15%	0.014%
23	15.240	2028	2032	2036	rVB7	3668	5945	0.10%	0.010%
24	15.581	2083	2090	2102	rBV	2839606	4178510	71.16%	6.914%
25	15.693	2102	2109	2124	rVV	659928	921116	15.69%	1.524%
26	15.822	2124	2131	2136	rVB2	38218	60072	1.02%	0.099%
27	15.957	2148	2154	2156	rBV6	4150	6631	0.11%	0.011%
28	16.263	2200	2206	2210	rBV9	5524	10320	0.18%	0.017%
29	16.375	2220	2225	2229	rVB7	4419	8287	0.14%	0.014%
30	17.122	2348	2352	2357	rBV2	10238	12964	0.22%	0.021%
31	17.340	2381	2389	2396	rBV	2307822	3331048	56.72%	5.511%
32	17.440	2399	2406	2419	rBV	3371400	4714968	80.29%	7.801%
33	17.575	2424	2429	2434	rVV6	13627	21194	0.36%	0.035%
34	17.710	2448	2452	2456	rBV6	6786	8515	0.15%	0.014%
35	18.010	2501	2503	2506	rBV3	8347	7963	0.14%	0.013%
36	18.234	2538	2541	2544	rBV4	9692	10501	0.18%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007510.D
Acq On : 20 Oct 2021 04:23
Operator : CG/JU
Sample : PB140007BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	19.251	2710	2714	2720	rBV2	46699	61967	1.06%	0.103%
38	19.316	2721	2725	2729	rBV	49438	66097	1.13%	0.109%
39	19.669	2779	2785	2795	rBV	4106459	5715439	97.33%	9.457%
40	21.428	3078	3084	3090	rBV	2866161	3866696	65.85%	6.398%
41	23.716	3466	3473	3483	rVB2	2811594	5872320	100.00%	9.716%
42	23.874	3493	3500	3510	rVB2	1909380	4035499	68.72%	6.677%




Sum of corrected areas: 60438241

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007510.D
Acq On : 20 Oct 2021 04:23
Operator : CG/JU
Sample : PB140007BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

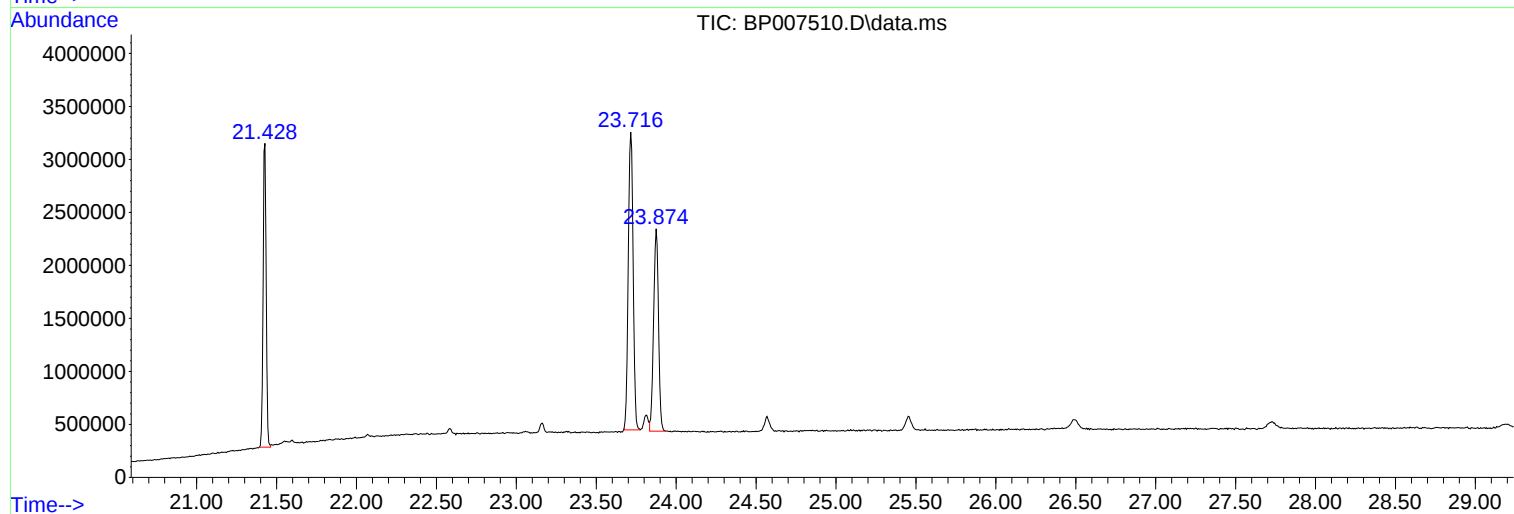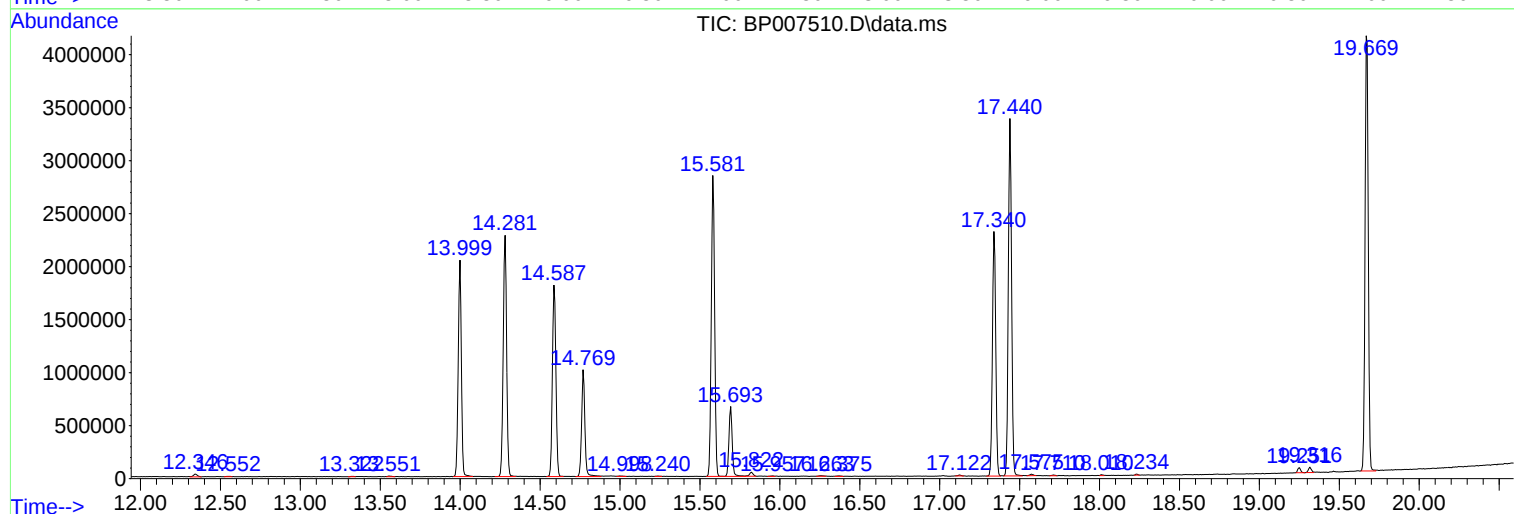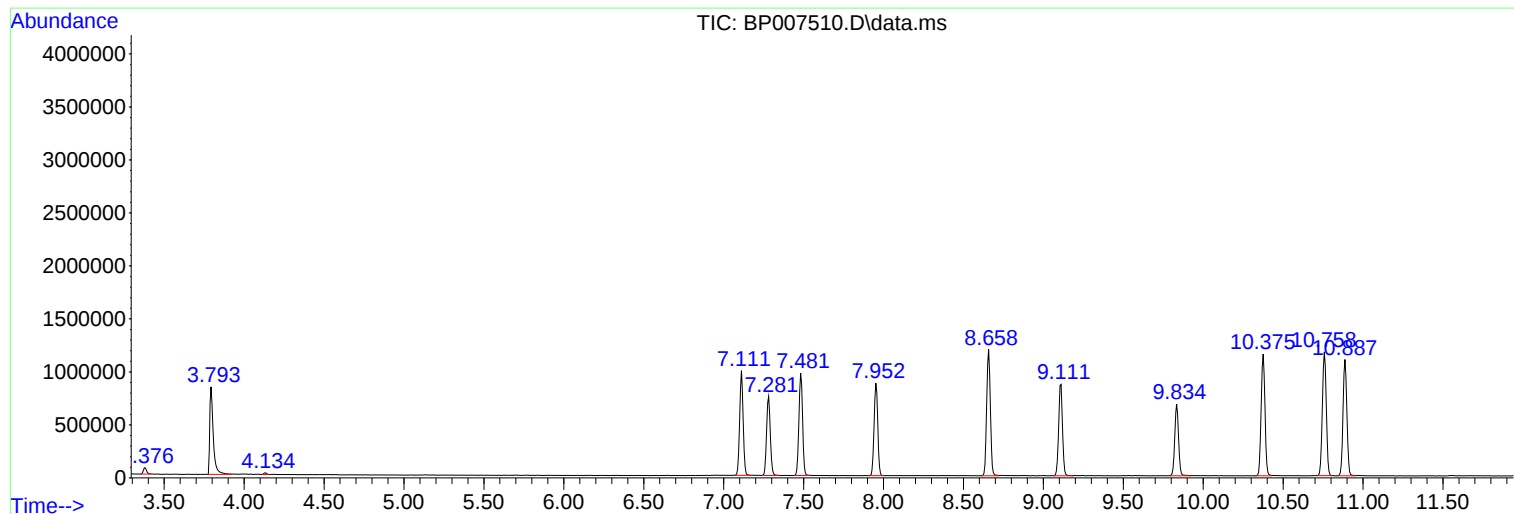

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007510.D
Acq On : 20 Oct 2021 04:23
Operator : CG/JU
Sample : PB140007BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007510.D
Acq On : 20 Oct 2021 04:23
Operator : CG/JU
Sample : PB140007BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------