

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007513.D
 Acq On : 20 Oct 2021 06:05
 Operator : CG/JU
 Sample : M4207-02
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	20	rVB	23789	30480	0.82%	0.084%
2	3.664	60	64	68	rBV4	6901	9933	0.27%	0.027%
3	3.816	87	90	95	rBV2	15045	22866	0.61%	0.063%
4	3.899	102	104	111	rVB3	8440	12936	0.35%	0.036%
5	4.040	123	128	138	rVB2	63125	104369	2.79%	0.289%
6	4.128	139	143	152	rVB	20813	35261	0.94%	0.098%
7	4.228	155	160	164	rBV	24487	38500	1.03%	0.107%
8	4.311	170	174	179	rBV6	4501	7172	0.19%	0.020%
9	4.505	203	207	212	rBV6	9587	13155	0.35%	0.036%
10	4.593	220	222	227	rVB4	8482	11146	0.30%	0.031%
11	5.052	295	300	307	rBV2	51122	75054	2.01%	0.208%
12	5.146	311	316	321	rBV9	3061	6481	0.17%	0.018%
13	5.587	388	391	398	rVB4	6703	11937	0.32%	0.033%
14	5.969	451	456	460	rBV6	7379	13516	0.36%	0.037%
15	6.334	512	518	523	rBV2	25173	39892	1.07%	0.110%
16	6.452	532	538	539	rBV6	3726	5387	0.14%	0.015%
17	6.934	615	620	623	rBV7	8146	15138	0.40%	0.042%
18	6.963	623	625	630	rVB6	5162	7205	0.19%	0.020%
19	7.110	643	650	661	rVB	401086	632015	16.90%	1.750%
20	7.281	673	679	687	rVV	306677	491751	13.15%	1.361%
21	7.387	694	697	703	rBV8	2657	5130	0.14%	0.014%
22	7.481	706	713	724	rBV	401542	632589	16.92%	1.751%
23	7.593	728	732	742	rVB6	12022	24673	0.66%	0.068%
24	7.769	757	762	766	rBV3	8701	14257	0.38%	0.039%
25	7.952	786	793	800	rBV	826084	1274981	34.10%	3.530%
26	8.199	829	835	843	rBV7	9566	19829	0.53%	0.055%
27	8.516	883	889	895	rVB3	9001	16488	0.44%	0.046%
28	8.657	906	913	922	rBV	468771	747848	20.00%	2.070%
29	8.775	926	933	938	rBV	15821	26774	0.72%	0.074%
30	9.104	979	989	996	rBV	353870	587753	15.72%	1.627%
31	9.287	1015	1020	1027	rVB9	5233	8730	0.23%	0.024%
32	9.575	1066	1069	1075	rVB7	6876	13097	0.35%	0.036%
33	9.834	1107	1113	1121	rBV	254762	422541	11.30%	1.170%
34	10.375	1197	1205	1214	rBV	474205	781455	20.90%	2.163%
35	10.540	1225	1233	1247	rBV	273663	443058	11.85%	1.227%
36	10.757	1262	1270	1277	rBV	1095448	1825654	48.83%	5.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007513.D
 Acq On : 20 Oct 2021 06:05
 Operator : CG/JU
 Sample : M4207-02
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	10.887	1285	1292	1299	rBV	355720	589743	15.77%	1.633%
38	11.287	1357	1360	1365	rVB6	4050	6254	0.17%	0.017%
39	11.545	1398	1404	1409	rBV10	6601	11844	0.32%	0.033%
40	11.645	1417	1421	1423	rBV4	5628	7629	0.20%	0.021%
41	12.075	1492	1494	1500	rVB7	4620	7217	0.19%	0.020%
42	12.340	1534	1539	1544	rVV3	11772	20419	0.55%	0.057%
43	12.416	1546	1552	1560	rVB	19620	34158	0.91%	0.095%
44	12.634	1585	1589	1594	rVV	12885	21029	0.56%	0.058%
45	12.957	1639	1644	1647	rBV7	6397	9837	0.26%	0.027%
46	13.204	1682	1686	1692	rVB8	7618	13163	0.35%	0.036%
47	13.498	1731	1736	1744	rVB2	32527	49037	1.31%	0.136%
48	13.757	1774	1780	1781	rVV6	5650	7863	0.21%	0.022%
49	13.792	1781	1786	1791	rVB6	14218	22934	0.61%	0.063%
50	13.916	1802	1807	1811	rVB6	14850	23885	0.64%	0.066%
51	13.998	1811	1821	1827	rBV	832671	1197887	32.04%	3.316%
52	14.151	1841	1847	1856	rVB	6384	16058	0.43%	0.044%
53	14.281	1859	1869	1880	rBV	963077	1459653	39.04%	4.041%
54	14.504	1902	1907	1911	rVB8	4019	6071	0.16%	0.017%
55	14.586	1913	1921	1928	rBV	1706935	2507703	67.07%	6.942%
56	14.639	1928	1930	1934	rVB5	3651	5091	0.14%	0.014%
57	14.769	1944	1952	1964	rBV	316456	487456	13.04%	1.349%
58	14.922	1974	1978	1981	rBV6	4379	8175	0.22%	0.023%
59	14.998	1984	1991	1997	rBV4	40704	69793	1.87%	0.193%
60	15.251	2033	2034	2041	rVB6	3784	5131	0.14%	0.014%
61	15.404	2058	2060	2065	rVB5	7558	10930	0.29%	0.030%
62	15.581	2082	2090	2097	rBV	1310418	1871009	50.04%	5.179%
63	15.686	2103	2108	2116	rBV	191890	290579	7.77%	0.804%
64	15.822	2126	2131	2137	rVB3	15934	20834	0.56%	0.058%
65	15.933	2146	2150	2154	rBV4	4697	6571	0.18%	0.018%
66	16.028	2161	2166	2171	rBV9	10838	19178	0.51%	0.053%
67	16.075	2171	2174	2176	rBV3	6266	8053	0.22%	0.022%
68	16.145	2182	2186	2187	rBV4	5120	7653	0.20%	0.021%
69	16.275	2202	2208	2209	rBV6	4059	6577	0.18%	0.018%
70	16.316	2212	2215	2217	rBV4	6284	7562	0.20%	0.021%
71	16.345	2218	2220	2223	rVB4	6683	7315	0.20%	0.020%
72	16.463	2235	2240	2242	rBV6	3887	6493	0.17%	0.018%
73	16.486	2242	2244	2251	rVB7	6936	10616	0.28%	0.029%
74	16.692	2275	2279	2284	rVV8	2994	6237	0.17%	0.017%
75	16.745	2285	2288	2292	rVB6	7187	8506	0.23%	0.024%
76	16.880	2308	2311	2315	rVB6	5619	7265	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007513.D
 Acq On : 20 Oct 2021 06:05
 Operator : CG/JU
 Sample : M4207-02
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

77	17.122	2349	2352	2356	rVV3	13940	19436	0.52%	0.054%
78	17.239	2369	2372	2376	rBV6	5790	7764	0.21%	0.021%
79	17.339	2382	2389	2394	rBV	2149891	3067201	82.03%	8.491%
80	17.380	2394	2396	2400	rVV	42633	51477	1.38%	0.143%
81	17.439	2400	2406	2417	rVV	1408272	2038500	54.52%	5.643%
82	17.533	2417	2422	2427	rVB6	26682	41031	1.10%	0.114%
83	17.739	2455	2457	2462	rVB5	9201	8273	0.22%	0.023%
84	17.857	2474	2477	2480	rBV5	7413	8633	0.23%	0.024%
85	18.022	2500	2505	2510	rBV	83486	106373	2.84%	0.294%
86	18.104	2517	2519	2525	rBV7	4925	6621	0.18%	0.018%
87	18.233	2534	2541	2549	rBV3	144083	224994	6.02%	0.623%
88	18.386	2564	2567	2571	rBV5	9462	14351	0.38%	0.040%
89	18.527	2588	2591	2595	rBV6	14657	20437	0.55%	0.057%
90	19.151	2693	2697	2701	rVB3	92731	110514	2.96%	0.306%
91	19.251	2711	2714	2717	rVB4	16973	17551	0.47%	0.049%
92	19.280	2717	2719	2722	rBV	25862	30327	0.81%	0.084%
93	19.316	2723	2725	2727	rVV2	25394	30016	0.80%	0.083%
94	19.345	2727	2730	2737	rVB	77825	106762	2.86%	0.296%
95	19.463	2747	2750	2758	rBV4	75808	107105	2.86%	0.296%
96	19.669	2779	2785	2794	rBV	1940597	2668306	71.36%	7.387%
97	21.145	3032	3036	3042	rBV2	180697	274899	7.35%	0.761%
98	21.421	3078	3083	3089	rBV	2671353	3727427	99.69%	10.319%
99	23.715	3466	3473	3481	rBV2	1222731	2383837	63.75%	6.599%
100	23.874	3493	3500	3509	rVB2	1850070	3739088	100.00%	10.351%


Sum of corrected areas: 36123382

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007513.D
Acq On : 20 Oct 2021 06:05
Operator : CG/JU
Sample : M4207-02
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B48

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

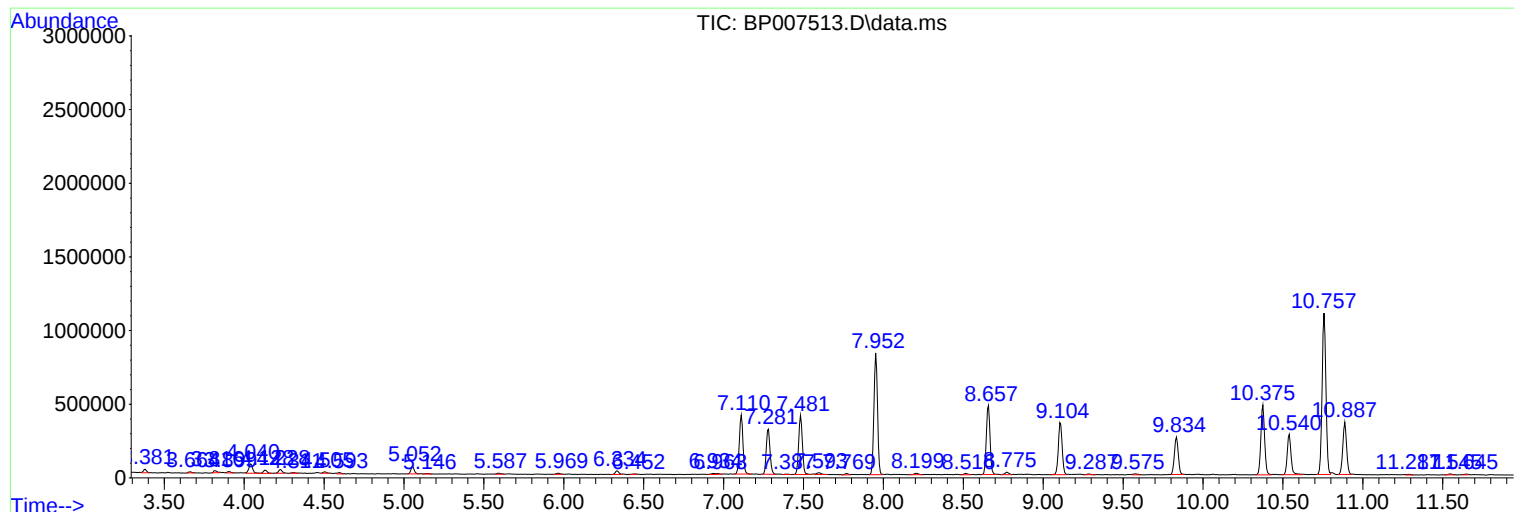

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007513.D
Acq On : 20 Oct 2021 06:05
Operator : CG/JU
Sample : M4207-02
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B48










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.540	4.85 ng/ul	443058	Naphthalene-d8	10.757

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-[2-(2-methylpropoxy)e...	162	C8H18O3	018912-80-6	72

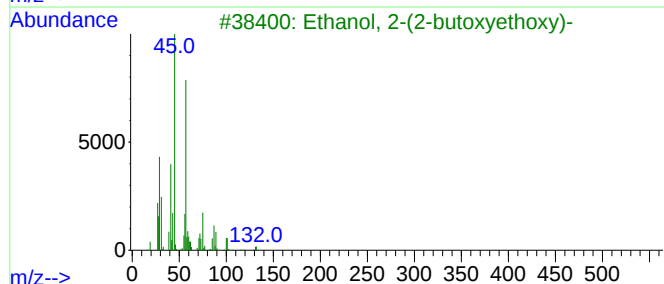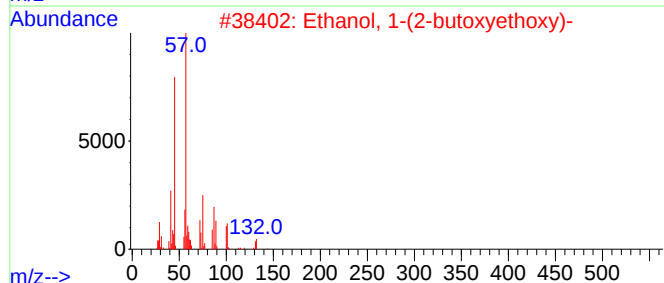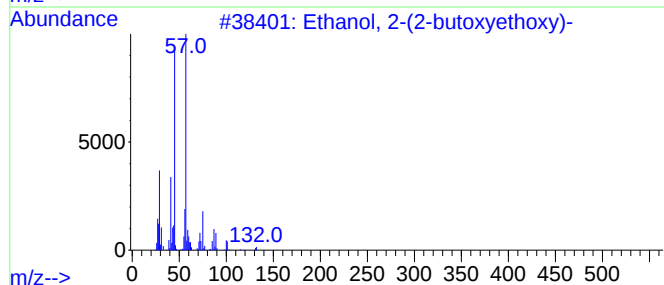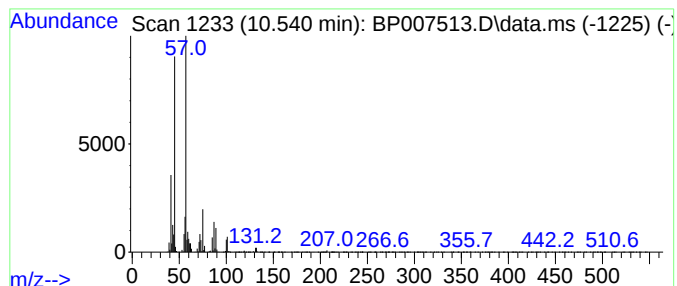

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007513.D
Acq On : 20 Oct 2021 06:05
Operator : CG/JU
Sample : M4207-02
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B48

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.540	4.8	ng/ul	443058	2	10.757	1825650	20.0