

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007519.D
 Acq On : 20 Oct 2021 09:28
 Operator : CG/JU
 Sample : PB139972BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK972

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	23	rVB	56886	78054	1.44%	0.144%
2	3.793	83	86	106	rBV	784744	1194288	22.01%	2.198%
3	4.134	139	144	148	rBV	11159	16206	0.30%	0.030%
4	7.111	643	650	659	rBV	929180	1441724	26.57%	2.653%
5	7.281	672	679	687	rVB	718868	1129698	20.82%	2.079%
6	7.481	706	713	721	rBV	913108	1451921	26.75%	2.672%
7	7.952	786	793	802	rBV	684683	1074814	19.81%	1.978%
8	8.658	905	913	925	rBV	1159960	1840148	33.91%	3.387%
9	9.111	981	990	1000	rBV	846369	1388413	25.58%	2.555%
10	9.834	1105	1113	1120	rBV	664657	1077708	19.86%	1.983%
11	10.375	1197	1205	1219	rBV	1121398	1857239	34.22%	3.418%
12	10.758	1262	1270	1279	rVB	903960	1538255	28.35%	2.831%
13	10.887	1283	1292	1303	rBV	1058714	1830748	33.74%	3.369%
14	12.346	1535	1540	1545	rBV2	22605	36259	0.67%	0.067%
15	13.004	1645	1652	1653	rBV7	3130	5447	0.10%	0.010%
16	13.563	1742	1747	1750	rVB6	4499	6334	0.12%	0.012%
17	13.999	1812	1821	1830	rBV	1946237	2651160	48.85%	4.879%
18	14.281	1862	1869	1881	rBV	2160551	3241730	59.74%	5.966%
19	14.587	1915	1921	1934	rBV	1416775	2096682	38.64%	3.859%
20	14.769	1944	1952	1965	rBV	897770	1337347	24.64%	2.461%
21	15.581	2083	2090	2098	rBV	2770413	4021872	74.11%	7.402%
22	15.693	2103	2109	2119	rBV	633407	850243	15.67%	1.565%
23	15.822	2126	2131	2137	rVB2	34926	52221	0.96%	0.096%
24	16.151	2183	2187	2192	rBV8	3426	6013	0.11%	0.011%
25	16.257	2201	2205	2208	rBV6	5623	8386	0.15%	0.015%
26	16.369	2218	2224	2227	rBV8	4106	6888	0.13%	0.013%
27	17.016	2331	2334	2340	rVB7	5911	8103	0.15%	0.015%
28	17.122	2346	2352	2358	rVB4	8667	18046	0.33%	0.033%
29	17.340	2382	2389	2398	rBV	1785921	2566087	47.29%	4.723%
30	17.440	2399	2406	2419	rVV2	3070079	4460504	82.19%	8.209%
31	17.575	2425	2429	2435	rBV4	15737	24011	0.44%	0.044%
32	17.716	2450	2453	2457	rVB4	6546	8370	0.15%	0.015%
33	18.228	2536	2540	2544	rBV7	9004	14352	0.26%	0.026%
34	18.534	2588	2592	2593	rBV4	4155	5881	0.11%	0.011%
35	19.251	2710	2714	2720	rBV2	43415	58527	1.08%	0.108%
36	19.316	2721	2725	2730	rVV2	46489	60103	1.11%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007519.D
Acq On : 20 Oct 2021 09:28
Operator : CG/JU
Sample : PB139972BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK972

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	19.669	2779	2785	2794	rBV	3905988	5346513	98.52%	9.840%
38	21.422	3078	3083	3089	rBV	2177204	2987953	55.06%	5.499%
39	23.716	3466	3473	3485	rBV2	2667988	5426835	100.00%	9.988%
40	23.874	3494	3500	3511	rVB2	1502079	3110045	57.31%	5.724%




Sum of corrected areas: 54335128

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007519.D
Acq On : 20 Oct 2021 09:28
Operator : CG/JU
Sample : PB139972BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

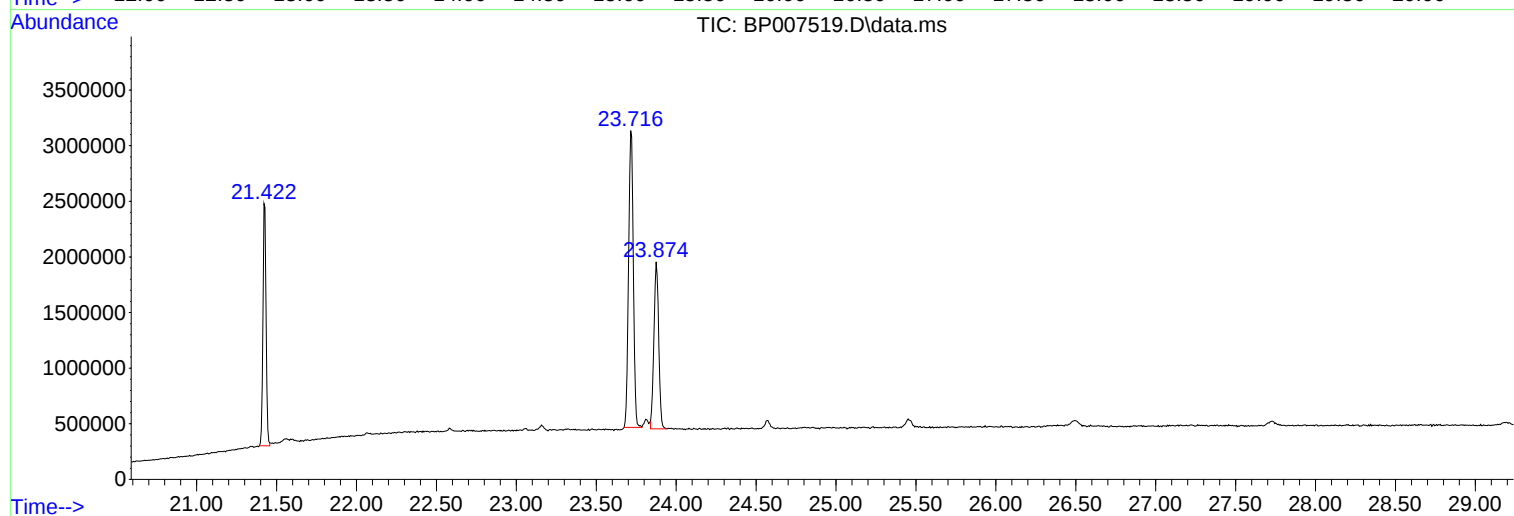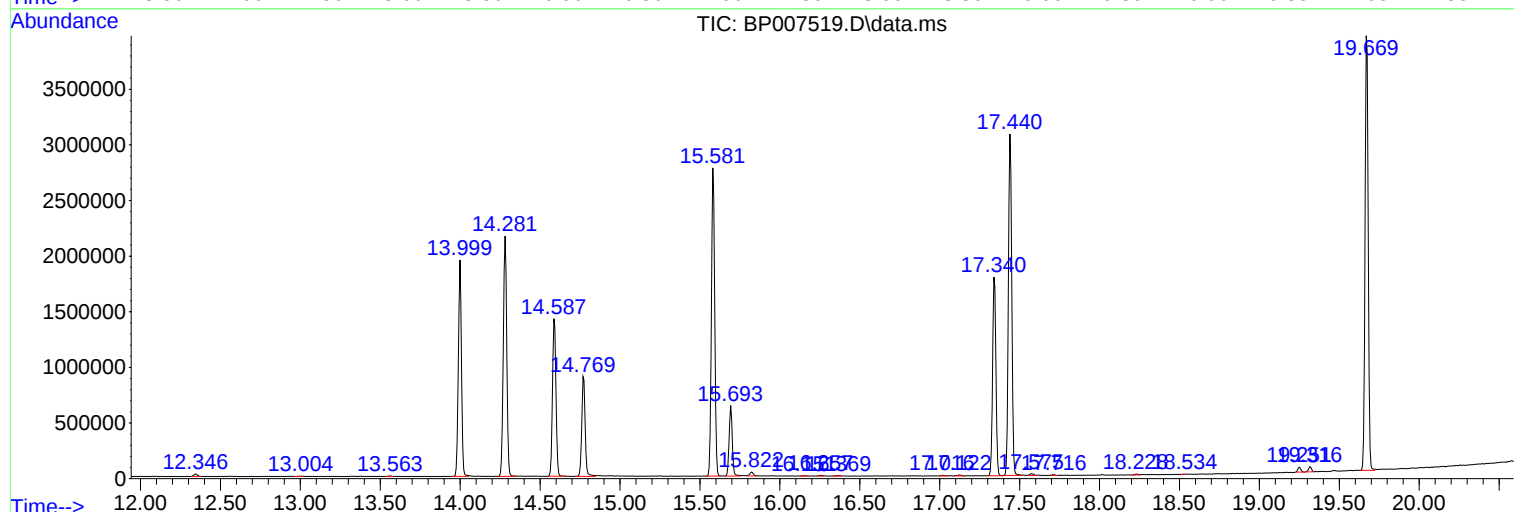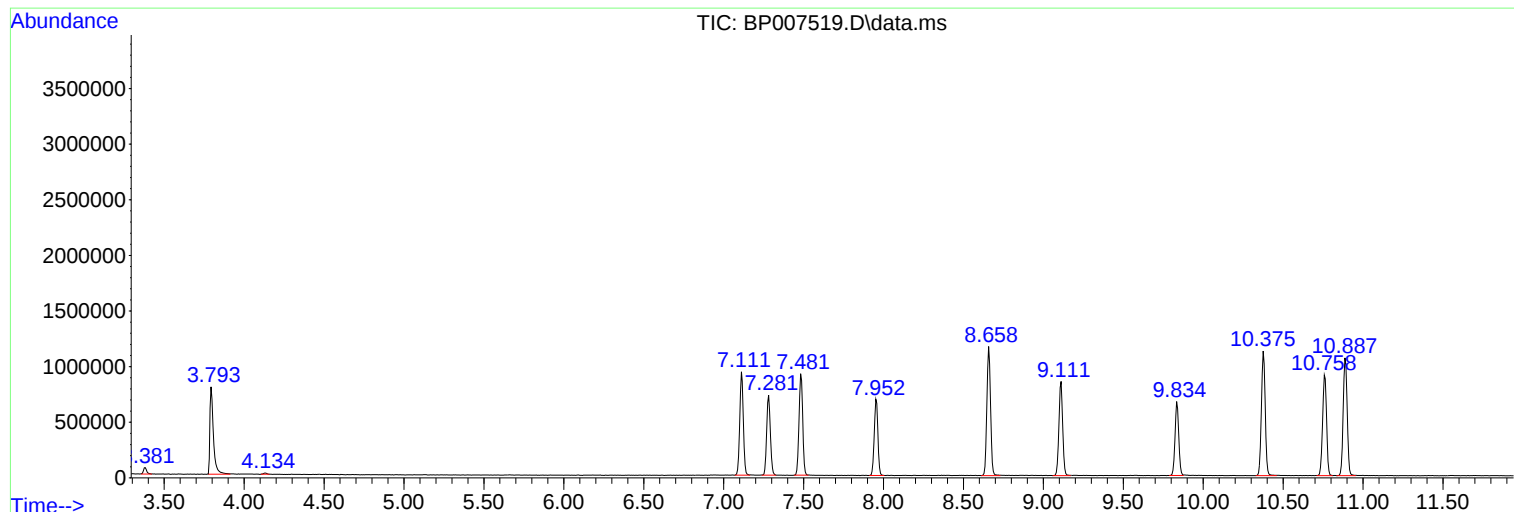

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007519.D
Acq On : 20 Oct 2021 09:28
Operator : CG/JU
Sample : PB139972BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007519.D
Acq On : 20 Oct 2021 09:28
Operator : CG/JU
Sample : PB139972BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc